

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080518\
 Data File : VU025876.D
 Acq On : 04 Aug 2018 16:34
 Operator : MD/SY
 Sample : J4340-23
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.626	5	11	16	rVB2	502	466	0.05%	0.005%
2	0.658	16	21	25	rBV3	418	447	0.05%	0.005%
3	0.709	35	37	38	rBV	173	86	0.01%	0.001%
4	0.809	65	68	72	rBV	171	185	0.02%	0.002%
5	0.841	77	78	80	rBV	158	52	0.01%	0.001%
6	0.854	80	82	84	rVB2	213	107	0.01%	0.001%
7	0.870	84	87	88	rBV	215	123	0.01%	0.001%
8	0.986	119	123	127	rVB2	446	360	0.04%	0.004%
9	1.008	127	130	132	rBV2	331	189	0.02%	0.002%
10	1.089	147	155	176	rBV	804334	901551	93.95%	10.464%
11	1.401	246	252	264	rVB	102325	103800	10.82%	1.205%
12	1.683	332	340	351	rBV	84720	103876	10.83%	1.206%
13	2.272	514	523	537	rVB	198457	302170	31.49%	3.507%
14	2.548	607	609	617	rVB2	508	541	0.06%	0.006%
15	2.587	617	621	624	rBV3	530	491	0.05%	0.006%
16	2.703	650	657	668	rVB3	5225	7915	0.82%	0.0092%
17	2.844	687	701	712	rBV2	3637	8401	0.88%	0.0098%
18	2.931	724	728	732	rBV2	220	221	0.02%	0.003%
19	2.957	732	736	737	rBV2	326	217	0.02%	0.003%
20	3.005	745	751	752	rBV	403	334	0.03%	0.004%
21	3.044	760	763	770	rVB3	465	431	0.04%	0.005%
22	3.089	774	777	780	rBV2	264	170	0.02%	0.002%
23	3.240	822	824	825	rBV2	220	92	0.01%	0.001%
24	3.285	833	838	839	rBV2	341	294	0.03%	0.003%
25	3.343	850	856	860	rBV3	445	519	0.05%	0.006%
26	3.378	863	867	869	rBV2	755	527	0.05%	0.006%
27	3.455	888	891	893	rBV	225	184	0.02%	0.002%
28	3.542	916	918	919	rBV	209	108	0.01%	0.001%
29	3.584	929	931	935	rBV	225	160	0.02%	0.002%
30	3.831	1006	1008	1010	rBV	211	132	0.01%	0.002%
31	3.880	1018	1023	1027	rVB	339	279	0.03%	0.003%
32	3.902	1027	1030	1036	rVB	297	249	0.03%	0.003%
33	3.934	1037	1040	1046	rBV2	254	219	0.02%	0.003%
34	3.957	1046	1047	1050	rVB2	186	89	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080518\
 Data File : VU025876.D
 Acq On : 04 Aug 2018 16:34
 Operator : MD/SY
 Sample : J4340-23
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

35	3.976	1050	1053	1055	rBV2	332	211	0.02%	0.002%
36	3.989	1055	1057	1060	rVV3	298	238	0.02%	0.003%
37	4.018	1064	1066	1068	rBV	195	82	0.01%	0.001%
38	4.043	1068	1074	1075	rBV2	323	299	0.03%	0.003%
39	4.079	1083	1085	1087	rVB2	233	110	0.01%	0.001%
40	4.095	1087	1090	1092	rVB	285	175	0.02%	0.002%
41	4.108	1092	1094	1095	rBV	225	105	0.01%	0.001%
42	4.182	1101	1117	1143	rBV	85461	234832	24.47%	2.726%
43	4.436	1194	1196	1199	rVB2	284	128	0.01%	0.001%
44	4.452	1199	1201	1203	rBV	223	81	0.01%	0.001%
45	4.468	1203	1206	1208	rBV2	417	240	0.03%	0.003%
46	4.506	1213	1218	1225	rVB4	497	703	0.07%	0.008%
47	4.539	1225	1228	1229	rBV	340	186	0.02%	0.002%
48	4.651	1245	1263	1286	rBV2	166529	396489	41.32%	4.602%
49	4.857	1325	1327	1329	rBV2	325	188	0.02%	0.002%
50	4.944	1351	1354	1355	rBV	63	27	0.00%	0.000%
51	4.989	1363	1368	1373	rBV5	457	612	0.06%	0.007%
52	5.085	1391	1398	1400	rVB2	306	281	0.03%	0.003%
53	5.111	1400	1406	1407	rBV	363	257	0.03%	0.003%
54	5.137	1413	1414	1417	rBV	153	76	0.01%	0.001%
55	5.346	1454	1479	1505	rBV2	319069	959570	100.00%	11.137%
56	5.513	1527	1531	1534	rBV3	469	423	0.04%	0.005%
57	5.545	1539	1541	1543	rBV2	263	132	0.01%	0.002%
58	5.664	1576	1578	1579	rBV2	284	107	0.01%	0.001%
59	5.677	1579	1582	1589	rVB2	475	394	0.04%	0.005%
60	5.754	1603	1606	1609	rVB3	310	190	0.02%	0.002%
61	5.809	1619	1623	1628	rVB2	436	454	0.05%	0.005%
62	5.831	1628	1630	1633	rBV2	165	83	0.01%	0.001%
63	5.889	1633	1648	1669	rBV	347145	677922	70.65%	7.868%
64	6.072	1699	1705	1707	rBV2	412	400	0.04%	0.005%
65	6.178	1732	1738	1744	rVB5	1414	1919	0.20%	0.022%
66	6.259	1760	1763	1768	rVB	292	230	0.02%	0.003%
67	6.336	1771	1787	1807	rBV	216281	439698	45.82%	5.103%
68	6.449	1820	1822	1824	rBV2	352	218	0.02%	0.003%
69	6.519	1839	1844	1845	rBV	311	273	0.03%	0.003%
70	6.613	1871	1873	1876	rBV	296	235	0.02%	0.003%
71	6.703	1899	1901	1902	rBV	153	85	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080518\
 Data File : VU025876.D
 Acq On : 04 Aug 2018 16:34
 Operator : MD/SY
 Sample : J4340-23
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

72	6.715	1902	1905	1908	rVV2	238	209	0.02%	0.002%
73	6.767	1918	1921	1924	rBV	336	295	0.03%	0.003%
74	6.847	1944	1946	1949	rBV2	466	346	0.04%	0.004%
75	7.047	2002	2008	2010	rBV3	399	421	0.04%	0.005%
76	7.166	2043	2045	2048	rBV2	212	140	0.01%	0.002%
77	7.230	2053	2065	2083	rBV	121633	218413	22.76%	2.535%
78	7.429	2124	2127	2129	rBV2	313	214	0.02%	0.002%
79	7.494	2142	2147	2149	rBV2	262	280	0.03%	0.003%
80	7.567	2157	2170	2191	rBV	433985	755168	78.70%	8.765%
81	7.850	2248	2258	2279	rBV	88454	151073	15.74%	1.753%
82	8.104	2335	2337	2340	rBV	245	134	0.01%	0.002%
83	8.149	2347	2351	2354	rBV2	398	349	0.04%	0.004%
84	8.233	2370	2377	2382	rVB3	1545	1868	0.19%	0.022%
85	8.313	2389	2402	2430	rBV	275324	487578	50.81%	5.659%
86	8.497	2455	2459	2465	rBV3	563	526	0.05%	0.006%
87	8.725	2527	2530	2532	rBV	261	165	0.02%	0.002%
88	8.805	2550	2555	2558	rBV3	369	370	0.04%	0.004%
89	9.092	2631	2644	2669	rBV	491129	823794	85.85%	9.561%
90	9.288	2703	2705	2707	rBV2	264	108	0.01%	0.001%
91	9.728	2840	2842	2844	rBV2	268	142	0.01%	0.002%
92	10.188	2981	2985	2988	rBV	388	322	0.03%	0.004%
93	10.352	3030	3036	3039	rBV3	449	524	0.05%	0.006%
94	10.436	3049	3062	3079	rVB	310560	493881	51.47%	5.732%
95	10.606	3111	3115	3116	rBV	487	354	0.04%	0.004%
96	10.841	3185	3188	3191	rVB2	400	213	0.02%	0.002%
97	11.487	3377	3389	3413	rBV	497436	790643	82.40%	9.177%
98	11.863	3493	3506	3522	rBV	458897	735743	76.67%	8.539%


Sum of corrected areas: 8615911

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080518\
Data File : VU025876.D
Acq On : 04 Aug 2018 16:34
Operator : MD/SY
Sample : J4340-23
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

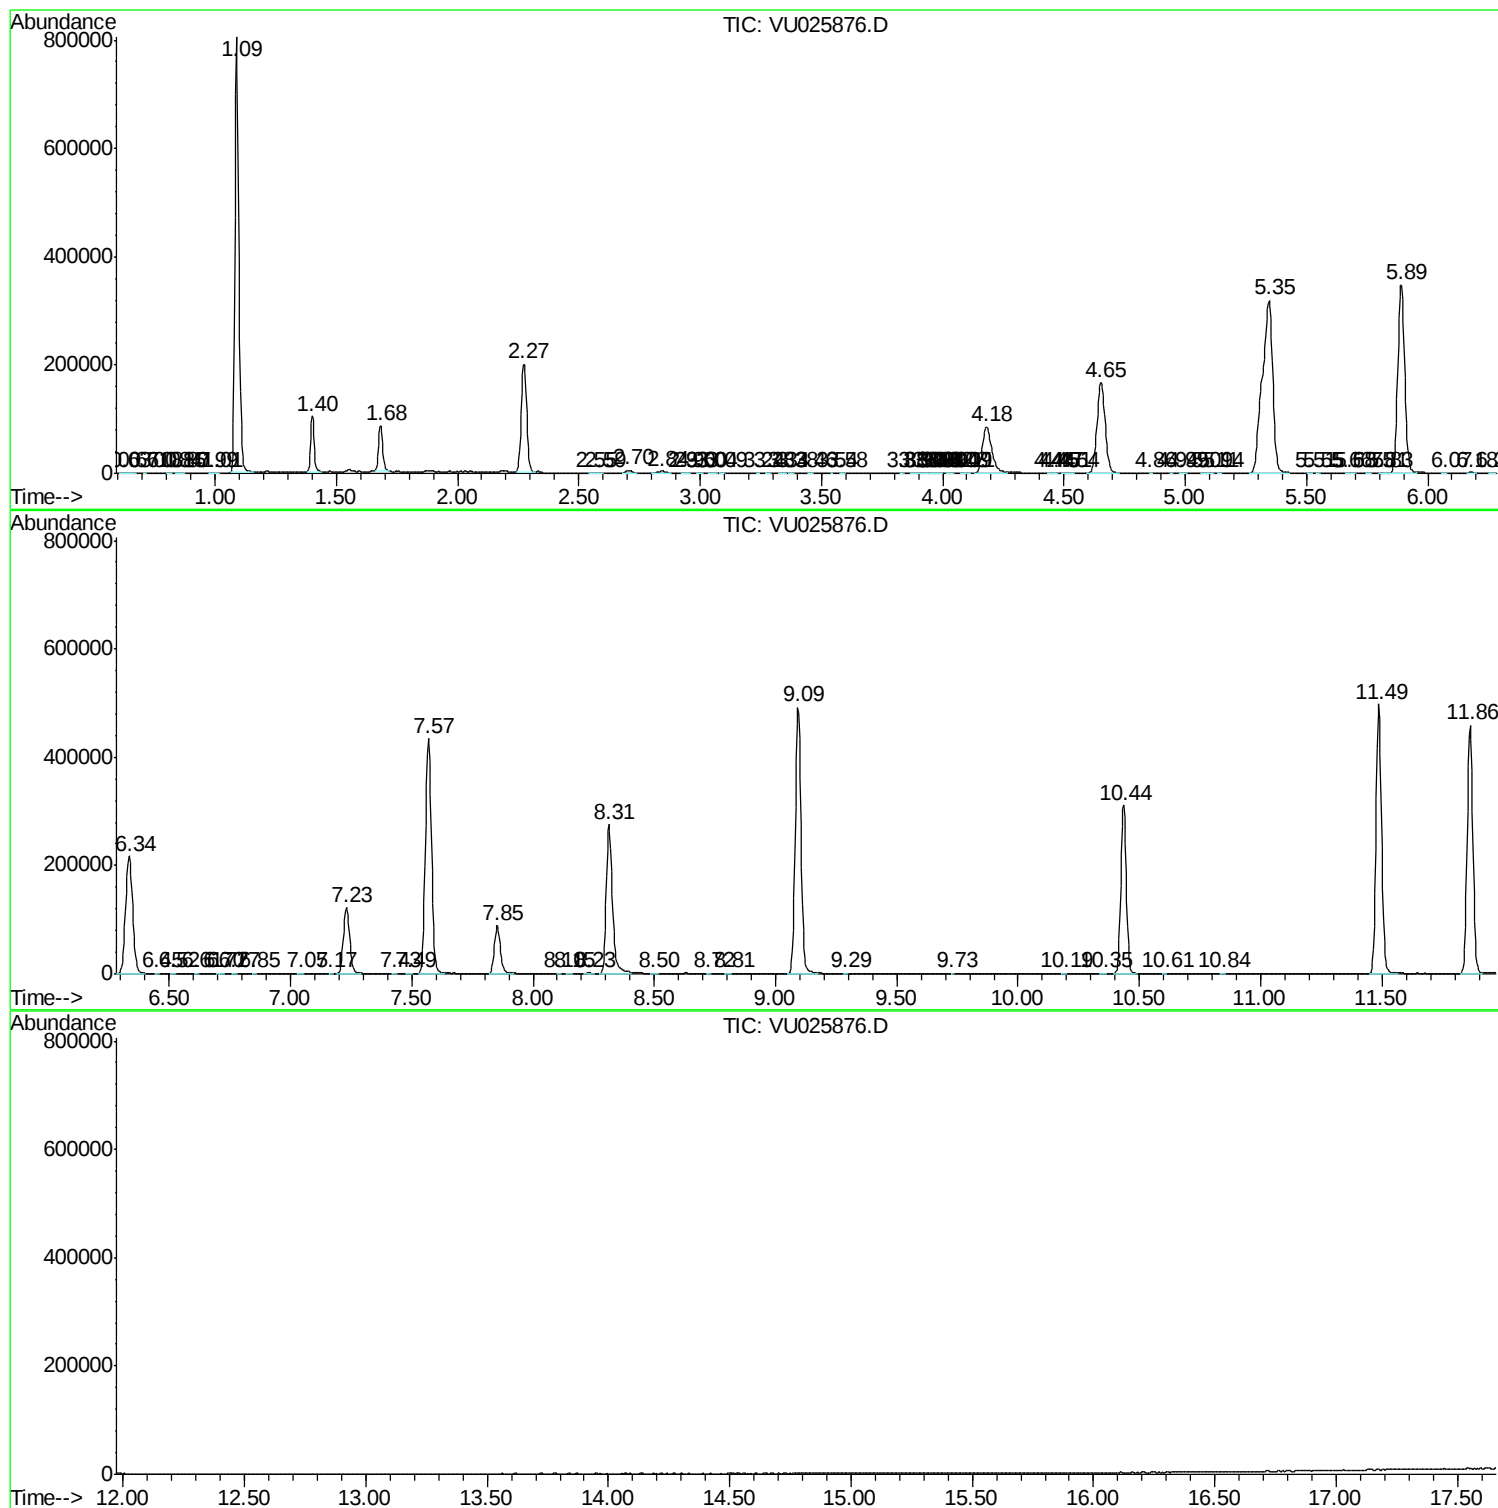

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080518\
Data File : VU025876.D
Acq On : 04 Aug 2018 16:34
Operator : MD/SY
Sample : J4340-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080518\
Data File : VU025876.D
Acq On : 04 Aug 2018 16:34
Operator : MD/SY
Sample : J4340-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc