


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080518\
Data File : VU025861.D
Acq On : 04 Aug 2018 09:26
Operator : MD/SY
Sample : BFB54
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB54

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Title : VOC Analysis
Last Update : Mon Aug 06 01:30:36 2018

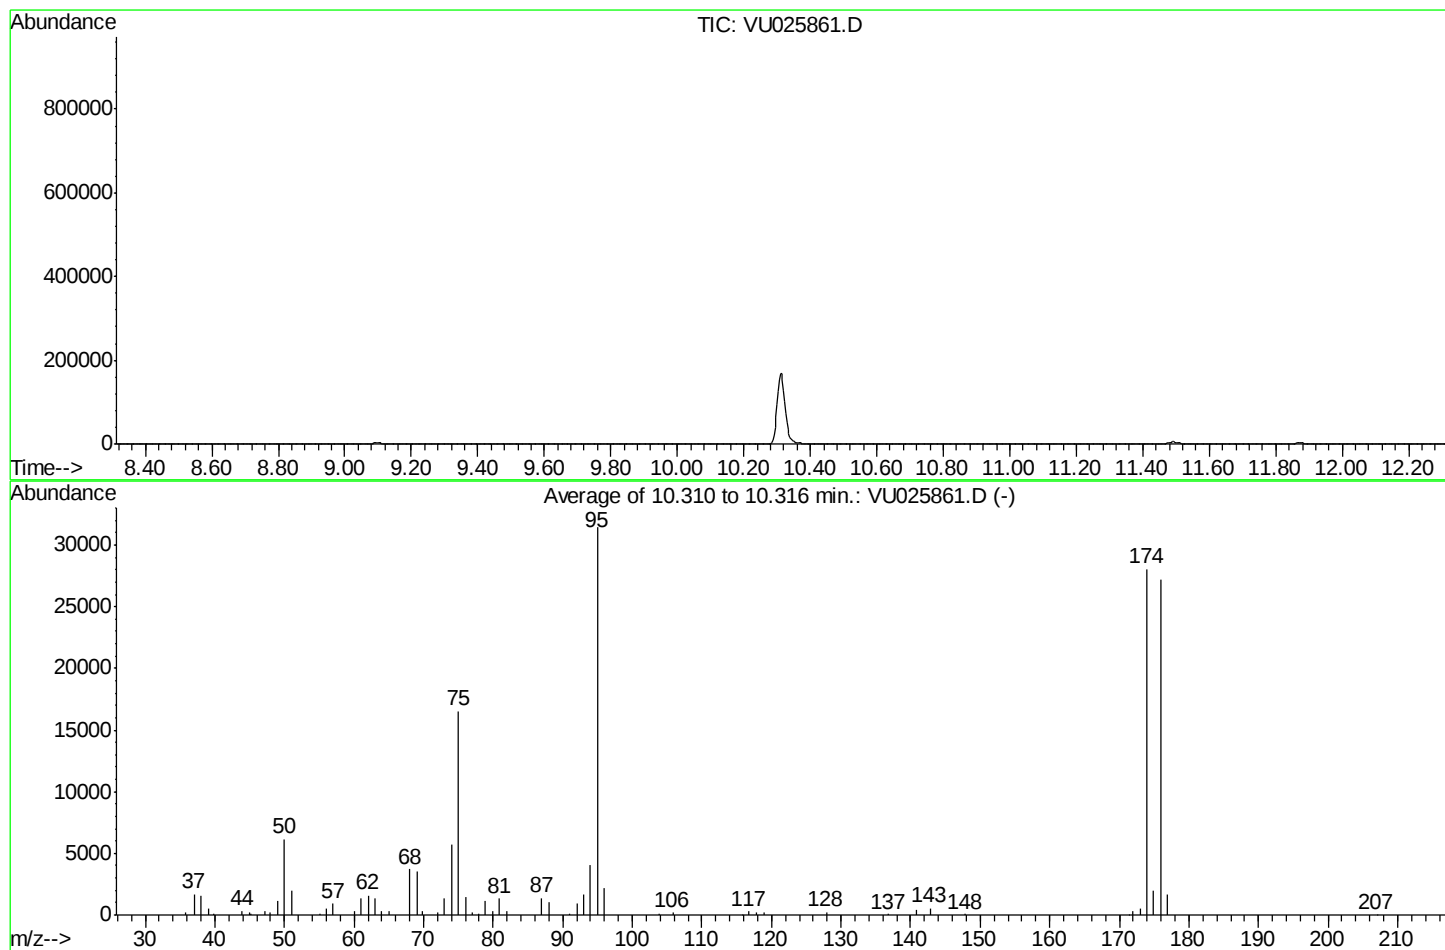

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	6177	PASS
75	95	30	80	52.6	16526	PASS
95	95	100	100	100.0	31440	PASS
96	95	5	9	7.0	2216	PASS
173	174	0.00	2	1.8	519	PASS
174	95	50	120	89.3	28082	PASS
175	174	5	9	7.2	2023	PASS
176	174	95	101	96.7	27154	PASS
177	176	5	9	6.0	1627	PASS

Scan 3011 (10.271 min): VU025861.D
BFB54

m/z	Abundance
44.10	247.0
207.00	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
35.00	263.0
37.00	1823.0
38.00	1643.0
39.00	575.0
39.80	102.0
43.90	607.0
44.90	340.0
47.20	237.0
47.90	173.0
49.00	1375.0
50.00	6349.0
51.00	2115.0
55.10	115.0
56.00	547.0
57.00	964.0
60.00	377.0
61.10	1453.0
62.00	1689.0
63.00	1386.0
64.00	316.0
65.00	373.0
68.00	3806.0
69.00	3610.0
69.90	305.0
72.00	174.0
73.00	1398.0
74.00	5879.0
75.00	17288.0
76.00	1480.0
77.00	174.0
78.90	1252.0
79.90	339.0
80.90	1414.0
81.90	282.0
87.00	1419.0
88.00	1262.0
91.10	146.0
92.00	1031.0
93.00	1625.0
94.00	4183.0
95.00	32216.0
96.00	2363.0
103.80	117.0
105.80	160.0
116.80	275.0
117.90	210.0
118.90	190.0
127.90	222.0
140.90	403.0
142.80	563.0
171.90	378.0
173.00	493.0
174.00	27936.0
175.00	2205.0
176.00	27384.0
176.90	1683.0
207.00	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
35.80	254.0
37.00	1724.0
38.00	1611.0
39.00	590.0
39.90	134.0
43.90	606.0
44.90	294.0
47.20	275.0
47.90	241.0
49.00	1182.0
50.00	6347.0
51.00	2011.0
55.10	115.0
56.00	541.0
57.00	963.0
60.00	352.0
61.00	1377.0
62.00	1608.0
63.00	1342.0
64.00	282.0
65.00	368.0
68.00	3891.0
69.00	3585.0
69.90	307.0
72.10	201.0
73.00	1449.0
74.00	5866.0
75.00	17016.0
76.00	1469.0
77.00	225.0
77.90	105.0
78.90	1209.0
79.90	357.0
80.90	1336.0
81.90	291.0
87.00	1439.0
88.00	1071.0
91.00	137.0
92.00	985.0
93.00	1677.0
94.00	4181.0
95.00	32496.0
96.00	2270.0
103.80	112.0
105.80	174.0
115.90	101.0
116.80	282.0
117.90	254.0
118.90	171.0
127.90	233.0
136.80	127.0
140.90	435.0
142.80	543.0
147.90	104.0
171.30	118.0
171.90	355.0
173.00	548.0
174.00	28832.0
175.00	2059.0
176.00	28016.0
176.90	1671.0
207.00	158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
35.80	261.0
37.00	1490.0
38.00	1415.0
39.00	509.0
40.00	187.0
43.90	487.0
45.10	254.0
47.10	284.0
47.90	279.0
49.00	1027.0
50.00	5836.0
51.00	1813.0
55.10	107.0
56.00	507.0
57.00	878.0
60.00	286.0
61.00	1306.0
62.00	1482.0
63.00	1200.0
64.00	194.0
65.00	305.0
68.00	3512.0
69.00	3324.0
69.90	237.0
72.10	164.0
73.00	1366.0
74.00	5441.0
75.00	15275.0
76.00	1313.0
77.00	226.0
77.80	106.0
78.90	1094.0
79.90	320.0
80.90	1203.0
81.90	299.0
87.00	1234.0
88.00	948.0
90.90	114.0
92.00	927.0
93.00	1544.0
94.00	3776.0
95.00	29608.0
96.00	2015.0
103.80	121.0
105.80	160.0
116.70	288.0
117.80	240.0
119.00	180.0
127.90	191.0
136.80	125.0
140.90	386.0
142.90	510.0
147.90	100.0
172.00	317.0
173.10	516.0
174.00	27480.0
174.90	1806.0
176.00	26064.0
176.90	1527.0
207.00	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54