


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU080519\
 Data File : VU033589.D
 Acq On : 05 Aug 2019 08:23
 Operator : JC/SP
 Sample : BFB47
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB47

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080319WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 05 17:10:43 2019

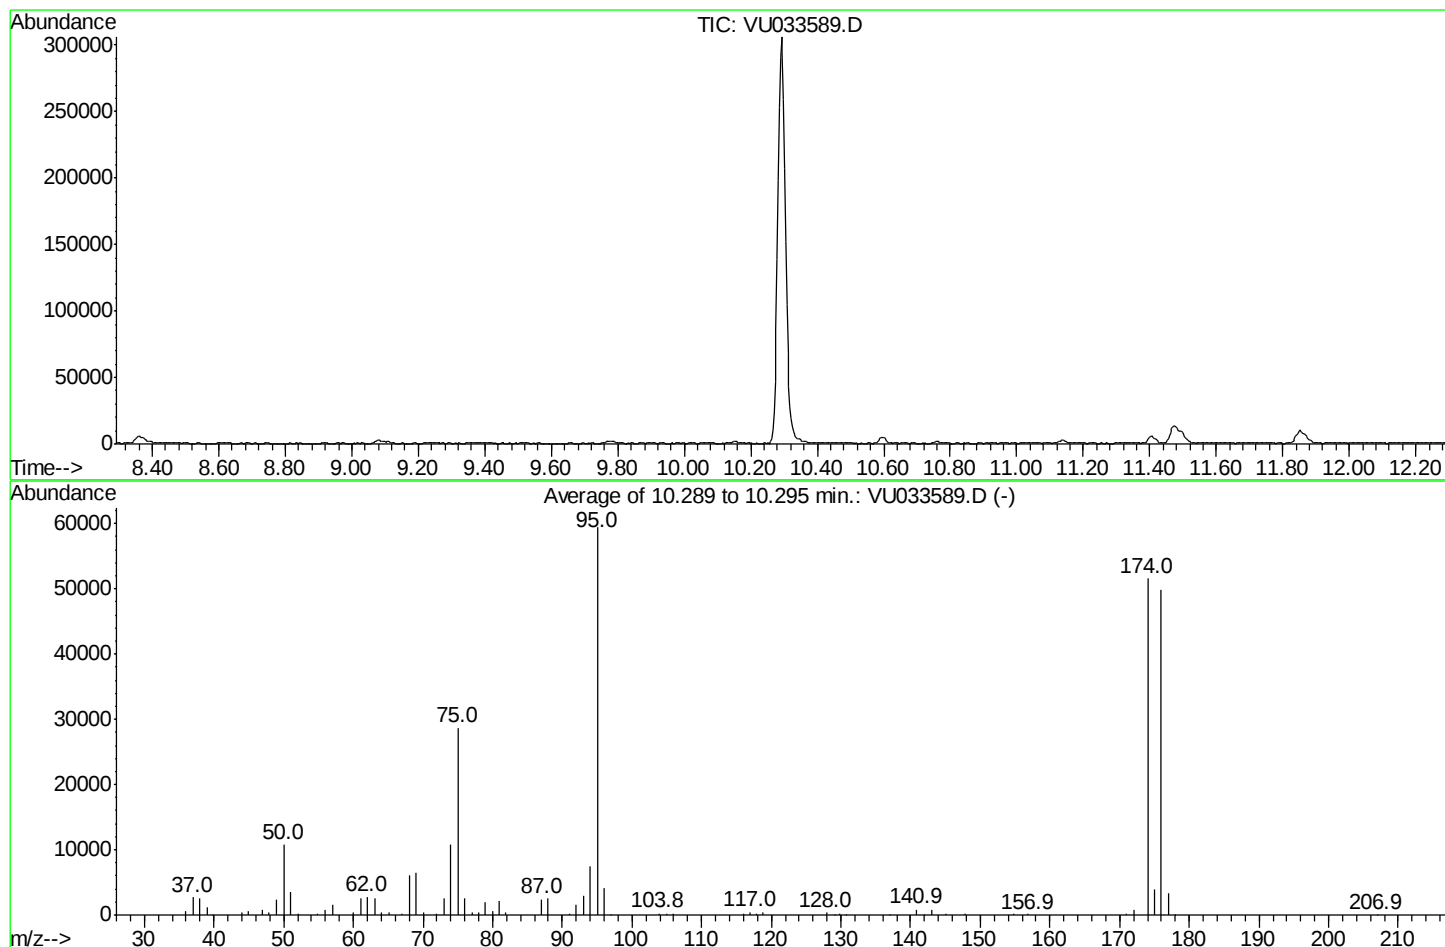

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	10766	PASS
75	95	30	80	48.4	28730	PASS
95	95	100	100	100.0	59416	PASS
96	95	5	9	6.9	4097	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.8	51589	PASS
175	174	5	9	7.5	3873	PASS
176	174	95	101	96.6	49826	PASS
177	176	5	9	6.5	3251	PASS

m/z	Abundance
36.00	655.0
37.00	2609.0
38.00	2459.0
39.00	1086.0
39.90	243.0
44.00	646.0
45.00	567.0
46.90	739.0
48.00	313.0
49.00	2302.0
50.00	10657.0
51.00	3570.0
52.00	166.0
54.90	155.0
56.00	820.0
57.00	1474.0
59.80	456.0
61.10	2594.0
62.00	2661.0
63.00	2506.0
64.00	329.0
65.00	443.0
67.00	207.0
68.00	5997.0
69.00	6495.0
70.00	481.0
72.00	326.0
73.00	2718.0
74.00	10756.0
75.00	28320.0
76.00	2503.0
77.00	442.0
78.00	304.0
79.00	1850.0
80.00	618.0
80.90	2100.0
81.90	397.0
87.00	2300.0
87.90	2415.0
91.00	226.0
92.00	1547.0
93.00	2884.0
94.00	7096.0
95.00	58320.0
96.00	3835.0
103.80	267.0
104.90	131.0
105.90	244.0
116.00	253.0
117.00	445.0
117.80	177.0
118.80	384.0
128.00	277.0
129.80	266.0
137.00	118.0
140.90	828.0
142.90	761.0
145.00	170.0
147.90	136.0
154.90	119.0
156.90	173.0
171.00	106.0
172.00	694.0
174.00	52240.0
175.00	3723.0
176.00	50632.0
177.00	3206.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	583.0
37.00	2606.0
38.00	2444.0
39.00	1220.0
39.90	251.0
44.00	734.0
44.90	573.0
47.00	819.0
47.90	326.0
49.00	2372.0
50.00	10595.0
51.00	3324.0
52.00	161.0
54.90	215.0
56.00	887.0
57.00	1631.0
60.00	413.0
61.10	2530.0
62.00	2850.0
63.10	2581.0
64.00	281.0
65.10	306.0
67.10	178.0
68.00	6026.0
69.00	6256.0
70.00	476.0
72.00	217.0
73.00	2387.0
74.00	10551.0
75.00	28464.0
76.00	2565.0
77.00	364.0
78.00	324.0
78.90	2008.0
80.00	511.0
80.90	2211.0
81.90	408.0
87.00	2405.0
88.00	2530.0
91.00	225.0
92.00	1664.0
93.00	2795.0
94.00	7548.0
95.00	58672.0
96.00	4278.0
97.00	110.0
103.90	278.0
105.00	107.0
105.80	305.0
116.00	230.0
116.90	456.0
117.80	168.0
118.90	389.0
127.90	372.0
129.00	126.0
129.80	306.0
130.80	110.0
140.90	766.0
142.00	110.0
143.00	675.0
145.00	232.0
147.80	115.0
154.80	175.0
156.90	141.0
171.10	151.0
172.00	687.0
174.00	49560.0
175.00	3929.0
176.00	47472.0
177.00	3194.0
178.00	130.0
206.90	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

Scan 2850 (10.254 min): VU033589.D
BFB47

m/z	Abundance
39.80	195.0
43.90	293.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	643.0
37.00	2772.0
38.00	2516.0
39.00	1221.0
39.90	243.0
44.00	745.0
45.00	590.0
46.90	807.0
47.90	336.0
49.00	2410.0
50.00	11048.0
51.00	3614.0
52.00	172.0
54.90	186.0
56.00	898.0
57.00	1676.0
59.90	439.0
61.10	2728.0
62.00	2941.0
63.10	2591.0
64.00	300.0
65.10	410.0
67.10	210.0
68.00	6268.0
69.00	6729.0
70.00	496.0
72.00	263.0
73.00	2673.0
74.00	11144.0
75.00	29408.0
76.00	2714.0
77.00	427.0
78.00	316.0
78.90	2037.0
80.00	610.0
80.90	2239.0
81.90	398.0
87.00	2395.0
88.00	2581.0
91.00	259.0
92.00	1660.0
93.00	2977.0
94.00	7792.0
95.00	61256.0
96.00	4178.0
97.00	110.0
103.80	286.0
104.90	130.0
105.80	271.0
116.00	277.0
116.90	501.0
117.80	177.0
118.80	407.0
127.90	339.0
129.90	307.0
140.90	843.0
142.90	725.0
145.00	225.0
147.80	131.0
154.80	149.0
156.90	175.0
171.00	145.0
172.00	732.0
174.00	52968.0
175.00	3967.0
176.00	51376.0
177.00	3355.0
178.00	113.0
206.90	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47