


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU080520\
Data File : VU039741.D
Acq On : 05 Aug 2020 09:58
Operator : SY/MD
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U072920DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Fri Jul 31 07:12:27 2020

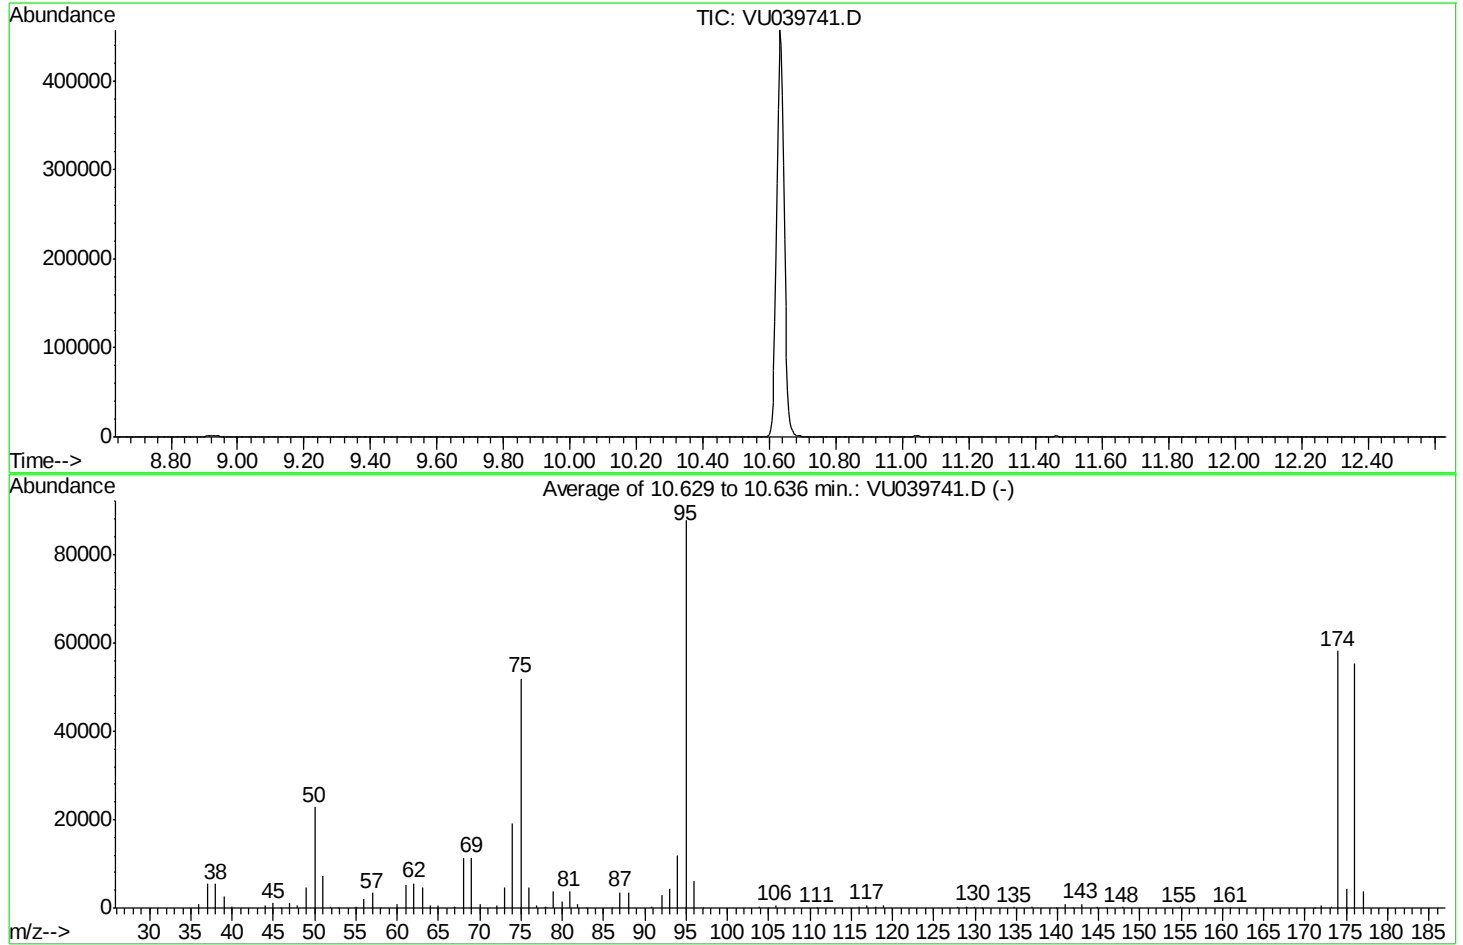

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.1	22869	PASS
75	95	30	60	59.2	51968	PASS
95	95	100	100	100.0	87717	PASS
96	95	5	9	6.8	5994	PASS
173	174	0.00	2	0.8	437	PASS
174	95	50	100	66.2	58090	PASS
175	174	5	9	7.7	4481	PASS
176	174	95	101	95.2	55288	PASS
177	176	5	9	6.8	3755	PASS