
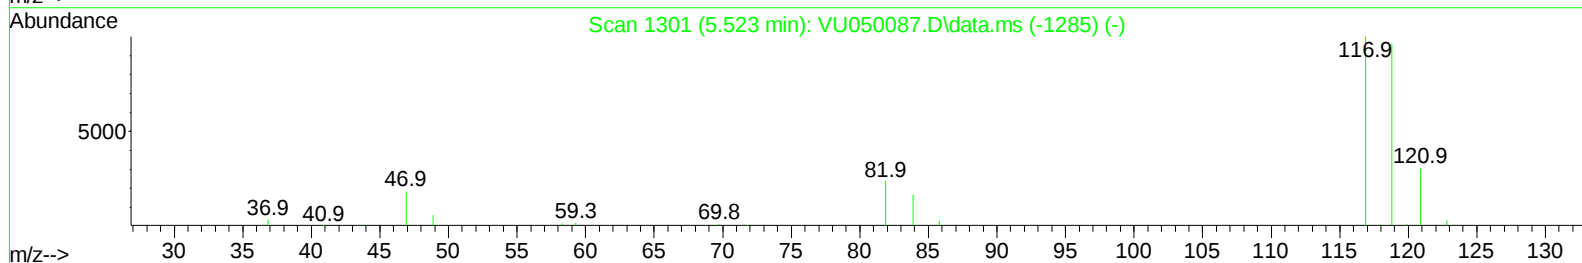
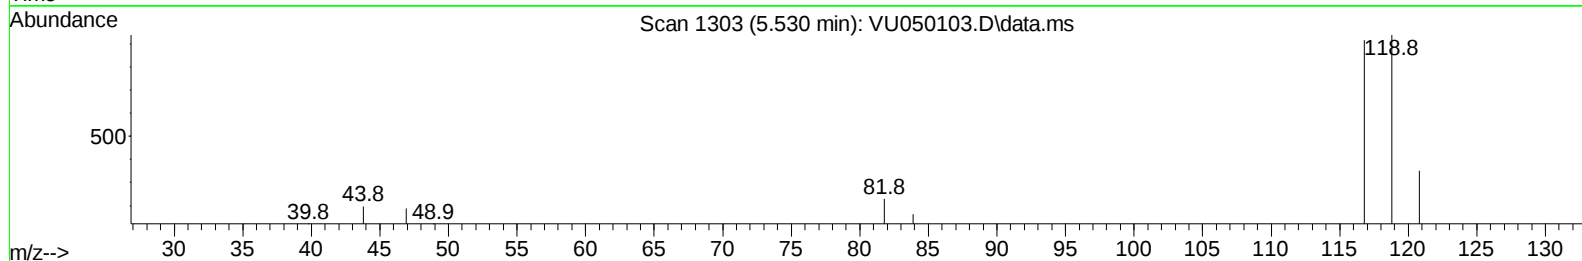


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080522\
 Data File : VU050103.D
 Acq On : 05 Aug 2022 17:54
 Operator : SY/MD
 Sample : N4027-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Quant Time: Aug 06 04:37:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 06 04:32:47 2022
 Response via : Initial Calibration

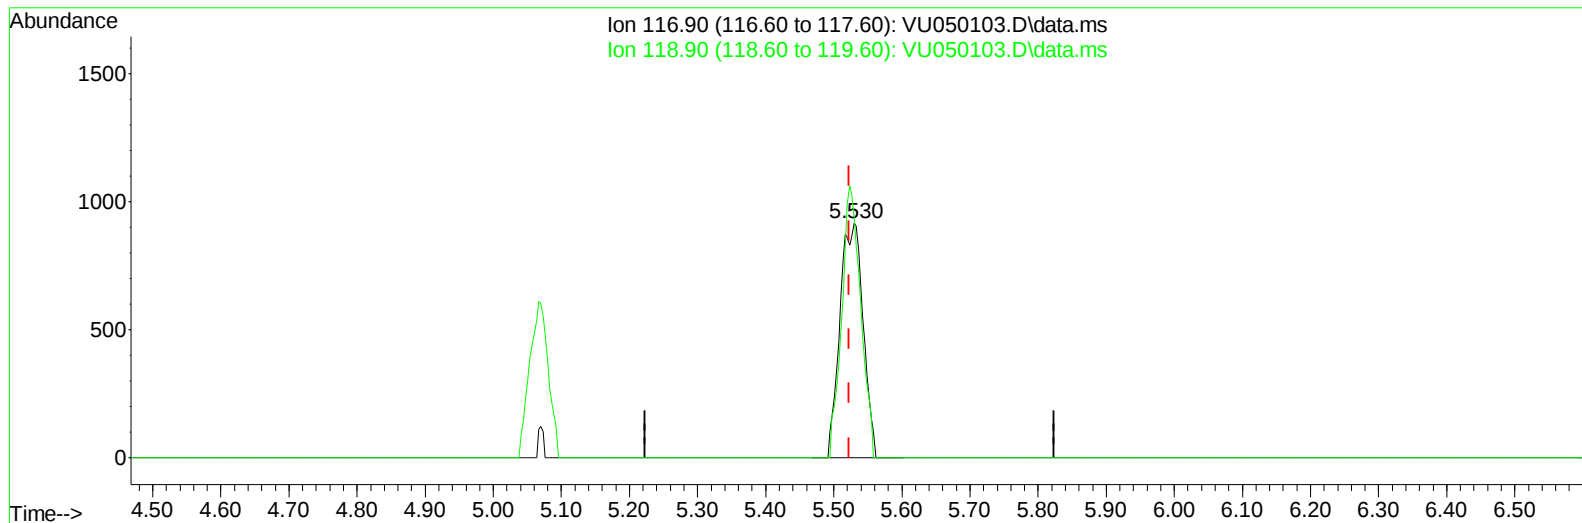

TIC: VU050103.D\data.ms

(31) Carbon tetrachloride (T)

5.530min (+ 0.006) 0.27 ug/L m

response 2160

Ion	Exp%	Act%
116.90	100.00	100.00
118.90	95.00	94.77
0.00	0.00	0.00
0.00	0.00	0.00