

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080522\
 Data File : VU050108.D
 Acq On : 05 Aug 2022 20:47
 Operator : SY/MD
 Sample : N4027-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBJJ0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050108.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	70	80	90	rBV	42220	50261	12.17%	1.806%
2	1.687	102	108	118	rBV	3406	4666	1.13%	0.168%
3	1.909	169	177	188	rBV	35848	46310	11.22%	1.664%
4	2.565	369	381	394	rBV	64506	103339	25.03%	3.712%
5	2.636	394	403	420	rVB	5781	10942	2.65%	0.393%
6	3.851	742	781	784	rBV	4186	16637	4.03%	0.598%
7	4.629	1011	1023	1045	rBV2	62738	163825	39.68%	5.885%
8	5.063	1143	1158	1176	rBV	68014	150386	36.43%	5.402%
9	5.726	1344	1364	1391	rBV2	134552	348020	84.29%	12.502%
10	6.250	1514	1527	1548	rBV	95081	181048	43.85%	6.504%
11	6.690	1648	1664	1684	rBV	86973	168455	40.80%	6.052%
12	7.568	1925	1937	1953	rBV	38345	66540	16.12%	2.390%
13	7.899	2027	2040	2058	rBV	150451	262341	63.54%	9.424%
14	8.182	2112	2128	2143	rBV2	22563	38686	9.37%	1.390%
15	8.639	2256	2270	2305	rBV3	174767	412863	100.00%	14.832%
16	8.790	2308	2317	2330	rVB3	11090	19146	4.64%	0.688%
17	9.417	2500	2512	2533	rBV	135192	227849	55.19%	8.185%
18	10.758	2916	2929	2947	rVB	73795	118125	28.61%	4.243%
19	11.812	3245	3257	3279	rBV	110290	176895	42.85%	6.355%
20	12.195	3361	3376	3396	rBV	128304	211112	51.13%	7.584%
21	12.893	3586	3593	3599	rBV3	4868	6236	1.51%	0.224%




Sum of corrected areas: 2783682

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080522\
Data File : VU050108.D
Acq On : 05 Aug 2022 20:47
Operator : SY/MD
Sample : N4027-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

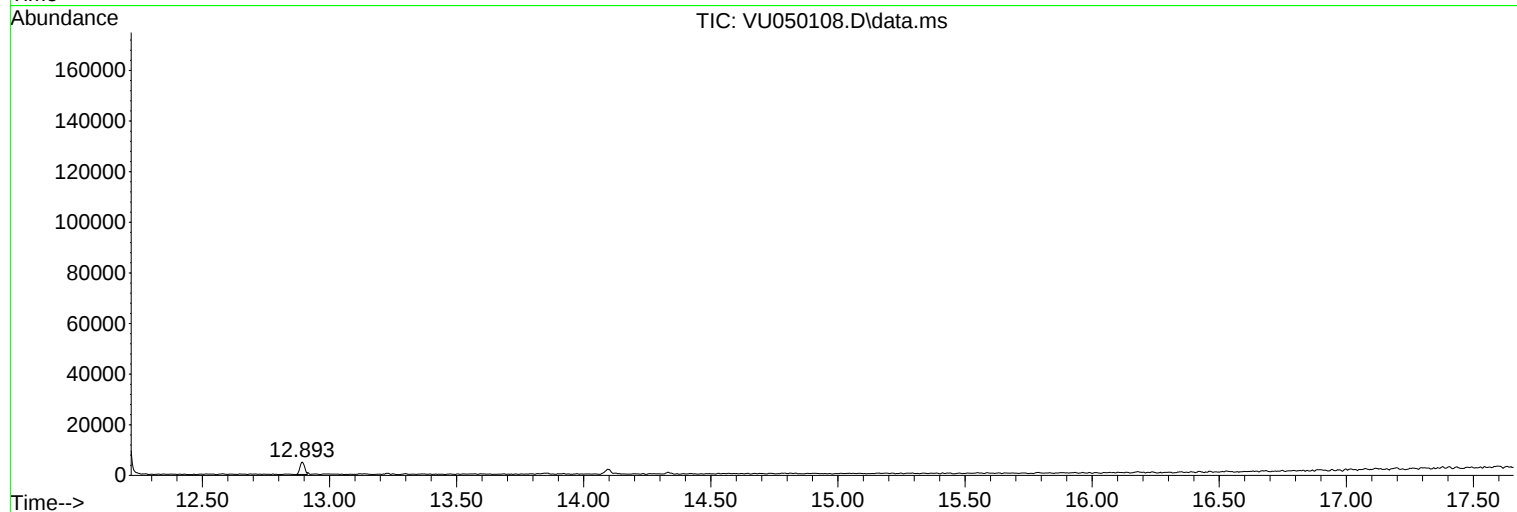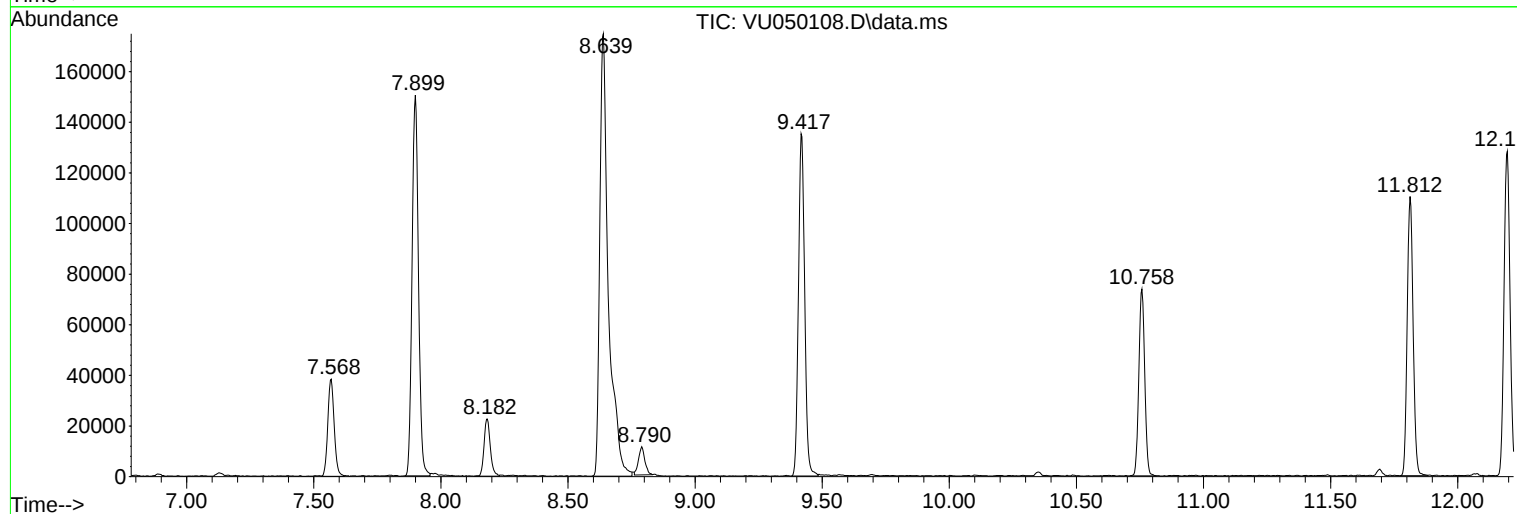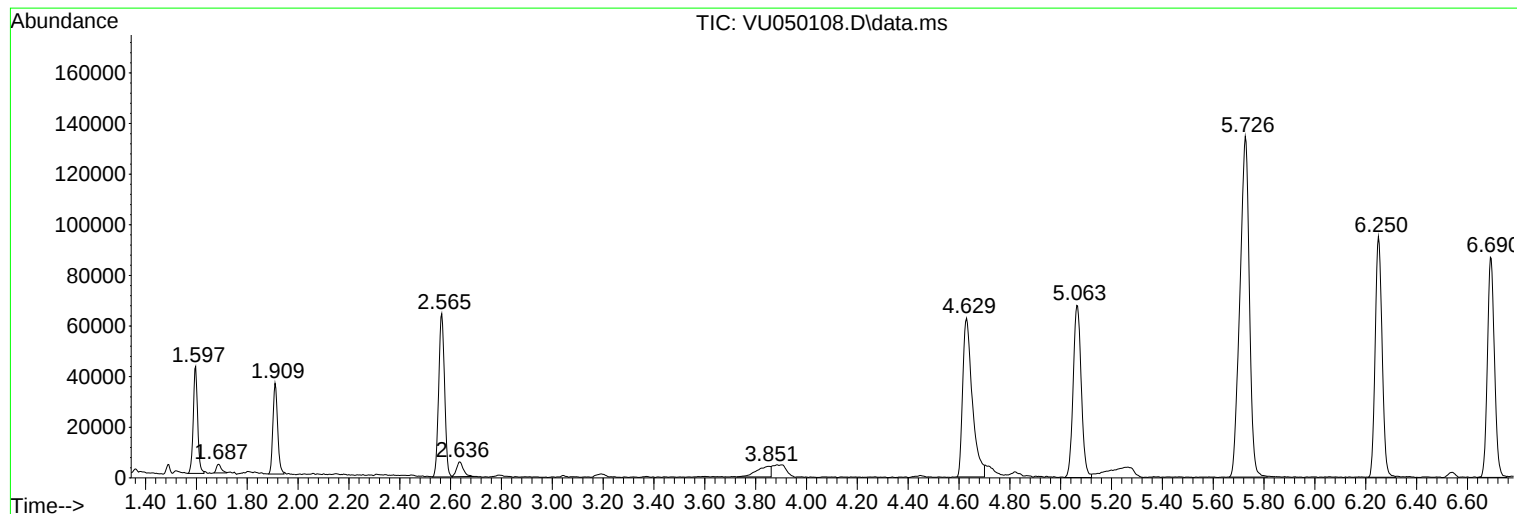

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080522\
Data File : VU050108.D
Acq On : 05 Aug 2022 20:47
Operator : SY/MD
Sample : N4027-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080522\
Data File : VU050108.D
Acq On : 05 Aug 2022 20:47
Operator : SY/MD
Sample : N4027-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc