

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080522\
 Data File : VU050128.D
 Acq On : 06 Aug 2022 04:59
 Operator : SY/MD
 Sample : N4075-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUV1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rVB2	59315	72188	17.86%	2.462%
2	1.912	169	178	188	rBV	31074	39637	9.81%	1.352%
3	2.202	262	268	279	rVB3	2879	4561	1.13%	0.156%
4	2.565	369	381	394	rBV	54377	87583	21.67%	2.987%
5	2.793	440	452	463	rBV2	3057	5187	1.28%	0.177%
6	3.353	610	626	650	rBV2	173926	367156	90.84%	12.520%
7	3.806	751	767	769	rBV	3393	6748	1.67%	0.230%
8	4.626	1008	1022	1056	rBV3	61271	205323	50.80%	7.001%
9	5.063	1141	1158	1176	rBV	59038	131235	32.47%	4.475%
10	5.726	1343	1364	1388	rBV3	112039	299494	74.10%	10.213%
11	5.941	1422	1431	1444	rVB5	2438	4693	1.16%	0.160%
12	6.250	1512	1527	1550	rBV	90160	171356	42.40%	5.843%
13	6.690	1652	1664	1684	rBV	74430	144635	35.79%	4.932%
14	7.565	1925	1936	1952	rBV2	30010	51938	12.85%	1.771%
15	7.899	2019	2040	2056	rBV	120729	211162	52.25%	7.200%
16	8.179	2115	2127	2143	rBV2	18034	30568	7.56%	1.042%
17	8.636	2256	2269	2303	rBV2	198220	404175	100.00%	13.782%
18	9.417	2500	2512	2533	rBV	130533	217761	53.88%	7.425%
19	10.755	2917	2928	2946	rBV	69799	113443	28.07%	3.868%
20	11.812	3243	3257	3275	rBV	107815	173953	43.04%	5.932%
21	12.192	3364	3375	3396	rBV	115788	189819	46.96%	6.473%




Sum of corrected areas: 2932615

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080522\
Data File : VU050128.D
Acq On : 06 Aug 2022 04:59
Operator : SY/MD
Sample : N4075-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUV1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

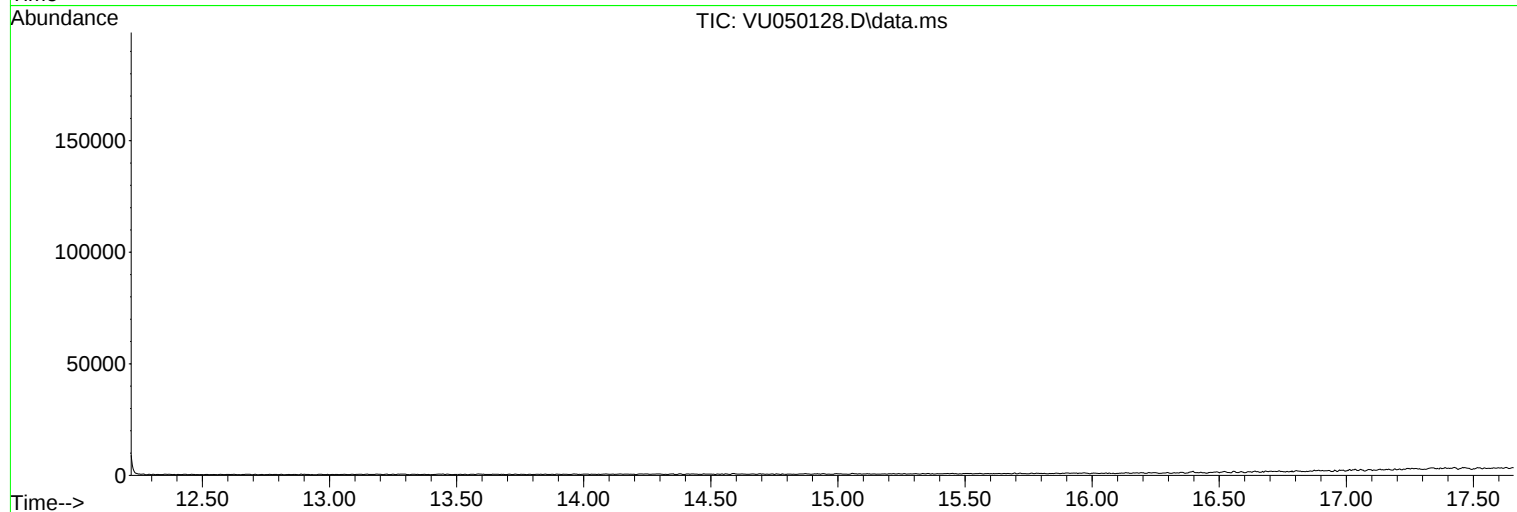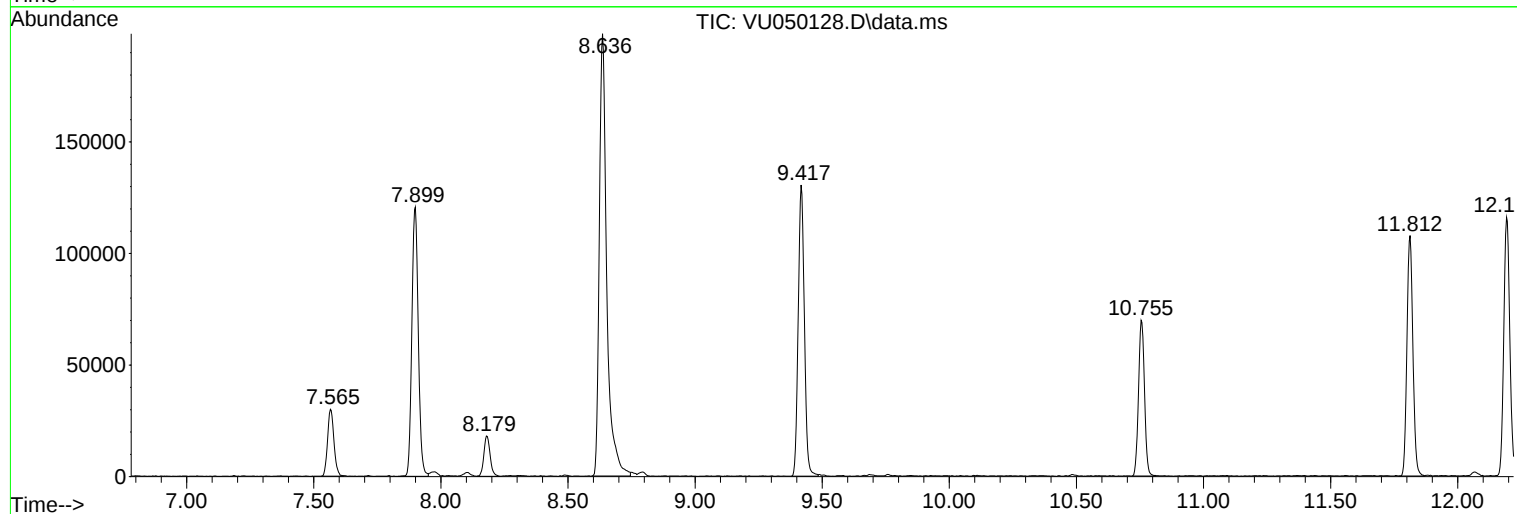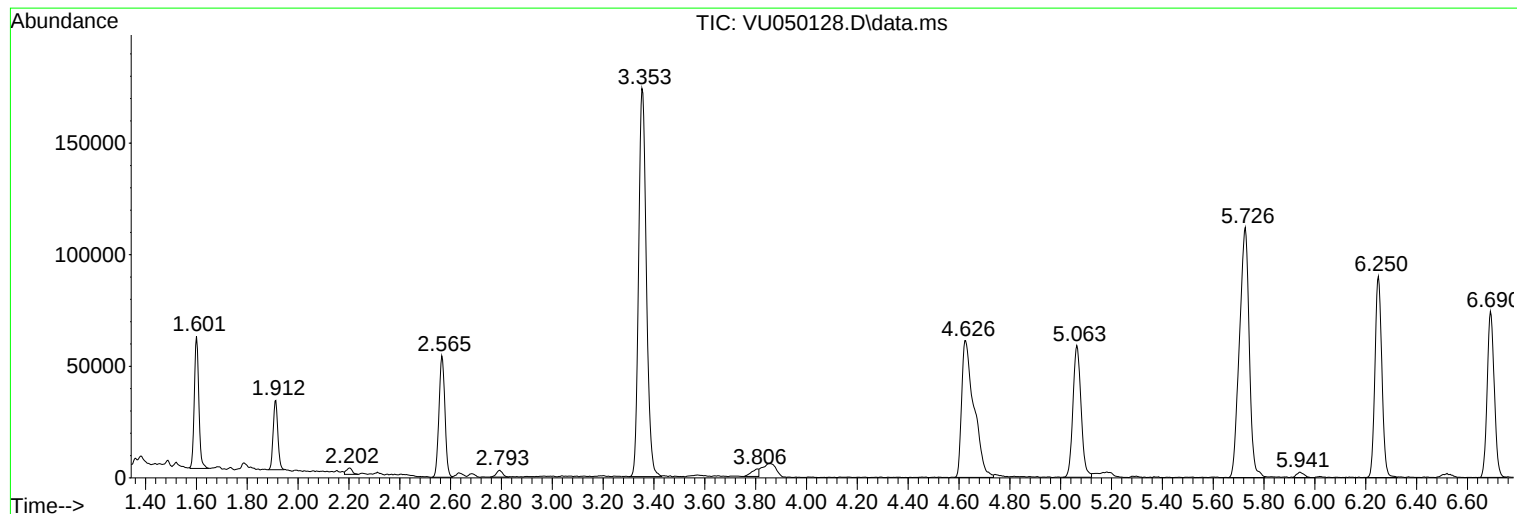

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080522\
Data File : VU050128.D
Acq On : 06 Aug 2022 04:59
Operator : SY/MD
Sample : N4075-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUV1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080522\
Data File : VU050128.D
Acq On : 06 Aug 2022 04:59
Operator : SY/MD
Sample : N4075-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUV1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc