
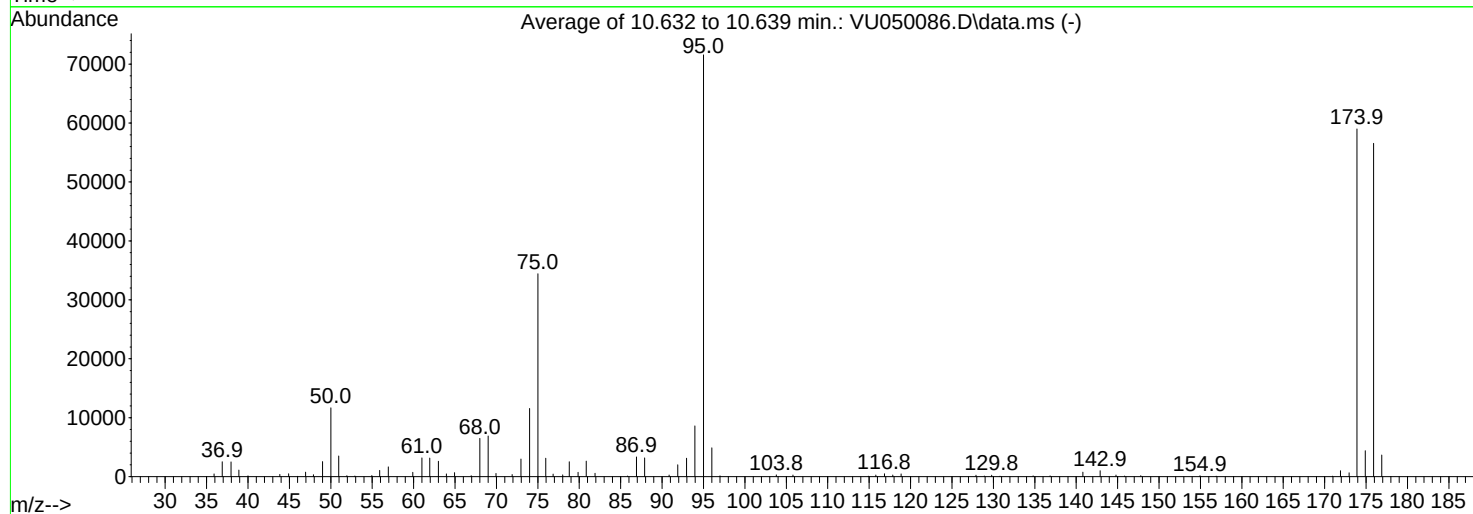


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080522\
 Data File : VU050086.D
 Acq On : 05 Aug 2022 08:14
 Operator : SY/MD
 Sample : BFB101
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB101

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Aug 09 03:59:45 2022

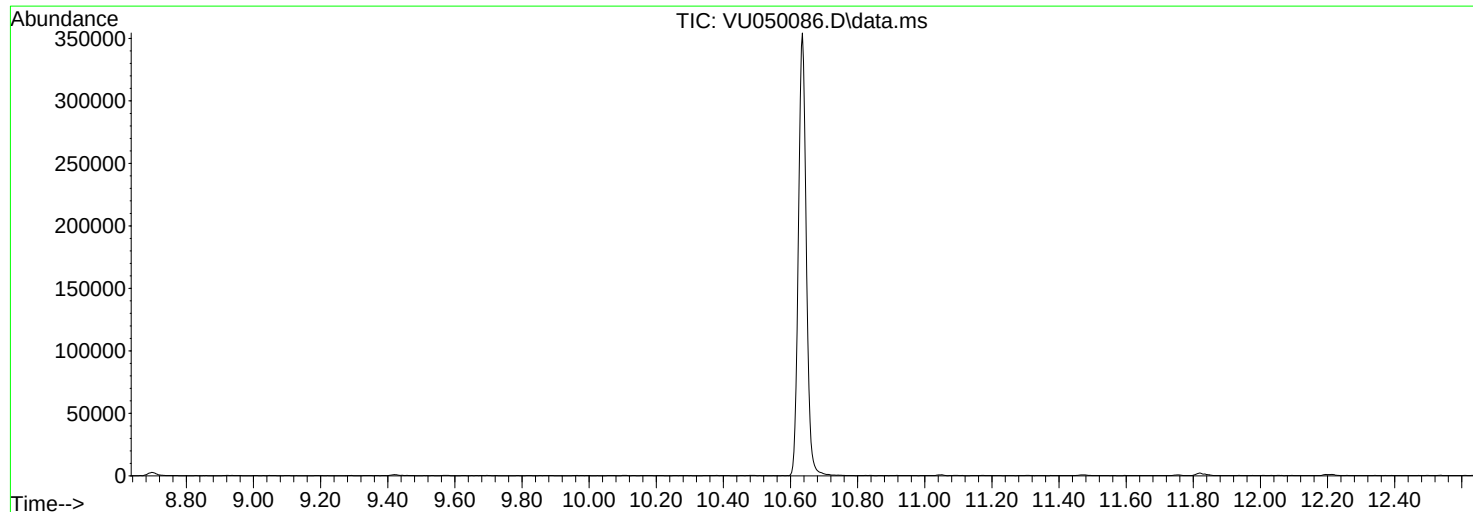

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	11672	PASS
75	95	30	80	48.1	34435	PASS
95	95	100	100	100.0	71573	PASS
96	95	5	9	6.8	4889	PASS
173	174	0.00	2	1.1	665	PASS
174	95	50	120	82.4	58989	PASS
175	174	5	9	7.5	4406	PASS
176	174	95	101	95.9	56547	PASS
177	176	5	9	6.5	3656	PASS

m/z	Abundance
43.80	199.0

Instrument :
MSVOA_U
ClientSampleId :
BFB101

m/z	Abundance
35.90	485.0
36.90	2570.0
38.00	2591.0
38.90	1134.0
40.00	142.0
43.90	533.0
44.90	519.0
46.00	135.0
46.90	717.0
47.90	326.0
49.00	2727.0
50.00	11843.0
51.00	3654.0
51.90	192.0
52.90	122.0
54.90	204.0
55.90	1031.0
56.90	1673.0
59.90	728.0
61.00	3376.0
62.00	3204.0
63.00	2717.0
64.00	469.0
65.00	711.0
66.90	164.0
68.00	6608.0
69.00	6987.0
70.00	560.0
71.90	326.0
73.00	3016.0
74.00	11653.0
75.00	34904.0
76.00	3311.0
76.80	393.0
78.00	312.0
78.80	2509.0
79.80	773.0
80.90	2688.0
81.90	592.0
85.80	110.0
86.90	3438.0
87.90	3186.0
90.80	294.0
91.90	2035.0
93.00	3136.0
94.00	8625.0
95.00	71392.0
96.00	5138.0
97.00	120.0
103.80	318.0
105.80	302.0
114.90	125.0
115.80	255.0
116.80	508.0
117.80	252.0
118.90	500.0
127.90	251.0
128.90	131.0
129.80	222.0
134.80	121.0
136.90	124.0
140.80	751.0
142.90	1023.0
144.80	308.0
145.90	105.0
147.80	161.0
155.00	154.0
170.90	122.0
171.90	964.0
173.00	735.0
173.90	58328.0
174.90	4331.0
175.90	55488.0
176.90	3713.0
178.00	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB101

m/z	Abundance
35.90	497.0
36.90	2636.0
37.90	2595.0
38.90	1145.0
40.00	134.0
43.90	587.0
44.90	497.0
46.90	783.0
47.90	349.0
49.00	2641.0
50.00	12126.0
51.00	3568.0
51.90	158.0
52.90	116.0
54.90	206.0
55.90	1123.0
56.90	1710.0
59.90	781.0
61.00	3300.0
62.00	3240.0
63.00	2673.0
64.00	472.0
65.00	688.0
67.00	178.0
68.00	6592.0
69.00	7126.0
70.00	579.0
71.90	348.0
72.90	3074.0
74.00	11966.0
75.00	35560.0
76.00	3214.0
76.90	465.0
78.00	326.0
78.80	2611.0
79.80	767.0
80.80	2736.0
81.90	591.0
85.90	130.0
86.90	3473.0
87.90	3317.0
90.80	290.0
91.90	2083.0
93.00	3202.0
94.00	8906.0
95.00	73792.0
96.00	5066.0
97.00	131.0
103.80	302.0
105.80	284.0
114.90	107.0
115.80	281.0
116.90	488.0
117.90	262.0
118.90	484.0
127.90	238.0
128.90	129.0
129.80	260.0
130.80	109.0
134.80	134.0
136.80	146.0
140.80	810.0
142.90	1070.0
144.80	295.0
145.90	106.0
147.80	161.0
154.90	162.0
156.90	114.0
159.00	102.0
171.00	101.0
171.90	1033.0
173.00	674.0
173.90	60944.0
174.90	4568.0
175.90	58592.0
176.90	3791.0

Instrument :
MSVOA_U
ClientSampleId :
BFB101

m/z	Abundance
35.90	437.0
36.90	2404.0
37.90	2323.0
38.90	1037.0
40.00	113.0
43.90	619.0
44.90	484.0
47.00	766.0
47.90	342.0
49.00	2331.0
50.00	11046.0
50.90	3278.0
52.00	129.0
52.90	110.0
55.00	191.0
55.90	1054.0
57.00	1576.0
59.90	695.0
61.00	2877.0
61.90	2983.0
63.00	2474.0
63.90	415.0
64.90	675.0
67.00	184.0
68.00	6260.0
69.00	6614.0
69.90	525.0
71.90	368.0
73.00	2895.0
74.00	11052.0
75.00	32840.0
75.90	2880.0
76.90	484.0
78.00	276.0
78.80	2434.0
79.90	696.0
80.90	2466.0
81.90	547.0
85.90	124.0
86.90	3135.0
87.90	3052.0
90.90	263.0
91.90	1890.0
92.90	2997.0
93.90	8268.0
95.00	69536.0
96.00	4462.0
97.00	132.0
103.80	260.0
105.80	266.0
115.80	269.0
116.90	448.0
117.90	269.0
118.80	433.0
127.90	230.0
128.90	102.0
129.80	258.0
130.80	106.0
134.80	133.0
136.80	158.0
140.80	723.0
142.90	946.0
144.80	255.0
145.80	106.0
147.80	147.0
154.90	169.0
156.90	123.0
171.90	1008.0
172.90	586.0
173.90	57696.0
174.90	4318.0
175.90	55560.0
176.90	3463.0

Instrument :
MSVOA_U
ClientSampleId :
BFB101