

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080524\
 Data File : VU060311.D
 Acq On : 05 Aug 2024 14:44
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Aug 06 06:03:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Aug 06 05:58:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.107	96	32152	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.631	95	7665	0.700	ug/l	0.00
Spiked Amount 1.000			Recovery	=	70.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	8328	0.700	ug/l	0.00
Spiked Amount 1.000			Recovery	=	70.000%	
Target Compounds						
15) Methylene Chloride	3.033	84	4172	0.347	ug/l	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080524\
Data File : VU060311.D
Acq On : 05 Aug 2024 14:44
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Aug 06 06:03:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Aug 06 05:58:50 2024
Response via : Initial Calibration




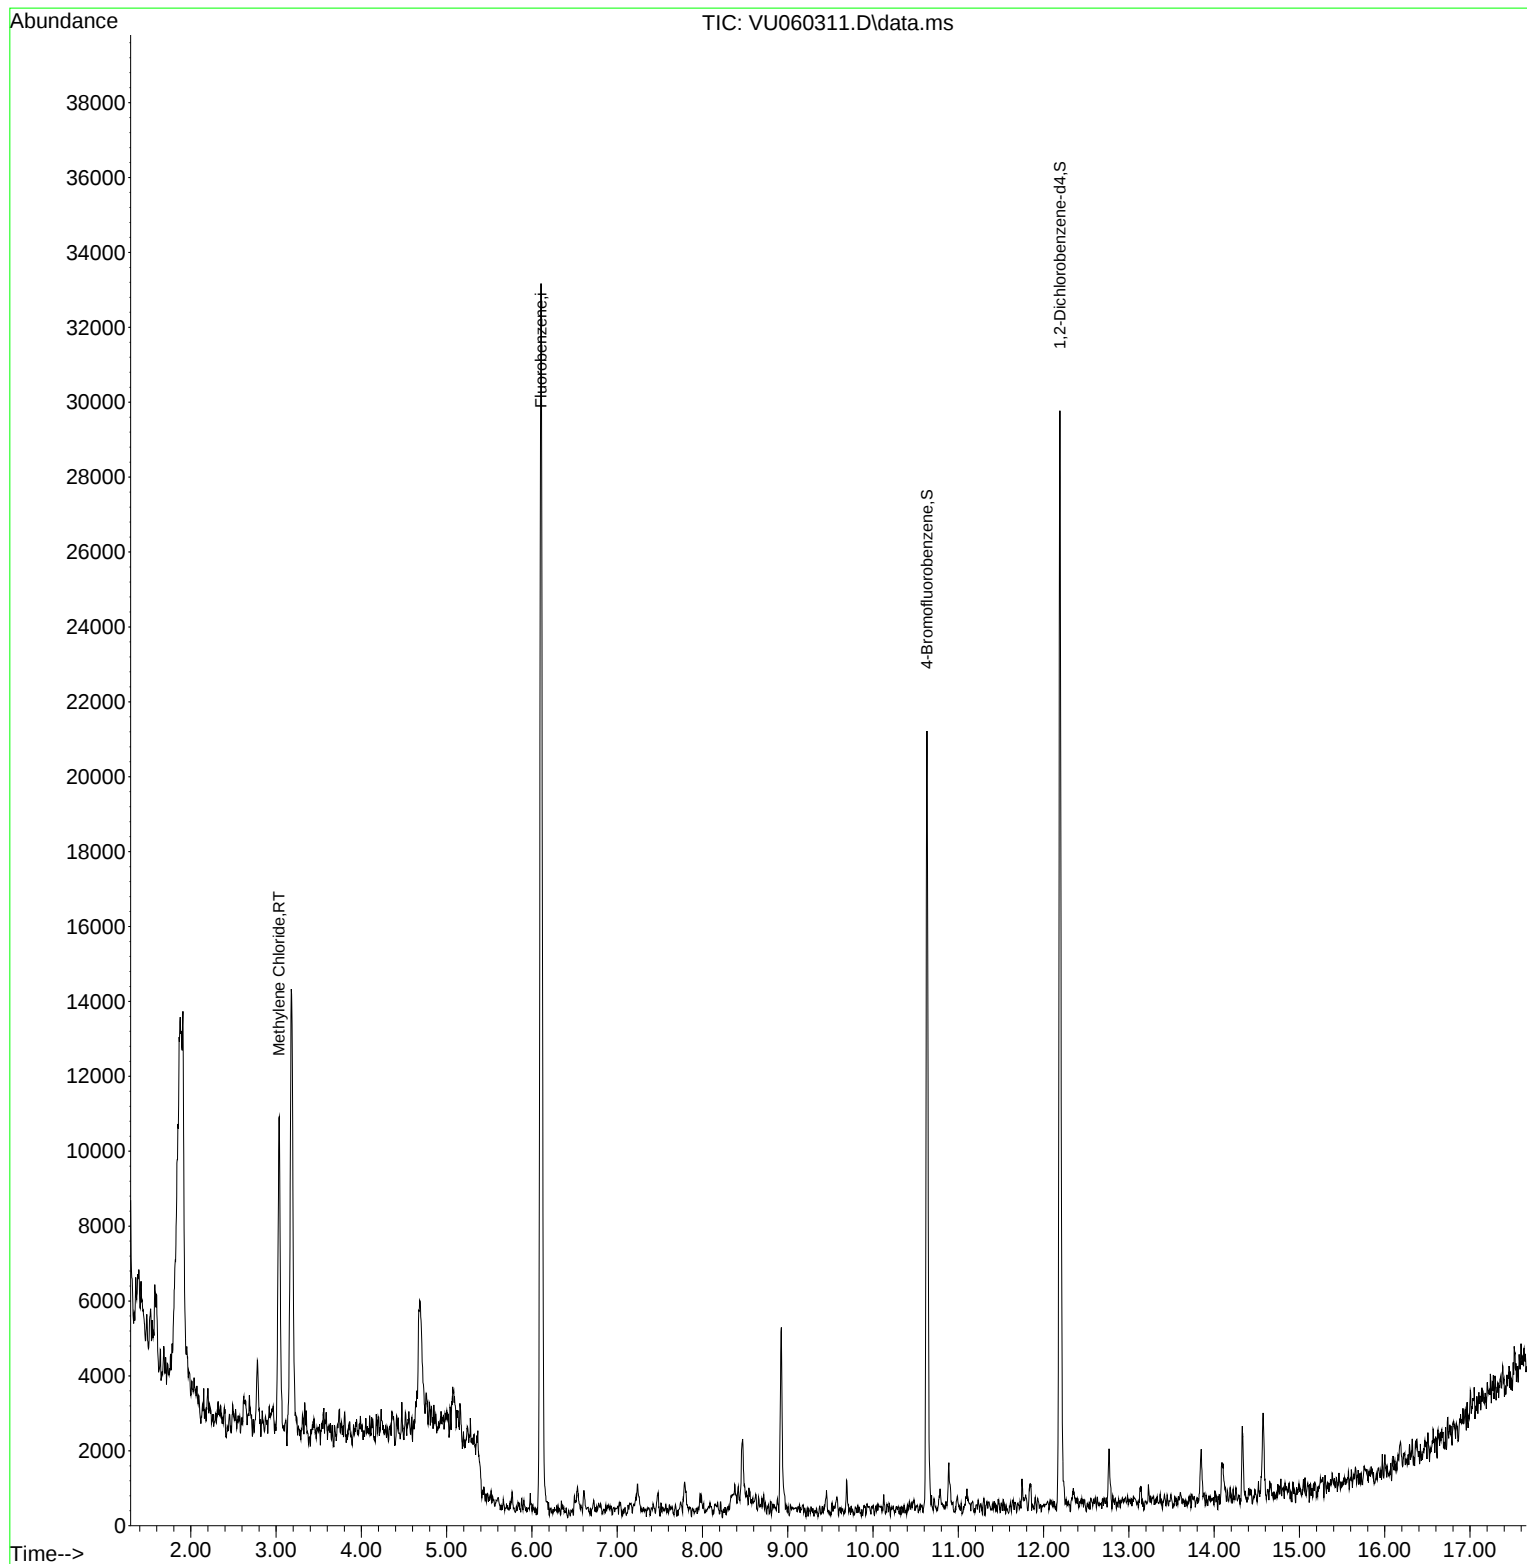


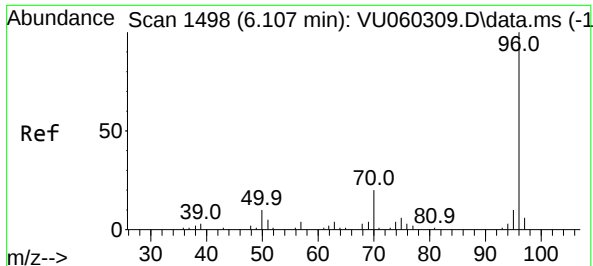

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.107 min Scan# 1498
Delta R.T. -0.000 min
Lab File: VU060311.D
Acq: 05 Aug 2024 14:44




Instrument :
MSVOA_U
ClientSampleId :
VIBLK


Tgt Ion:	96	Resp:	32152
Ion	Ratio	Lower	Upper
96	100		
70	18.6	17.2	25.8
95	10.0	7.9	11.9
97	6.7	0.0	0.0

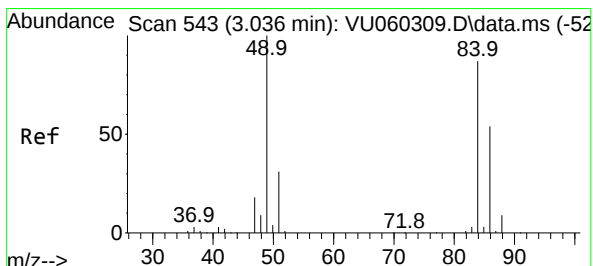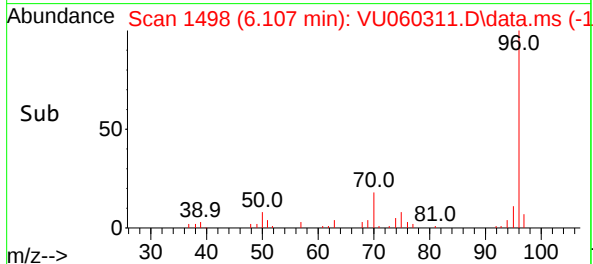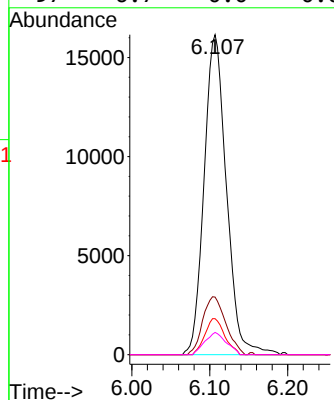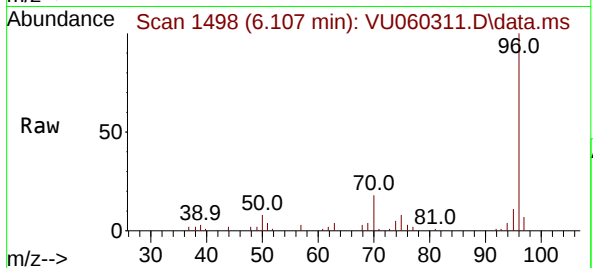

#15
Methylene Chloride
Concen: 0.347 ug/l
RT: 3.033 min Scan# 542
Delta R.T. -0.003 min
Lab File: VU060311.D
Acq: 05 Aug 2024 14:44

Tgt Ion:	84	Resp:	4172
Ion	Ratio	Lower	Upper
84	100		
49	104.9	92.1	138.1
51	29.5	0.0	72.4
86	63.0	50.1	75.1

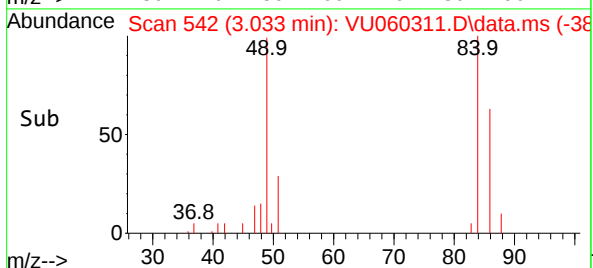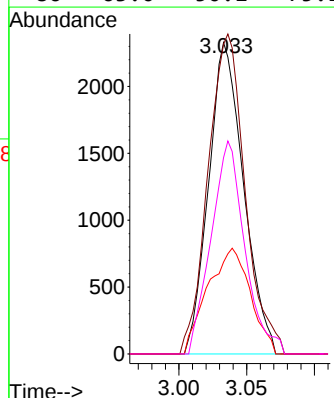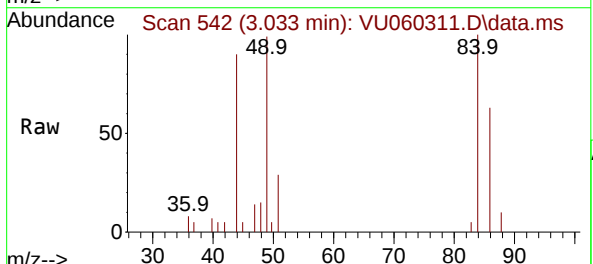

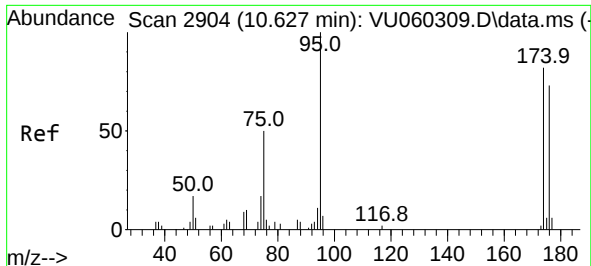

#57

4-Bromofluorobenzene

Concen: 0.700 ug/l

RT: 10.631 min Scan# 2905

Delta R.T. 0.003 min

Lab File: VU060311.D

Acq: 05 Aug 2024 14:44

Instrument :

MSVOA_U

ClientSampleId :

VIBLK





Tgt Ion: 95 Resp: 7665

Ion Ratio Lower Upper

95 100

174 81.5 65.6 98.4

176 82.9 60.4 90.6

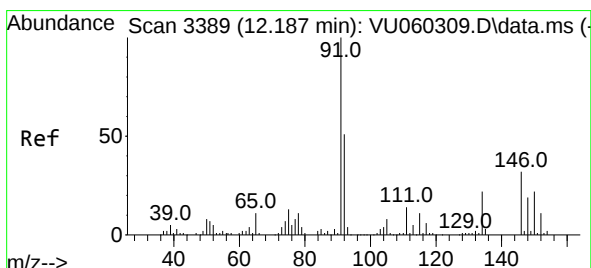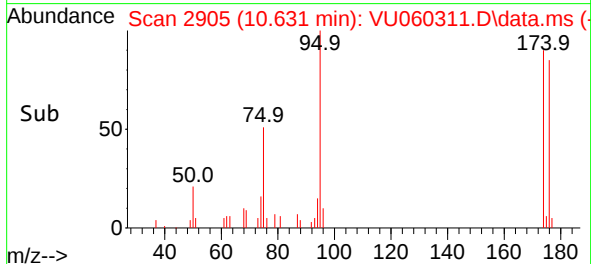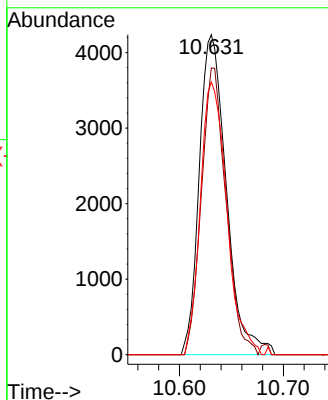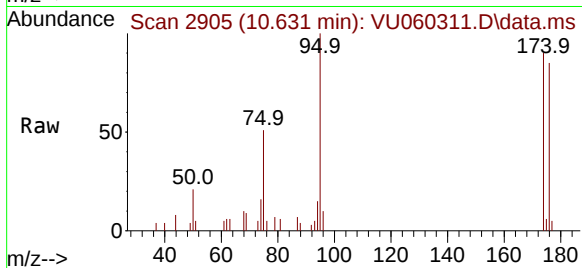

#68

1,2-Dichlorobenzene-d4

Concen: 0.700 ug/l

RT: 12.190 min Scan# 3390

Delta R.T. 0.003 min

Lab File: VU060311.D

Acq: 05 Aug 2024 14:44

Tgt Ion: 152 Resp: 8328

Ion Ratio Lower Upper

152 100

115 68.3 0.0 325.2

150 165.1 0.0 684.2

