

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080524\
 Data File : VU060311.D
 Acq On : 05 Aug 2024 14:44
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU060311.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.779	458	463	469	rBV3	1342	1609	2.51%	0.671%
2	3.036	532	543	556	rVB3	8302	15348	23.95%	6.405%
3	3.178	572	587	601	rBV	11978	27763	43.32%	11.586%
4	3.335	633	636	640	rBV3	846	661	1.03%	0.276%
5	3.538	693	699	702	rBV4	594	790	1.23%	0.330%
6	3.682	742	744	751	rBV3	580	676	1.05%	0.282%
7	3.805	778	782	787	rVB3	815	790	1.23%	0.330%
8	4.358	951	954	958	rBV2	655	718	1.12%	0.300%
9	4.682	1047	1055	1068	rBV4	2639	6831	10.66%	2.851%
10	5.071	1170	1176	1178	rBV6	1151	1290	2.01%	0.538%
11	5.155	1200	1202	1211	rVB5	1213	1383	2.16%	0.577%
12	6.107	1485	1498	1517	rBV	32867	64087	100.00%	26.745%
13	6.534	1626	1631	1641	rVB3	640	1008	1.57%	0.421%
14	6.608	1649	1654	1663	rBV3	595	851	1.33%	0.355%
15	7.480	1915	1925	1927	rBV4	553	766	1.20%	0.320%
16	7.743	1997	2007	2014	rBV2	359	718	1.12%	0.300%
17	7.792	2014	2022	2025	rBV3	823	1228	1.92%	0.512%
18	8.470	2223	2233	2239	rBV4	1647	2796	4.36%	1.167%
19	8.923	2365	2374	2389	rBV2	4955	8403	13.11%	3.507%
20	9.454	2532	2539	2544	rVB3	571	648	1.01%	0.270%
21	9.576	2570	2577	2583	rVB3	507	789	1.23%	0.329%
22	9.689	2606	2612	2618	rBV3	874	929	1.45%	0.388%
23	10.631	2891	2905	2920	rBV	20870	33624	52.47%	14.032%
24	10.785	2944	2953	2959	rBV3	600	922	1.44%	0.385%
25	10.888	2978	2985	2995	rBV3	1149	1613	2.52%	0.673%
26	11.746	3248	3252	3256	rBV4	788	705	1.10%	0.294%
27	12.190	3378	3390	3403	rBV2	29390	47646	74.35%	19.884%
28	12.766	3562	3569	3580	rVB4	1615	2514	3.92%	1.049%
29	13.846	3896	3905	3912	rBV4	1393	2089	3.26%	0.872%
30	14.090	3973	3981	3984	rBV2	1129	1428	2.23%	0.596%
31	14.328	4050	4055	4065	rBV4	2018	2660	4.15%	1.110%
32	14.573	4121	4131	4137	rBV	2160	3357	5.24%	1.401%
33	16.000	4571	4575	4582	rVV4	633	667	1.04%	0.278%
34	16.505	4729	4732	4738	rVB4	783	759	1.18%	0.317%
35	16.740	4800	4805	4808	rBV3	865	840	1.31%	0.351%
36	17.518	5045	5047	5052	rVV4	829	714	1.11%	0.298%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080524\
Data File : VU060311.D
Acq On : 05 Aug 2024 14:44
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER




Sum of corrected areas: 239620

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080524\
Data File : VU060311.D
Acq On : 05 Aug 2024 14:44
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

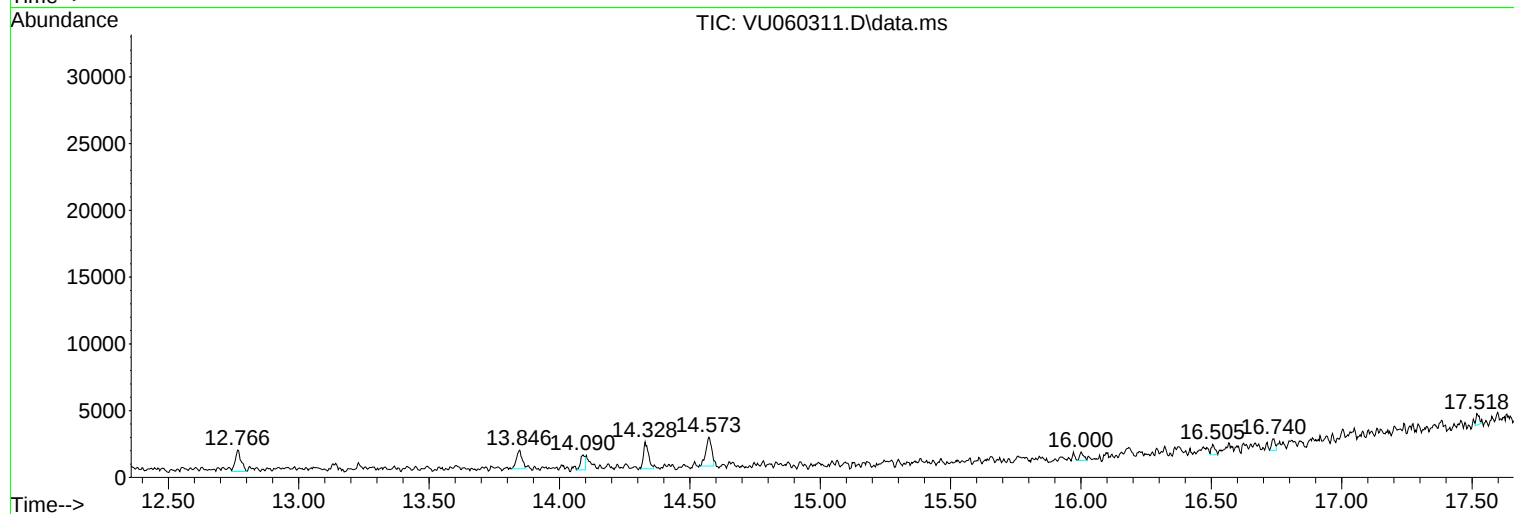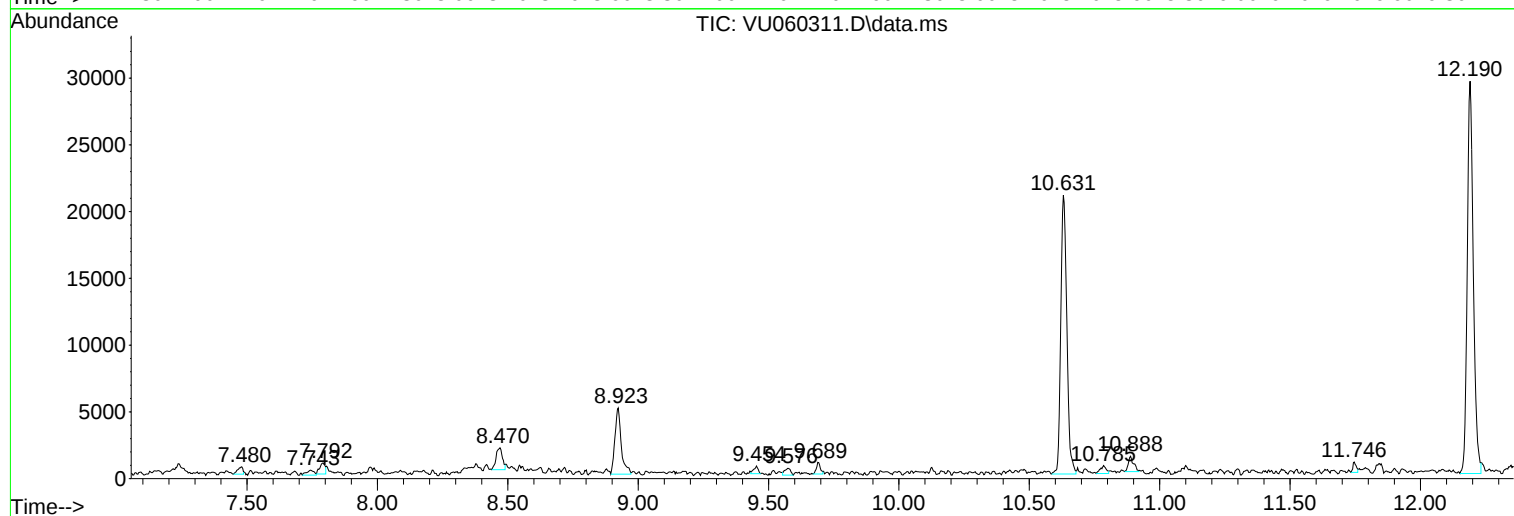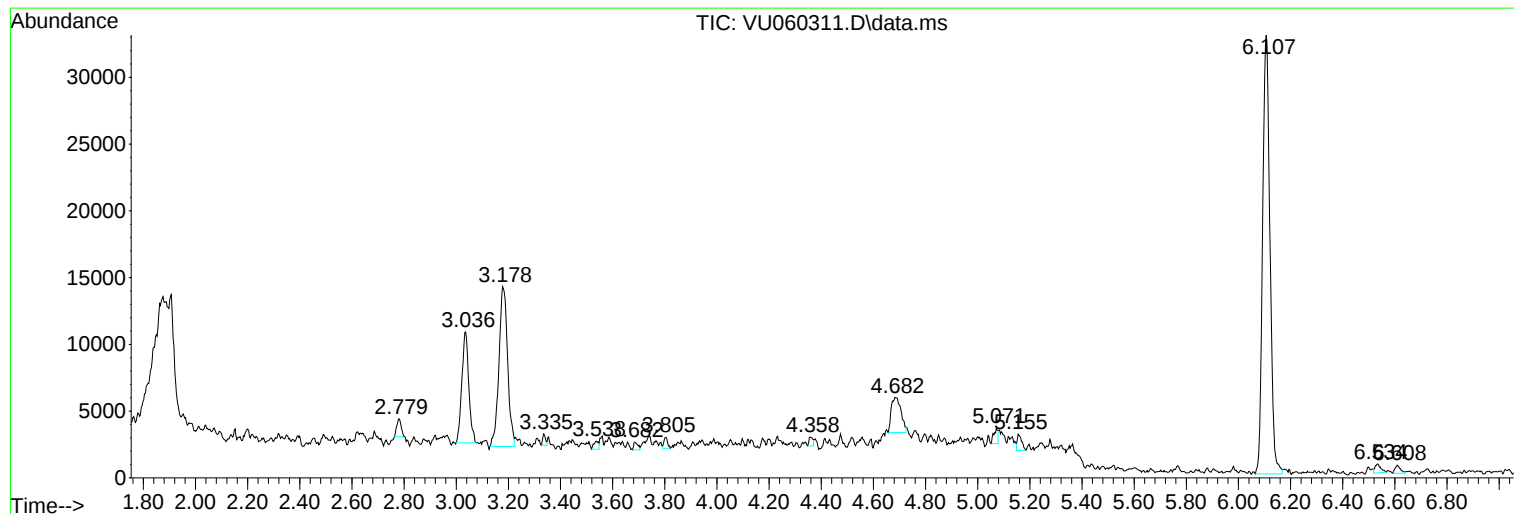

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080524\
Data File : VU060311.D
Acq On : 05 Aug 2024 14:44
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080524\
Data File : VU060311.D
Acq On : 05 Aug 2024 14:44
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc