


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080524\
Data File : VU060304.D
Acq On : 05 Aug 2024 09:32
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U080524DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Aug 06 11:07:28 2024

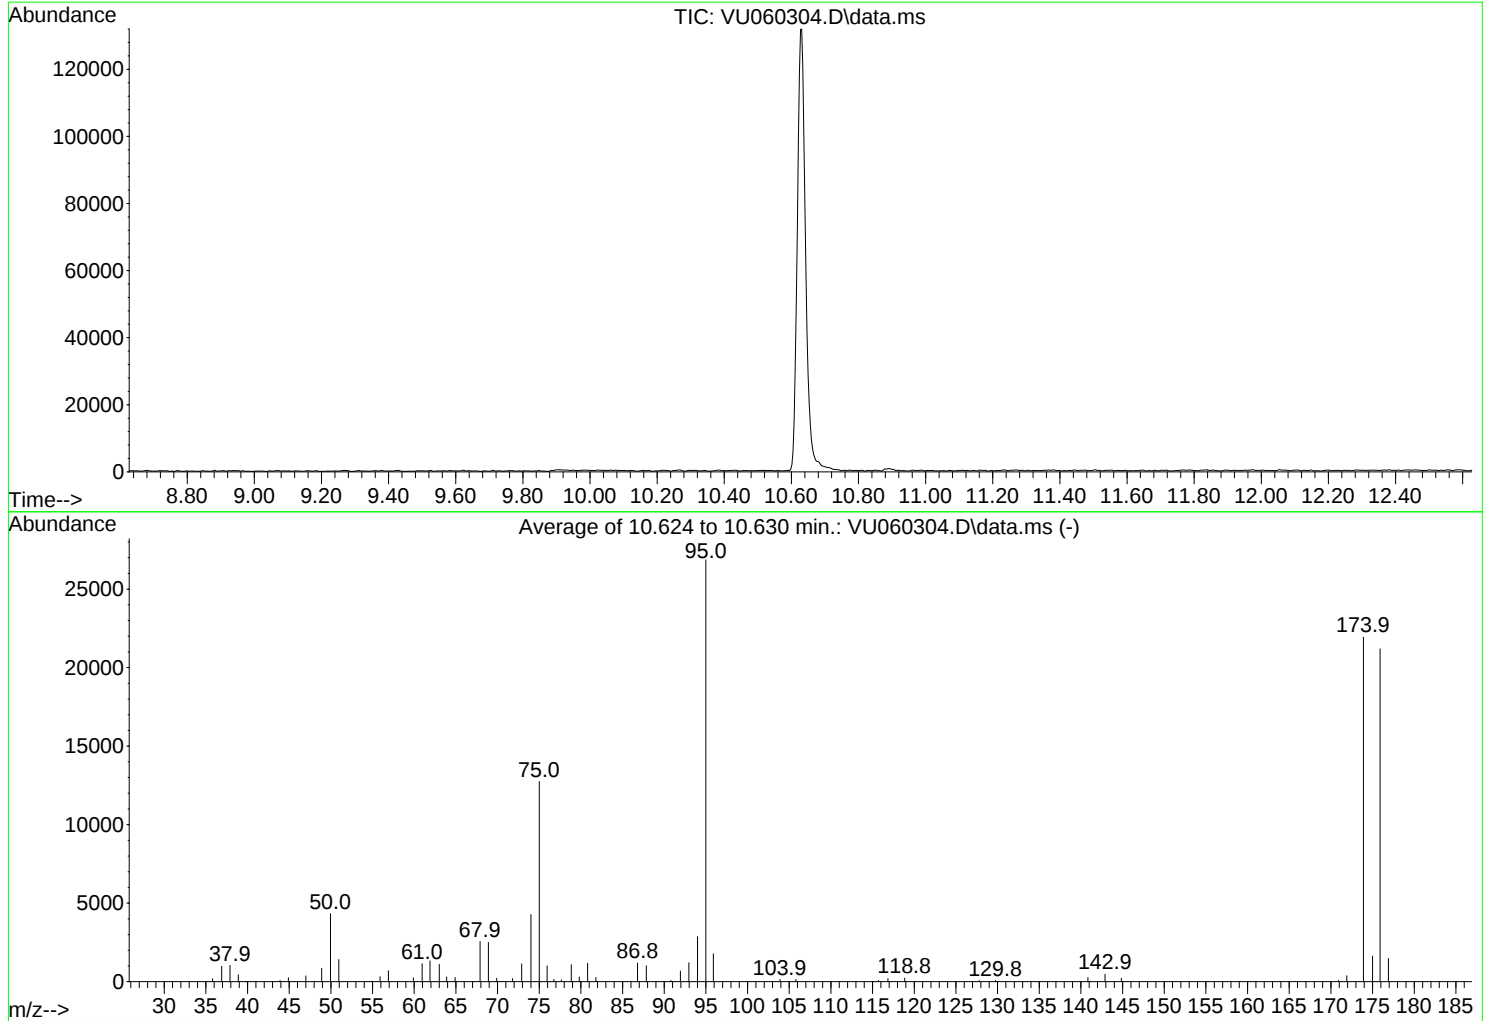

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	4335	PASS
75	95	30	60	47.5	12747	PASS
95	95	100	100	100.0	26864	PASS
96	95	5	9	6.6	1773	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.7	21936	PASS
175	174	5	9	7.4	1630	PASS
176	174	95	101	96.6	21197	PASS
177	176	5	9	7.0	1478	PASS