

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU080618\
 Data File : VU025882.D
 Acq On : 06 Aug 2018 13:46
 Operator : MD/SY
 Sample : J4278-05
 Misc : 7.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EO-03-080118-C

Quant Time: Aug 07 03:55:52 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U072718W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 07 00:49:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.98	168	168984	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	268037	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	273617	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.49	152	176444	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.31	65	138153	52.47	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.94%	
35) Dibromofluoromethane	4.88	113	116799	50.10	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.20%	
50) Toluene-d8	7.57	98	400670	49.11	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.22%	
62) 4-Bromofluorobenzene	10.31	95	161475	51.00	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.00%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.33	50	650	0.266	ug/l #	75
5) Bromomethane	1.60	94	834	0.743	ug/l	82
10) Methyl Iodide	2.38	142	273	8.721	ug/l #	39
11) Tert butyl alcohol	2.83	59	6651	11.538	ug/l #	73
13) Acrolein	2.19	56	19	Below Cal	#	1
16) Acetone	2.35	43	4056	3.160	ug/l	96
18) Methyl Acetate	2.63	43	4147	1.342	ug/l	94
20) Methylene Chloride	2.68	84	5967	2.623	ug/l #	81
25) 2-Butanone	4.30	43	3290	1.883	ug/l	99
29) Tetrahydrofuran	4.67	42	377	0.360	ug/l #	32
31) Cyclohexane	4.97	56	4322	Below Cal	#	33
36) 1,1-Dichloropropene	4.98	75	13107	4.184	ug/l #	49
37) Ethyl Acetate	4.30	43	3290	1.013	ug/l #	69
38) Carbon Tetrachloride	4.98	117	16061	4.527	ug/l #	16
39) Methylcyclohexane	6.41	83	2975	0.829	ug/l	97
55) 1,1,2-Trichloroethane	8.05	97	805	0.341	ug/l #	15
68) m/p-Xylenes	9.38	106	922	0.206	ug/l	76
76) 1,2,3-Trichloropropane	10.31	75	83757	21.545	ug/l #	37
80) 1,3,5-Trimethylbenzene	10.78	105	4881	0.477	ug/l	99
81) trans-1,4-Dichloro-2-buten	10.31	75	83757	54.023	ug/l #	100
84) 1,2,4-Trimethylbenzene	11.16	105	12150	1.172	ug/l	97
85) sec-Butylbenzene	11.33	105	3504	0.282	ug/l	98
86) p-Isopropyltoluene	11.44	119	4500	0.405	ug/l	92
89) n-Butylbenzene	11.89	91	13971	1.363	ug/l #	48
90) Hexachloroethane	12.15	117	1647	0.834	ug/l #	7
93) 1,2,4-Trichlorobenzene	13.51	180	1202	0.295	ug/l #	1
95) Naphthalene	13.75	128	6909	1.765	ug/l #	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080618\
Data File : VU025882.D
Acq On : 06 Aug 2018 13:46
Operator : MD/SY
Sample : J4278-05
Misc : 7.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EO-03-080118-C

Quant Time: Aug 07 03:55:52 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U072718W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 07 00:49:55 2018
Response via : Initial Calibration

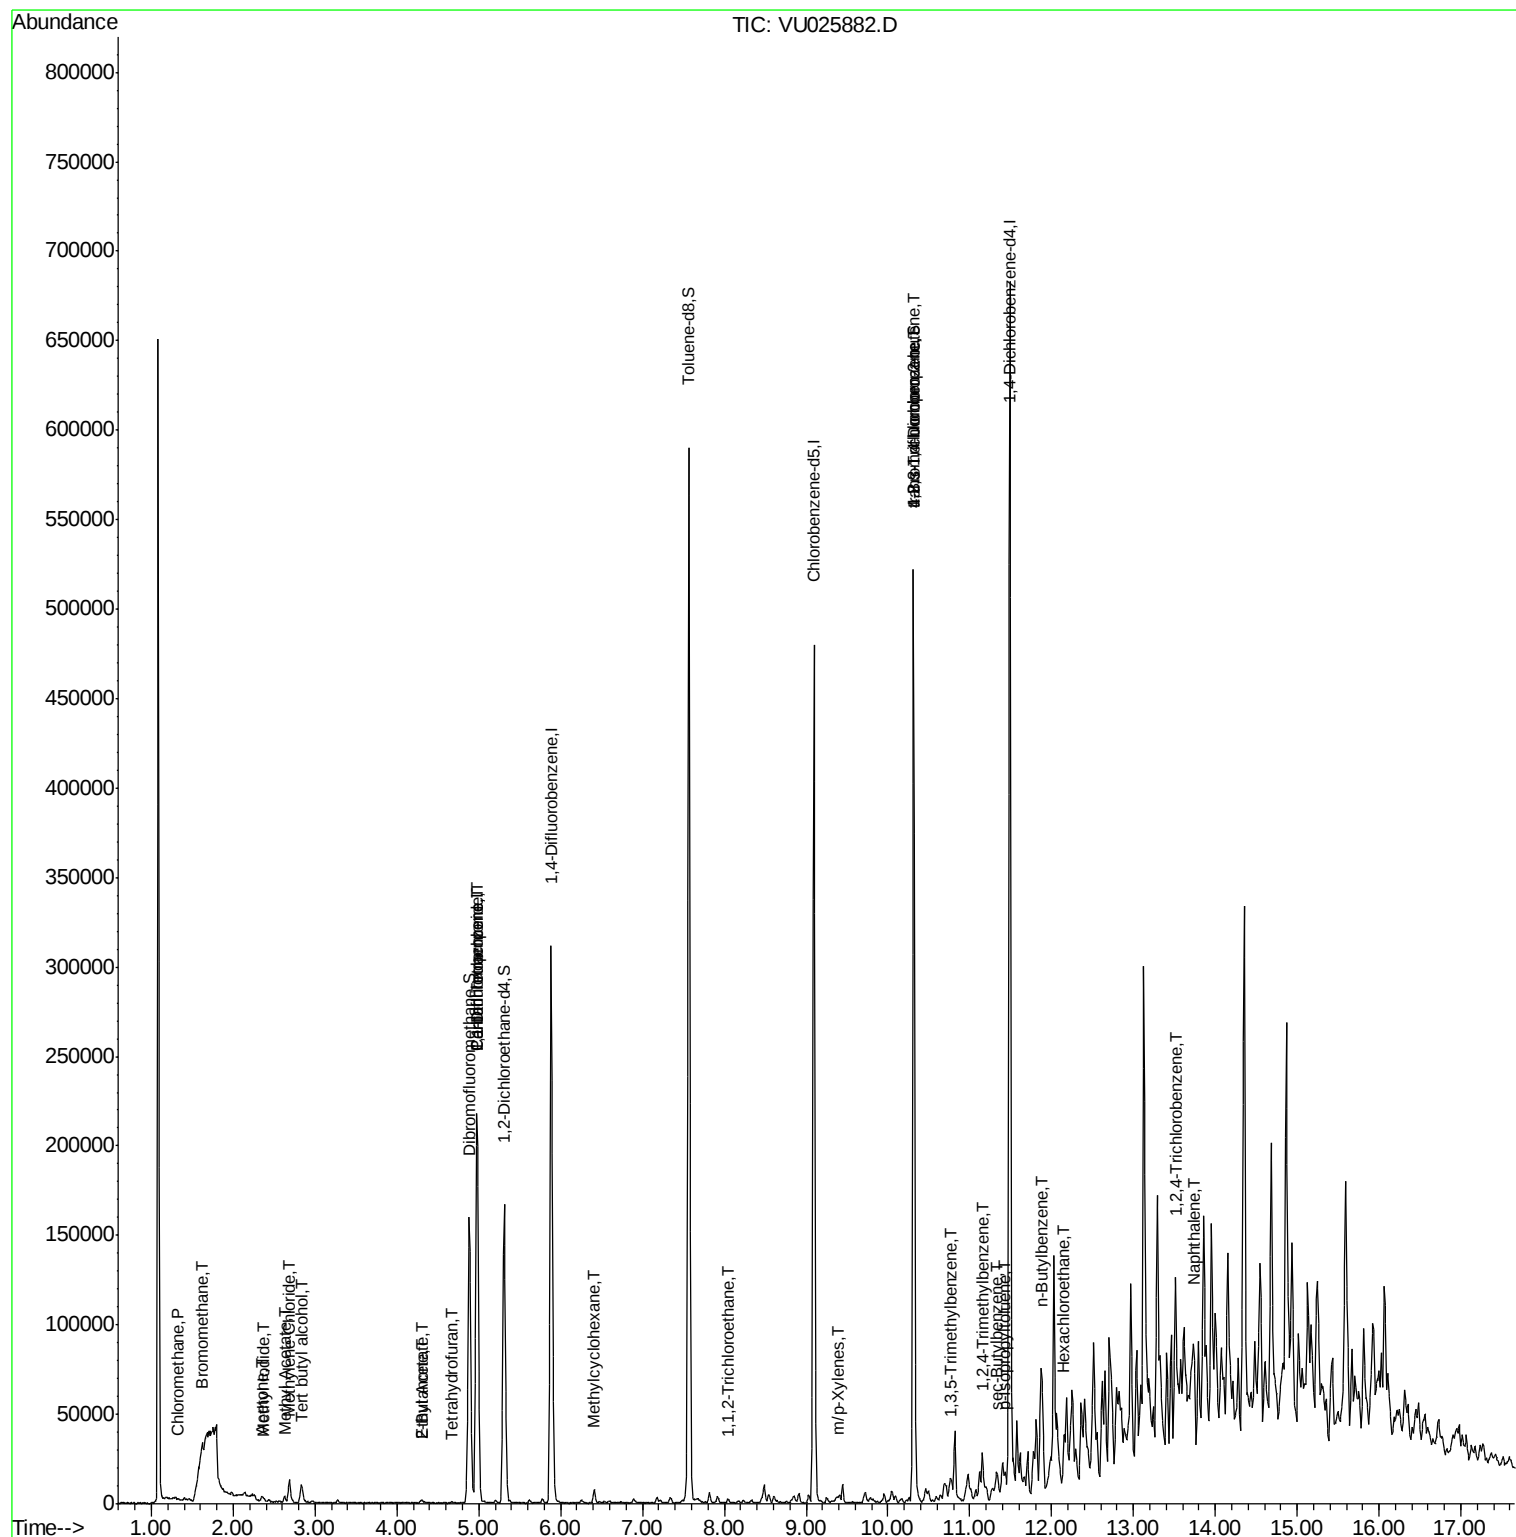

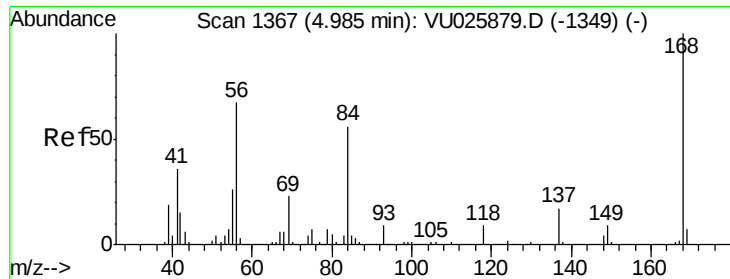

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.98 min Scan# 1365

Delta R.T. -0.01 min

Lab File: VU025882.D

Acq: 06 Aug 2018 13:46

Instrument :

MSVOA_U

ClientSampleId :


EO-03-080118-C

Tgt Ion:168 Resp: 168984

Ion Ratio Lower Upper

168 100

99 54.9 42.8 64.2

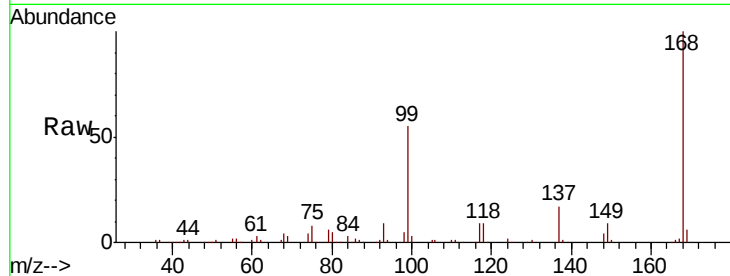

Abundance Ion 167.90 (167.60 to 168.60): VU025879.D (-1349) (-)

Ion 98.90 (98.60 to 99.60): VU025882.D (-1275) (-)

4.98

80000

60000



40000

20000

0

4.90 4.95 5.00 5.05 5.10

Time-->

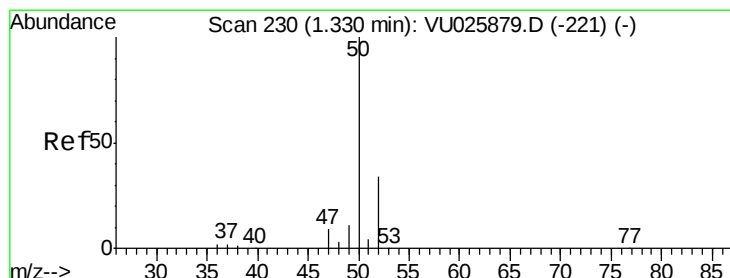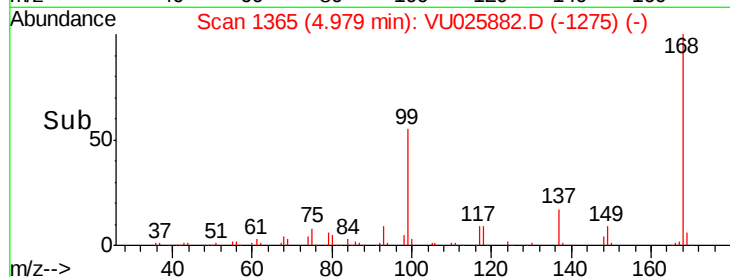

#3

Chloromethane

Concen: 0.266 ug/l

RT: 1.33 min Scan# 229

Delta R.T. -0.00 min

Lab File: VU025882.D


Acq: 06 Aug 2018 13:46

Tgt Ion: 50 Resp: 650

Ion Ratio Lower Upper

50 100

52 18.9 26.5 39.7#

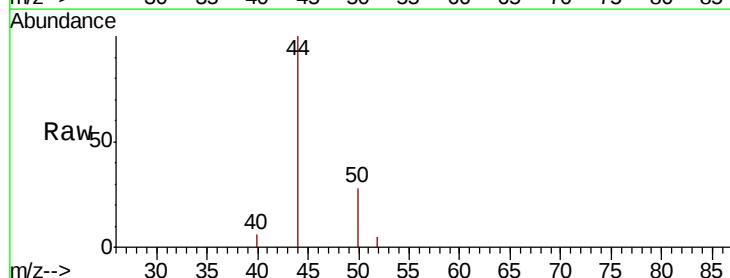

Abundance Ion 49.90 (49.60 to 50.60): VU025879.D (-221) (-)

Ion 51.90 (51.60 to 52.60): VU025882.D (-137) (-)

1.33

600


400


200

0

1.30 1.32 1.34 1.36

Time-->

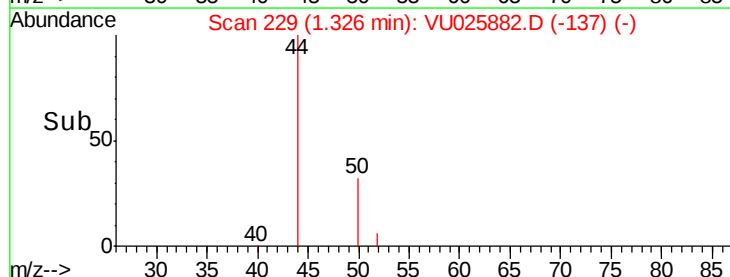



#5

Bromomethane

Concen: 0.743 ug/l

RT: 1.60 min Scan# 315

Delta R.T. -0.02 min

Lab File: VU025882.D

Acq: 06 Aug 2018 13:46

Instrument :

MSVOA_U

ClientSampleId :


EO-03-080118-C

Tgt Ion: 94 Resp: 834

Ion Ratio Lower Upper




94 100

96 76.7 75.0 112.4



Abundance Ion 93.90 (93.60 to 94.60): VU025879.D

Ion 95.90 (95.60 to 96.60): VU025882.D

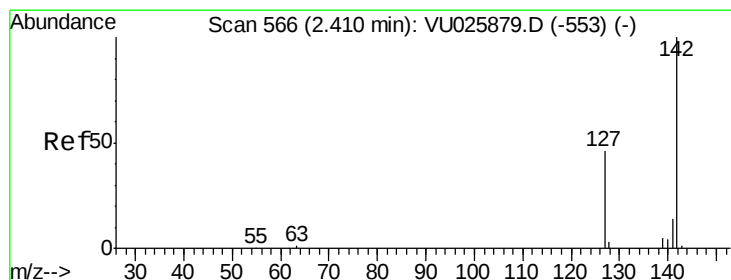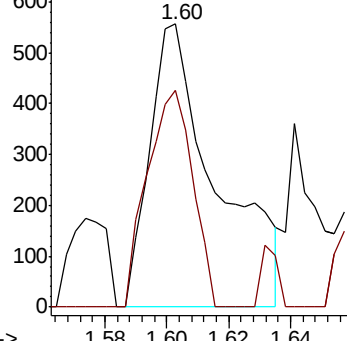

#10

Methyl Iodide

Concen: 8.721 ug/l

RT: 2.38 min Scan# 556

Delta R.T. -0.03 min

Lab File: VU025882.D

Acq: 06 Aug 2018 13:46


Tgt Ion: 142 Resp: 273

Ion Ratio Lower Upper

142 100

127 0.0 36.5 54.7#



141 0.0 11.4 17.2#




Abundance Ion 141.80 (141.50 to 142.50): VU025879.D

Ion 126.80 (126.50 to 127.50): VU025882.D

Ion 140.80 (140.50 to 141.50): VU025882.D




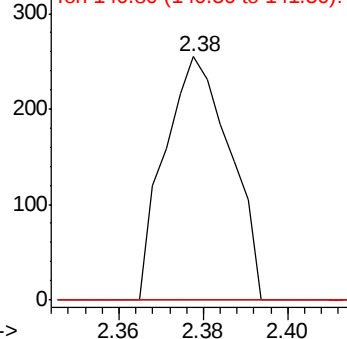




#11
Tert butyl alcohol
Concen: 11.538 ug/l
RT: 2.83 min Scan# 697
Delta R.T. 0.00 min
Lab File: VU025882.D
Acq: 06 Aug 2018 13:46




Instrument :
MSVOA_U
ClientSampleId :
EO-03-080118-C


Tgt Ion: 59 Resp: 6651
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

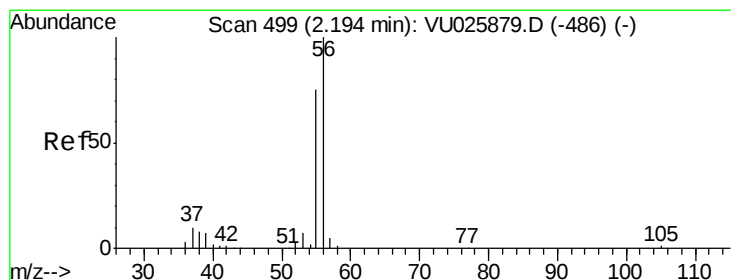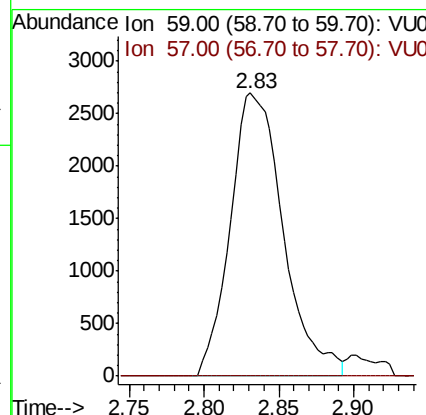

#13
Acrolein
Concen: Below Cal
RT: 2.19 min Scan# 499
Delta R.T. 0.00 min
Lab File: VU025882.D
Acq: 06 Aug 2018 13:46

Tgt Ion: 56 Resp: 19
Ion Ratio Lower Upper
56 100
55 1010.5 57.2 85.8#

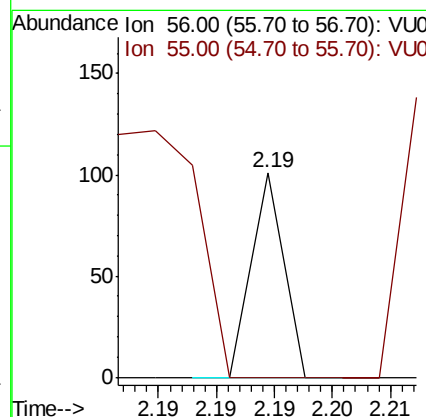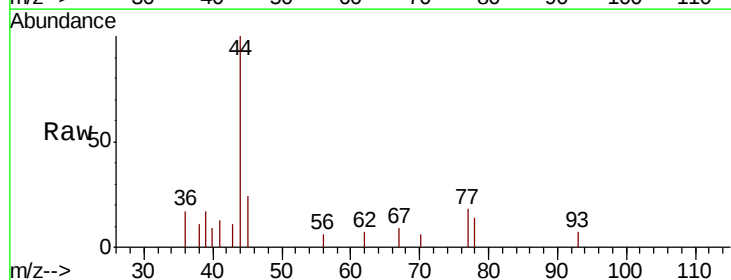

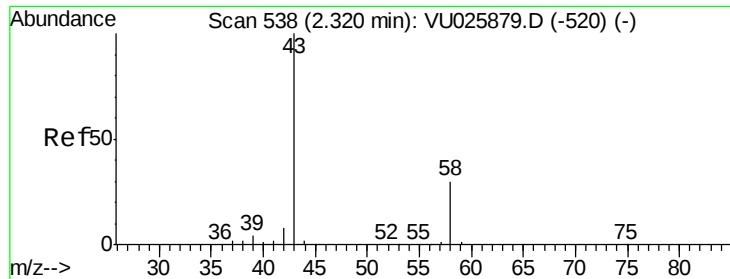

#16

Acetone

Concen: 3.160 ug/l

RT: 2.35 min Scan# 547

Delta R.T. 0.03 min

Lab File: VU025882.D

Acq: 06 Aug 2018 13:46

Instrument :

MSVOA_U

ClientSampleId :


EO-03-080118-C

Tgt Ion: 43 Resp: 4056

Ion Ratio Lower Upper




43 100

58 26.5 23.1 34.7

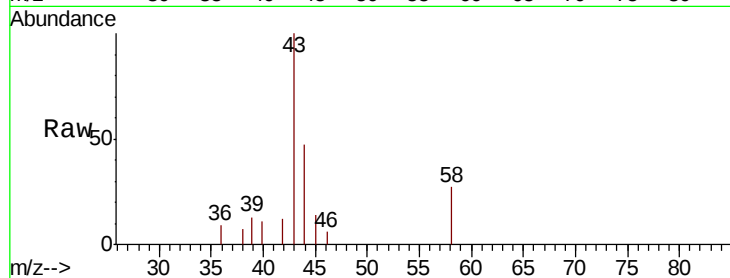

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

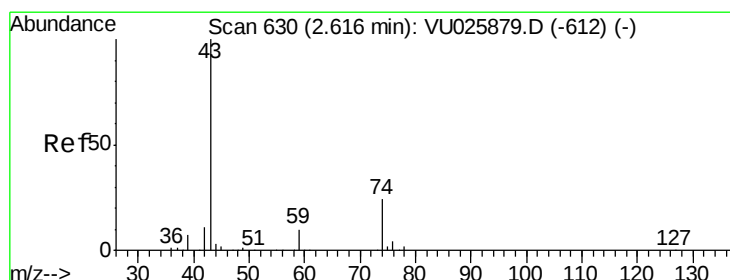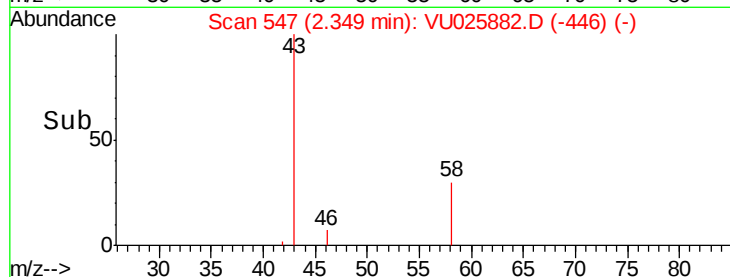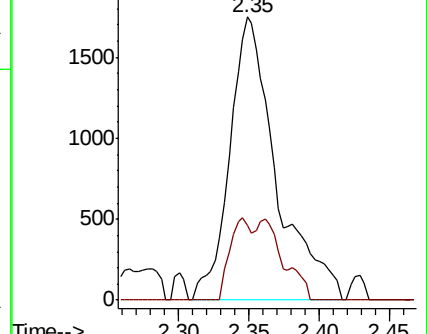

#18

Methyl Acetate

Concen: 1.342 ug/l

RT: 2.63 min Scan# 633

Delta R.T. 0.01 min

Lab File: VU025882.D


Acq: 06 Aug 2018 13:46

Tgt Ion: 43 Resp: 4147

Ion Ratio Lower Upper



43 100


74 19.9 18.5 27.7

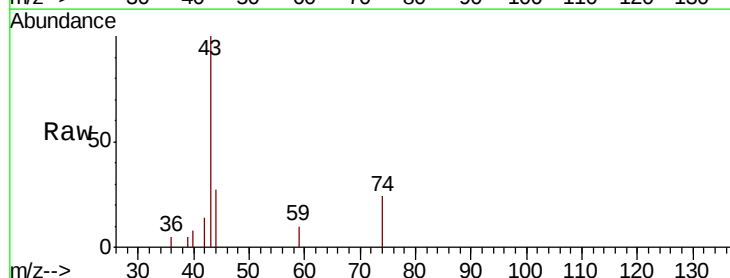

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 74.00 (73.70 to 74.70): VU0

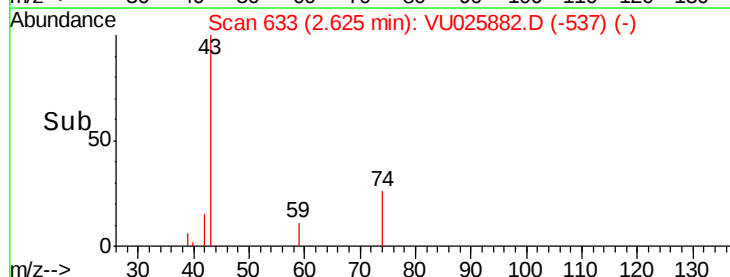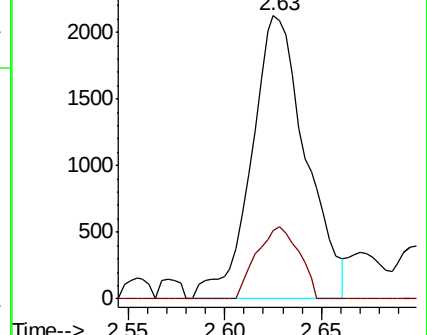



#20

Methylene Chloride

Concen: 2.623 ug/l

RT: 2.68 min Scan# 651

Delta R.T. -0.02 min

Lab File: VU025882.D

Acq: 06 Aug 2018 13:46

Instrument :

MSVOA_U

ClientSampleId :

EO-03-080118-C

Tgt Ion: 84 Resp: 5967


Ion Ratio Lower Upper

84 100

49 99.5 101.8 152.6#

51 31.3 30.8 46.2

86 53.5 51.9 77.9






Abundance Ion 83.90 (83.60 to 84.60): VU0

Ion 48.90 (48.60 to 49.60): VU0

Ion 50.90 (50.60 to 51.60): VU0

Ion 85.90 (85.60 to 86.60): VU0

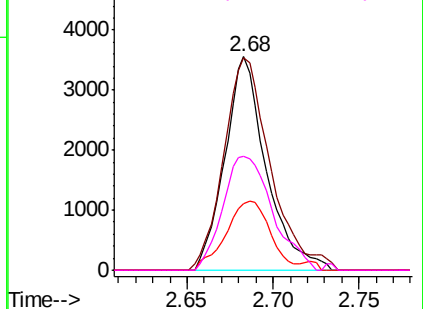

#25

2-Butanone

Concen: 1.883 ug/l

RT: 4.30 min Scan# 1155

Delta R.T. 0.04 min

Lab File: VU025882.D


Acq: 06 Aug 2018 13:46

Tgt Ion: 43 Resp: 3290

Ion Ratio Lower Upper



43 100


72 25.6 21.0 31.4



Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 72.00 (71.70 to 72.70): VU0

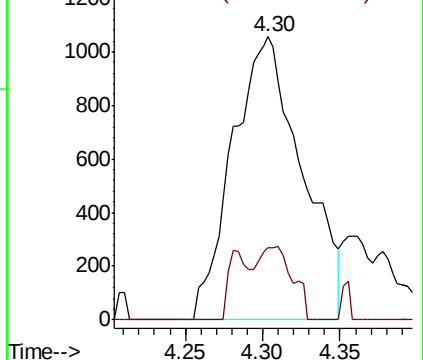







#29
Tetrahydrofuran
Concen: 0.360 ug/l
RT: 4.67 min Scan# 1268
Delta R.T. 0.03 min
Lab File: VU025882.D
Acq: 06 Aug 2018 13:46

Instrument :
MSVOA_U
ClientSampleId :
EO-03-080118-C

Tgt Ion: 42 Resp: 377
Ion Ratio Lower Upper
42 100
72 0.0 36.7 55.1#
71 0.0 33.9 50.9#




Abundance Ion 42.00 (41.70 to 42.70): VU0
Ion 72.00 (71.70 to 72.70): VU0
Ion 71.00 (70.70 to 71.70): VU0


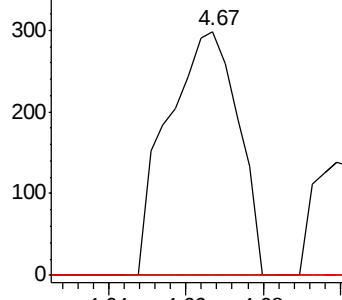



#33
1,2-Dichloroethane-d4
Concen: 52.471 ug/l
RT: 5.31 min Scan# 1468
Delta R.T. -0.00 min
Lab File: VU025882.D
Acq: 06 Aug 2018 13:46

Tgt Ion: 65 Resp: 138153
Ion Ratio Lower Upper
65 100
67 51.6 0.0 103.6



Abundance Ion 64.90 (64.60 to 65.60): VU0
Ion 66.90 (66.60 to 67.60): VU0




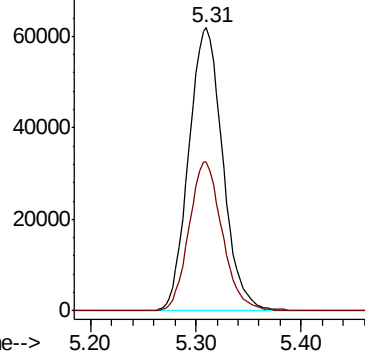




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.89 min Scan# 1647
 Delta R.T. -0.00 min
 Lab File: VU025882.D
 Acq: 06 Aug 2018 13:46




Instrument :
 MSVOA_U
 ClientSampleId :
 EO-03-080118-C


Tgt Ion:	114	Resp:	268037
Ion	Ratio	Lower	Upper
114	100		
63	21.0	0.0	41.6
88	15.6	0.0	32.4

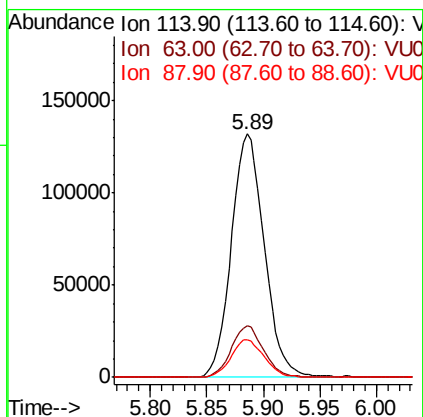

#35
 Dibromofluoromethane
 Concen: 50.101 ug/l
 RT: 4.88 min Scan# 1335
 Delta R.T. -0.01 min
 Lab File: VU025882.D
 Acq: 06 Aug 2018 13:46

Tgt Ion:	113	Resp:	116799
Ion	Ratio	Lower	Upper
113	100		
111	99.7	81.7	122.5
192	20.3	17.1	25.7



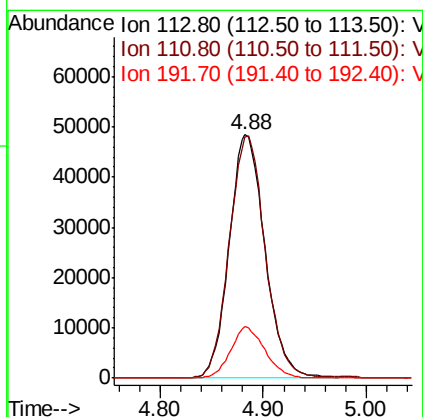





#36
 1,1-Dichloropropene
 Concen: 4.184 ug/l
 RT: 4.98 min Scan# 1364
 Delta R.T. -0.16 min
 Lab File: VU025882.D
 Acq: 06 Aug 2018 13:46




Instrument :
 MSVOA_U
 ClientSampleId :
 EO-03-080118-C


Tgt Ion	Ratio	Lower	Upper
75	100		
110	8.3	17.6	52.9#
77	0.0	24.4	36.6#

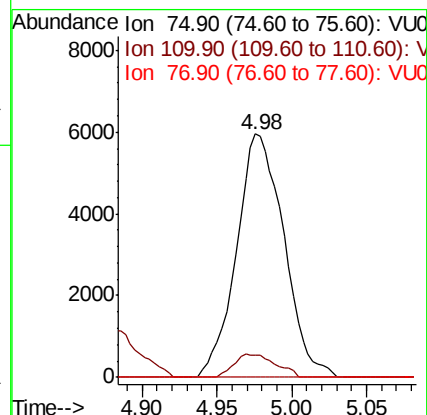

#37
 Ethyl Acetate
 Concen: 1.013 ug/l
 RT: 4.30 min Scan# 1155
 Delta R.T. -0.08 min
 Lab File: VU025882.D
 Acq: 06 Aug 2018 13:46

Tgt Ion	Ratio	Lower	Upper
43	100		
61	0.0	10.7	16.1#
70	0.0	8.4	12.6#

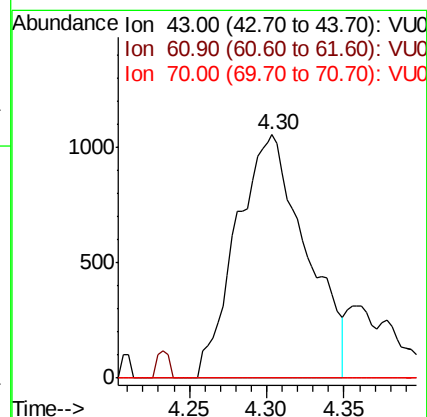



#38

Carbon Tetrachloride

Concen: 4.527 ug/l

RT: 4.98 min Scan# 1364

Delta R.T. -0.16 min

Lab File: VU025882.D

Acq: 06 Aug 2018 13:46

Instrument :

MSVOA_U

ClientSampleId :

EO-03-080118-C


Tgt Ion:117 Resp: 16061

Ion Ratio Lower Upper

117 100

119 4.4 75.7 113.5#




121 0.0 24.6 36.8#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

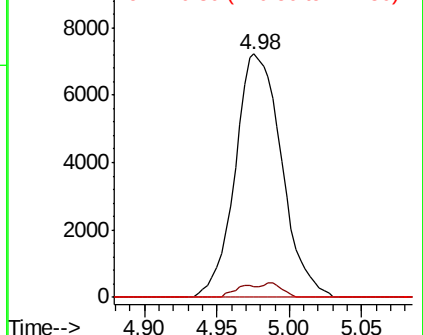

#39

Methylcyclohexane

Concen: 0.829 ug/l

RT: 6.41 min Scan# 1810

Delta R.T. -0.01 min

Lab File: VU025882.D

Acq: 06 Aug 2018 13:46


Tgt Ion: 83 Resp: 2975

Ion Ratio Lower Upper

83 100

55 76.2 60.0 90.0



98 41.7 36.1 54.1




Abundance Ion 83.00 (82.70 to 83.70): VU0

Ion 55.00 (54.70 to 55.70): VU0

Ion 98.00 (97.70 to 98.70): VU0

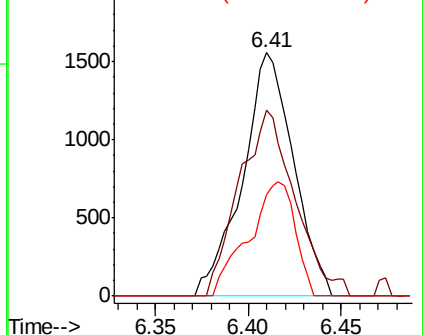



#50

Toluene-d8

Concen: 49.115 ug/l

RT: 7.57 min Scan# 2170

Delta R.T. 0.00 min

Lab File: VU025882.D

Acq: 06 Aug 2018 13:46

Instrument :

MSVOA_U

ClientSampleId :





EO-03-080118-C

Tgt Ion: 98 Resp: 400670

Ion Ratio Lower Upper

98 100

100 63.8 51.1 76.7

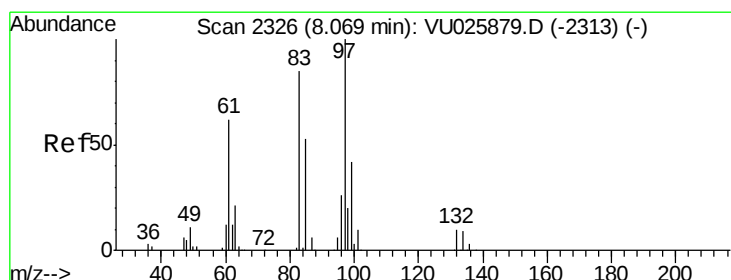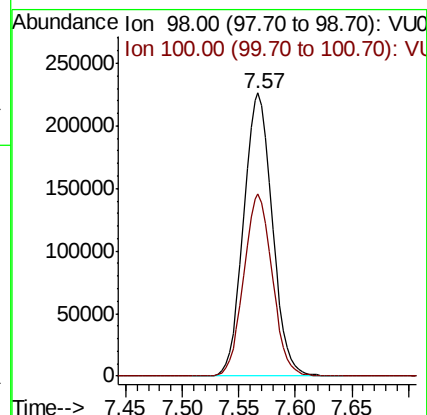

#55

1,1,2-Trichloroethane

Concen: 0.341 ug/l

RT: 8.05 min Scan# 2320

Delta R.T. -0.02 min

Lab File: VU025882.D

Acq: 06 Aug 2018 13:46

Tgt Ion: 97 Resp: 805




Ion Ratio Lower Upper


97 100

83 0.0 68.9 103.3#

85 0.0 44.4 66.6#

99 0.0 51.0 76.4#

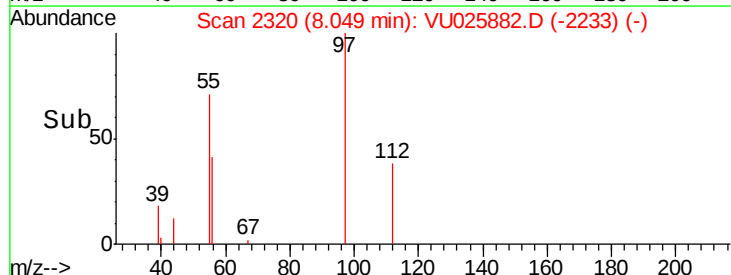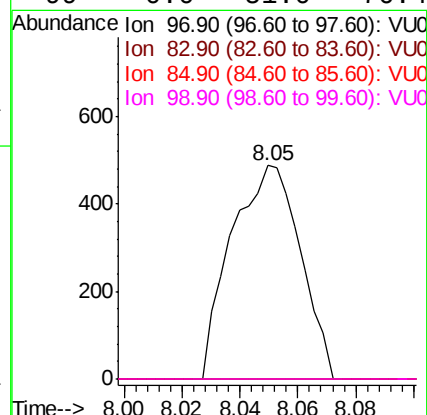

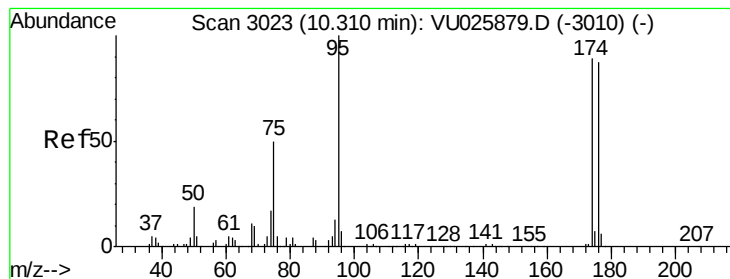

#62

4-Bromofluorobenzene

Concen: 50.996 ug/l

RT: 10.31 min Scan# 3024

Delta R.T. 0.00 min

Lab File: VU025882.D

Acq: 06 Aug 2018 13:46

Instrument :

MSVOA_U

ClientSampleId :

EO-03-080118-C


Tgt Ion: 95 Resp: 161475

Ion Ratio Lower Upper

95 100

174 88.6 0.0 172.2




176 85.9 0.0 162.6

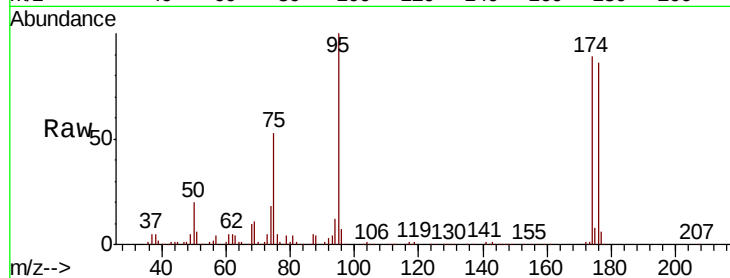

Abundance Ion 94.90 (94.60 to 95.60): VU025879.D (-3010) (-)

Ion 173.80 (173.50 to 174.50): VU025879.D (-3010) (-)

Ion 175.80 (175.50 to 176.50): VU025879.D (-3010) (-)

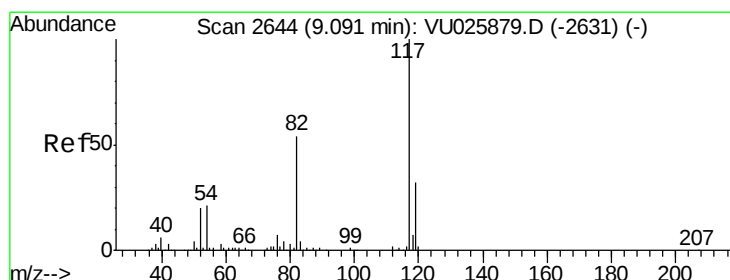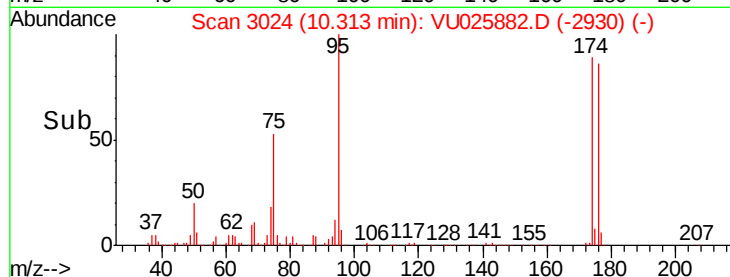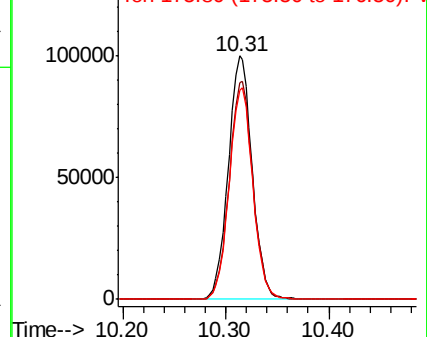

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 9.09 min Scan# 2645

Delta R.T. 0.00 min

Lab File: VU025882.D

Acq: 06 Aug 2018 13:46


Tgt Ion: 117 Resp: 273617

Ion Ratio Lower Upper

117 100

82 54.7 46.0 69.0



119 32.3 26.0 39.0

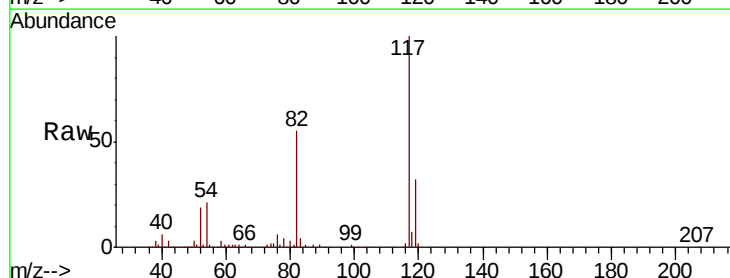


Abundance Ion 116.90 (116.60 to 117.60): VU025879.D (-2631) (-)

Ion 82.00 (81.70 to 82.70): VU025879.D (-2631) (-)

Ion 118.90 (118.60 to 119.60): VU025879.D (-2631) (-)

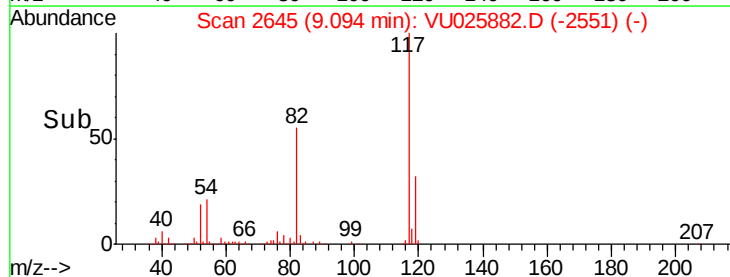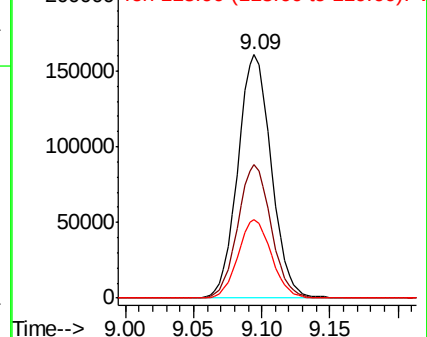







#68
m/p-Xylenes
Concen: 0.206 ug/l
RT: 9.38 min Scan# 2735
Delta R.T. 0.01 min
Lab File: VU025882.D
Acq: 06 Aug 2018 13:46

Instrument :
MSVOA_U
ClientSampleId :
EO-03-080118-C

Tgt Ion:106 Resp: 922
Ion Ratio Lower Upper
106 100
91 240.2 162.3 243.5




Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VU0


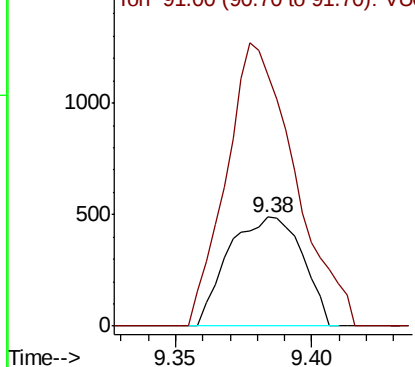



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.49 min Scan# 3390
Delta R.T. 0.00 min
Lab File: VU025882.D
Acq: 06 Aug 2018 13:46

Tgt Ion:152 Resp: 176444
Ion Ratio Lower Upper
152 100
115 57.8 40.1 120.3
150 158.8 0.0 351.4



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V




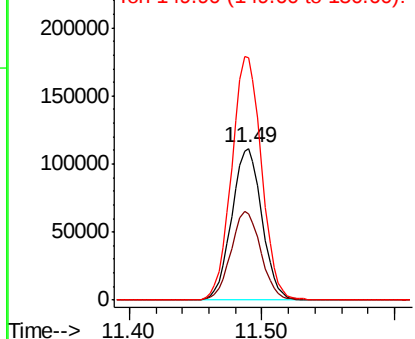




#76
 1,2,3-Trichloropropane
 Concen: 21.545 ug/l
 RT: 10.31 min Scan# 3024
 Delta R.T. -0.18 min
 Lab File: VU025882.D
 Acq: 06 Aug 2018 13:46




Instrument :
 MSVOA_U
 ClientSampleId :
 EO-03-080118-C


Tgt Ion: 75 Resp: 83757
 Ion Ratio Lower Upper
 75 100
 77 1.3 20.4 61.3#

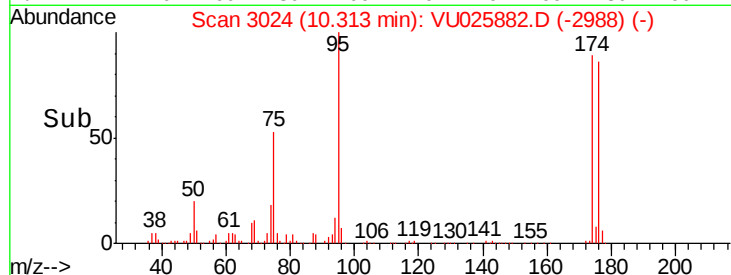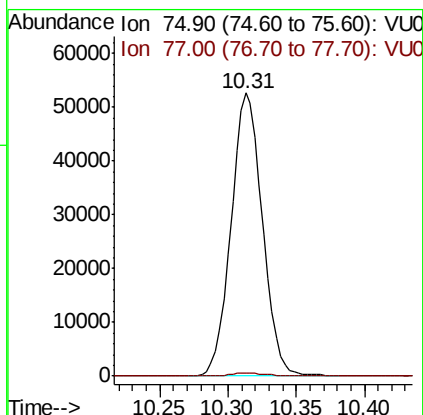

#80
 1,3,5-Trimethylbenzene
 Concen: 0.477 ug/l
 RT: 10.78 min Scan# 3169
 Delta R.T. 0.00 min
 Lab File: VU025882.D
 Acq: 06 Aug 2018 13:46

Tgt Ion: 105 Resp: 4881
 Ion Ratio Lower Upper
 105 100
 120 48.6 24.1 72.2



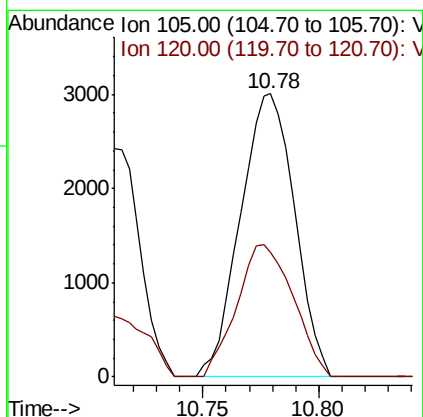





#81
trans-1,4-Dichloro-2-butene
Concen: 54.023 ug/l
RT: 10.31 min Scan# 3024
Delta R.T. -0.18 min
Lab File: VU025882.D
Acq: 06 Aug 2018 13:46




Instrument :
MSVOA_U
ClientSampleId :
EO-03-080118-C


Tgt Ion: 75 Resp: 83757
Ion Ratio Lower Upper
75 100
53 0.2 0.0 0.0#
89 0.0 0.0 0.0

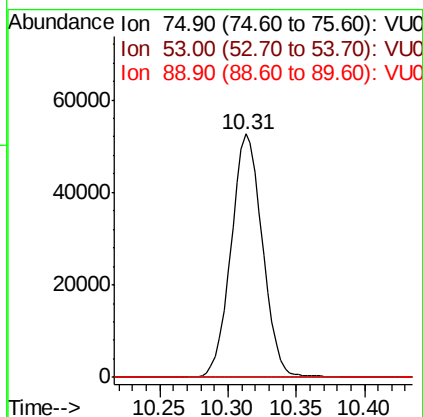

#84
1,2,4-Trimethylbenzene
Concen: 1.172 ug/l
RT: 11.16 min Scan# 3286
Delta R.T. 0.00 min
Lab File: VU025882.D
Acq: 06 Aug 2018 13:46

Tgt Ion: 105 Resp: 12150
Ion Ratio Lower Upper
105 100
120 42.5 22.3 66.8

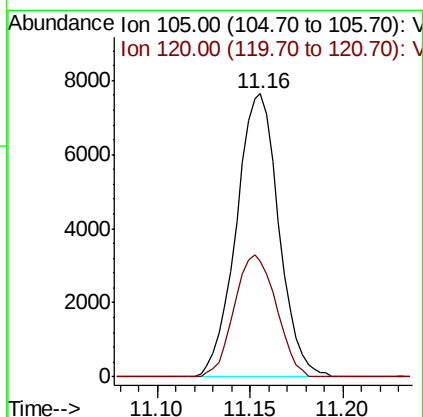



#85

sec-Butylbenzene

Concen: 0.282 ug/l

RT: 11.33 min Scan# 3339

Delta R.T. 0.00 min

Lab File: VU025882.D

Acq: 06 Aug 2018 13:46

Instrument :

MSVOA_U

ClientSampleId :


EO-03-080118-C

Tgt Ion:105 Resp: 3504

Ion Ratio Lower Upper




105 100

134 19.4 10.3 30.8



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 134.00 (133.70 to 134.70): V

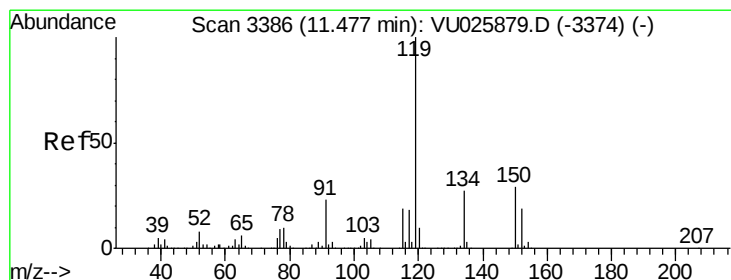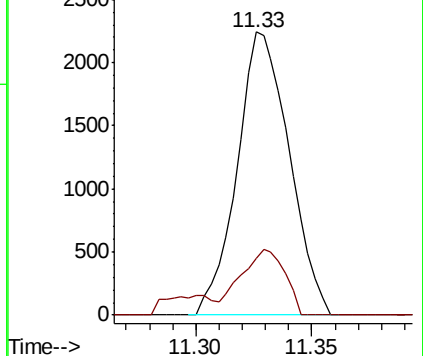

#86

p-Isopropyltoluene

Concen: 0.405 ug/l

RT: 11.44 min Scan# 3373

Delta R.T. -0.04 min

Lab File: VU025882.D

Acq: 06 Aug 2018 13:46


Tgt Ion:119 Resp: 4500

Ion Ratio Lower Upper

119 100

134 25.7 13.2 39.5



91 32.2 12.0 36.1




Abundance Ion 119.00 (118.70 to 119.70): V

Ion 134.00 (133.70 to 134.70): V

Ion 91.00 (90.70 to 91.70): VU0




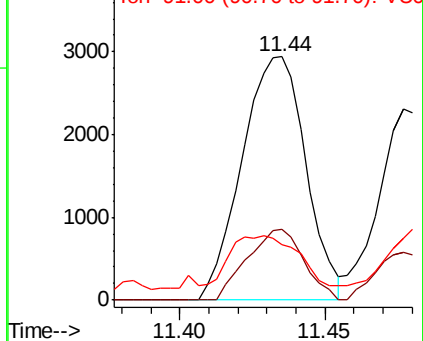




#89
n-Butylbenzene
Concen: 1.363 ug/l
RT: 11.89 min Scan# 3514
Delta R.T. -0.00 min
Lab File: VU025882.D
Acq: 06 Aug 2018 13:46




Instrument :
MSVOA_U
ClientSampleId :
EO-03-080118-C


Tgt Ion: 91 Resp: 13971
Ion Ratio Lower Upper
91 100
92 34.4 26.5 79.5
134 80.3 13.6 40.7#

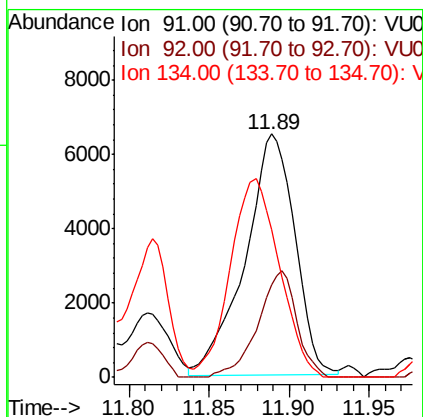

#90
Hexachloroethane
Concen: 0.834 ug/l
RT: 12.15 min Scan# 3594
Delta R.T. -0.00 min
Lab File: VU025882.D
Acq: 06 Aug 2018 13:46

Tgt Ion: 117 Resp: 1647
Ion Ratio Lower Upper
117 100
201 0.0 42.5 127.6#


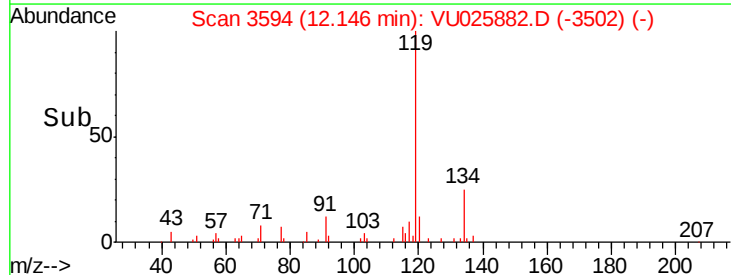
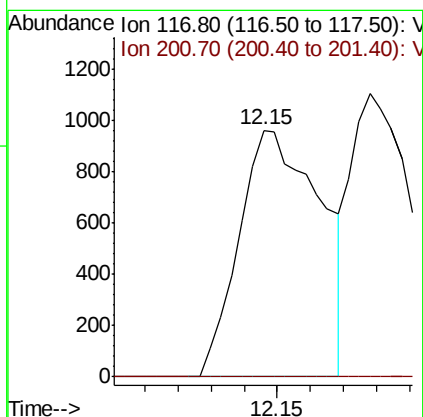



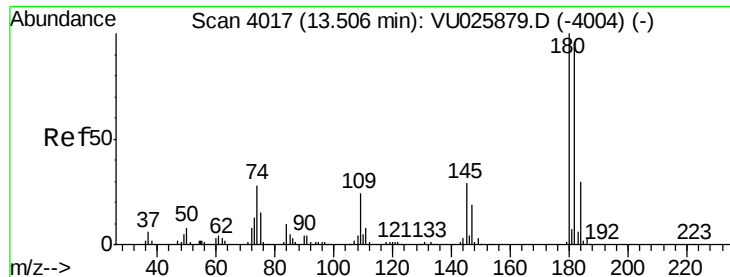

#93
 1,2,4-Trichlorobenzene
 Concen: 0.295 ug/l
 RT: 13.51 min Scan# 4017
 Delta R.T. 0.00 min
 Lab File: VU025882.D
 Acq: 06 Aug 2018 13:46

Instrument :
 MSVOA_U
 ClientSampleId :
 EO-03-080118-C

Tgt Ion:180 Resp: 1202
 Ion Ratio Lower Upper
 180 100
 182 98.5 47.3 141.9
 145 301.5 14.9 44.7#

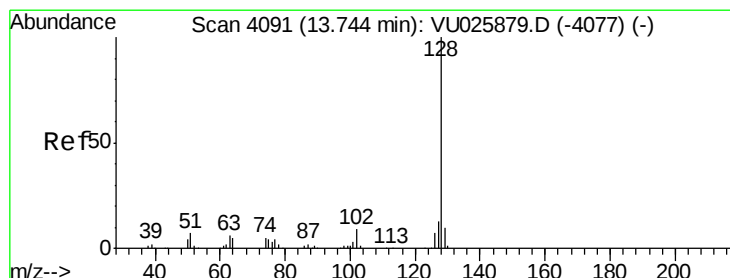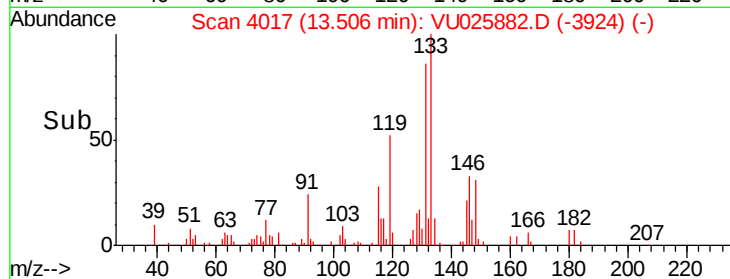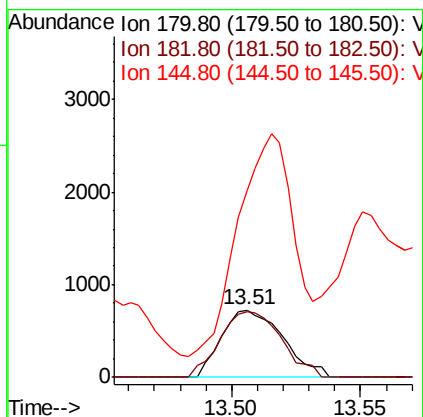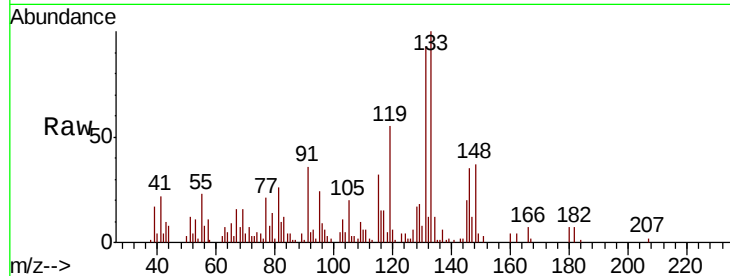

#95
 Naphthalene
 Concen: 1.765 ug/l
 RT: 13.75 min Scan# 4092
 Delta R.T. 0.00 min
 Lab File: VU025882.D
 Acq: 06 Aug 2018 13:46

Tgt Ion:128 Resp: 6909
 Ion Ratio Lower Upper
 128 100
 127 12.5 10.5 15.7
 129 15.4 8.3 12.5#

