


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU080618\
Data File : VU025878.D
Acq On : 06 Aug 2018 11:19
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U072718W.M
Title : SW846 8260
Last Update : Tue Aug 07 00:49:55 2018

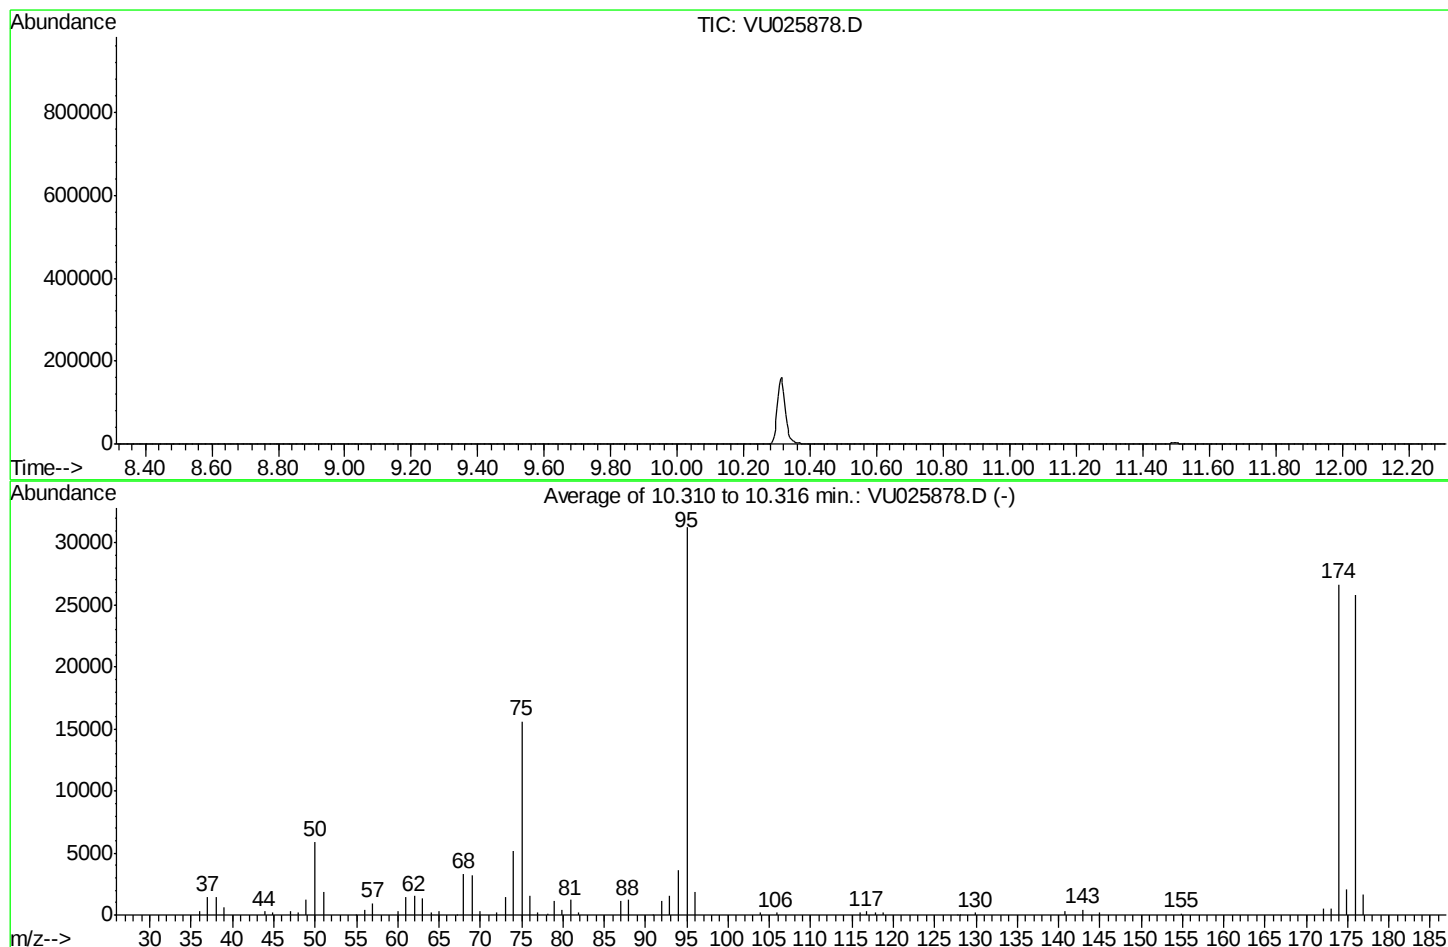

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	5892	PASS
75	95	30	60	49.9	15596	PASS
95	95	100	100	100.0	31264	PASS
96	95	5	9	6.1	1911	PASS
173	174	0.00	2	1.8	492	PASS
174	95	50	100	85.2	26634	PASS
175	174	5	9	7.6	2030	PASS
176	174	95	101	96.8	25770	PASS
177	176	5	9	6.5	1675	PASS