


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080619\
Data File : VU033601.D
Acq On : 06 Aug 2019 08:19
Operator : JC/SP
Sample : BFB48
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB48

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080519WMA.M
Title : VOC Analysis
Last Update : Wed Aug 07 16:40:40 2019

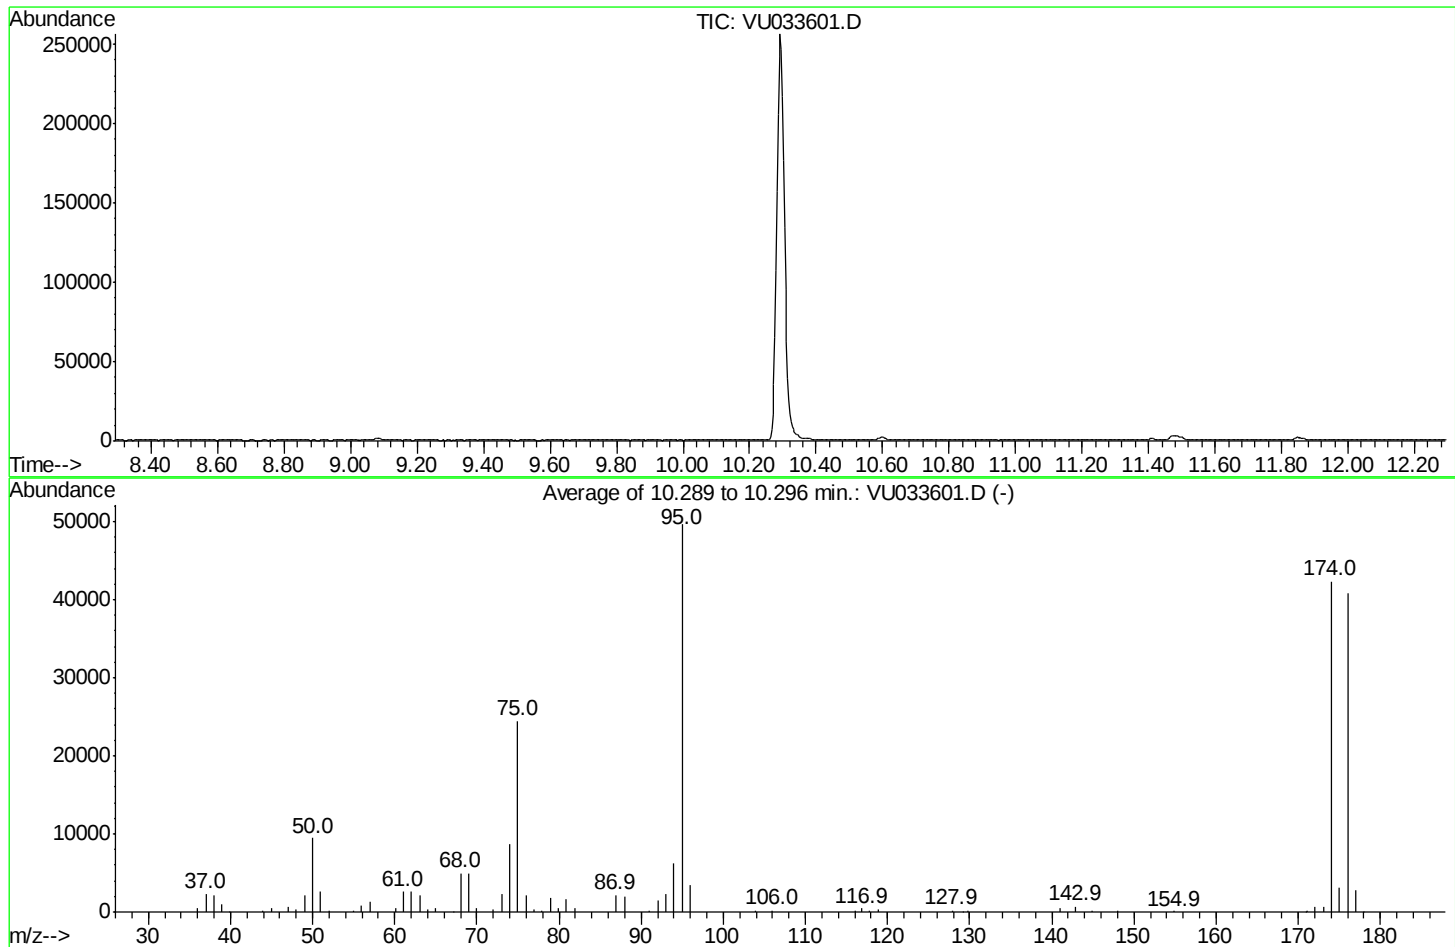

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	9488	PASS
75	95	30	80	49.3	24453	PASS
95	95	100	100	100.0	49645	PASS
96	95	5	9	7.1	3511	PASS
173	174	0.00	2	1.5	631	PASS
174	95	50	120	85.3	42325	PASS
175	174	5	9	7.3	3108	PASS
176	174	95	101	96.3	40778	PASS
177	176	5	9	6.7	2718	PASS

Scan 2850 (10.254 min): VU033601.D
BFB48

m/z	Abundance
40.00	205.0
44.00	394.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.00	496.0
37.00	2448.0
38.00	2002.0
39.00	1004.0
39.90	235.0
43.90	713.0
45.00	518.0
47.00	523.0
48.00	323.0
49.00	2050.0
50.00	9679.0
51.00	2474.0
51.90	148.0
55.00	168.0
55.90	788.0
57.00	1386.0
60.10	428.0
61.00	2444.0
62.00	2642.0
63.10	2195.0
64.00	346.0
65.00	407.0
67.10	115.0
68.00	4891.0
69.00	4826.0
69.90	451.0
72.00	272.0
73.00	2208.0
74.00	8642.0
75.00	24112.0
76.00	2004.0
76.90	297.0
77.90	225.0
78.90	1828.0
79.90	475.0
80.90	1740.0
81.90	483.0
86.90	2055.0
87.90	1949.0
90.90	231.0
92.00	1519.0
93.00	2229.0
94.00	6135.0
95.00	48160.0
96.00	3532.0
103.90	193.0
106.00	249.0
116.00	209.0
116.90	422.0
117.90	180.0
118.90	327.0
127.90	217.0
129.80	156.0
141.00	471.0
142.90	668.0
144.90	227.0
147.90	157.0
154.90	134.0
170.90	115.0
172.00	672.0
173.10	668.0
174.00	39944.0
174.90	2970.0
176.00	39208.0
177.00	2550.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.00	458.0
37.00	2431.0
38.00	2075.0
39.00	989.0
39.90	224.0
43.90	609.0
45.00	559.0
47.00	645.0
48.00	382.0
49.00	2238.0
50.00	9878.0
51.00	2597.0
52.00	195.0
55.00	187.0
55.90	785.0
57.00	1407.0
60.10	454.0
61.00	2650.0
62.00	2684.0
63.00	2173.0
64.00	318.0
65.00	510.0
68.00	5156.0
69.00	5048.0
69.90	469.0
71.90	254.0
73.10	2429.0
74.00	8962.0
75.00	25240.0
76.00	2193.0
76.90	339.0
77.90	208.0
78.90	1897.0
79.90	521.0
80.90	1734.0
81.90	463.0
86.90	2376.0
88.00	2101.0
90.90	203.0
92.00	1516.0
93.00	2373.0
94.00	6434.0
95.00	51288.0
96.00	3611.0
104.00	221.0
106.00	253.0
116.00	198.0
116.90	435.0
117.90	216.0
118.90	310.0
127.90	242.0
129.20	100.0
129.90	142.0
140.90	464.0
142.90	690.0
144.90	237.0
148.00	183.0
154.90	176.0
171.10	142.0
172.00	771.0
173.00	629.0
174.00	43664.0
174.90	3152.0
176.00	42024.0
177.00	2840.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.00	384.0
37.00	2100.0
38.00	2095.0
39.00	869.0
39.90	208.0
44.00	542.0
45.00	489.0
47.00	590.0
48.00	366.0
49.00	2154.0
50.10	8909.0
51.00	2625.0
52.00	203.0
55.00	163.0
55.90	774.0
57.00	1282.0
60.00	420.0
61.00	2638.0
62.00	2448.0
63.00	1955.0
64.00	291.0
65.00	532.0
68.00	4866.0
69.00	4893.0
69.90	420.0
71.90	274.0
73.10	2315.0
74.00	8290.0
75.00	24008.0
76.00	2250.0
77.00	358.0
77.90	200.0
78.90	1728.0
79.90	555.0
80.90	1612.0
81.90	364.0
86.90	2205.0
88.00	2063.0
90.90	176.0
92.00	1325.0
93.00	2275.0
94.00	5962.0
95.00	49488.0
96.00	3390.0
104.00	217.0
106.00	246.0
116.00	172.0
116.90	397.0
117.80	213.0
118.90	273.0
127.90	257.0
129.20	100.0
129.90	114.0
140.90	454.0
142.90	636.0
145.00	244.0
148.00	175.0
154.90	168.0
171.10	151.0
172.00	773.0
173.00	597.0
174.00	43368.0
175.00	3204.0
176.00	41104.0
177.00	2766.0
177.90	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48