

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080620\
 Data File : VU039768.D
 Acq On : 06 Aug 2020 19:50
 Operator : SY/MD
 Sample : L3578-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 07 04:31:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 07 04:28:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	111210	5.00	ug/L	0.02
28) Chlorobenzene-d5	9.43	117	105835	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	48652	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.58	65	442525	73.69	ug/L	-0.02
Spiked Amount	5.000	Range	40 - 130	Recovery	=	1473.80%#
7) Chloroethane-d5	1.92	69	21248	3.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	65.40%
11) 1,1-Dichloroethene-d2	2.59	63	437104	36.14	ug/L	0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	722.80%#
20) 2-Butanone-d5	4.93	46	460	0.17	ug/L	0.27
Spiked Amount	50.000	Range	40 - 130	Recovery	=	0.34%#
24) Chloroform-d	5.14	84	52743	3.52	ug/L	0.06
Spiked Amount	5.000	Range	70 - 125	Recovery	=	70.40%
26) 1,2-Dichloroethane-d4	5.74	65	39481	4.42	ug/L	0.03
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.40%
32) Benzene-d6	5.77	84	118445	4.71	ug/L	0.03
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
36) 1,2-Dichloropropane-d6	6.72	67	41387	4.80	ug/L	0.02
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.00%
41) Toluene-d8	7.92	98	103358	4.63	ug/L	0.01
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.60%
43) trans-1,3-Dichloropropene-	8.20	79	17273	5.22	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	104.40%
46) 2-Hexanone-d5	8.65	63	90680	50.69	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.38%
57) 1,1,2,2-Tetrachloroethane-	10.76	84	38348	4.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	40873	4.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.20%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	1.40	85	914	0.102	ug/L	94
3) Chloromethane	1.58	50	442975	46.970	ug/L #	45
8) Chloroethane	1.95	64	6735	1.016	ug/L #	52
9) Trichlorofluoromethane	2.38	101	14511	1.032	ug/L	99
10) 1,1,2-Trichloro-1,2,2-trif	2.59	101	905474	118.665	ug/L	96
12) 1,1-Dichloroethene	2.60	96	737259	111.136	ug/L #	77
13) Acetone	2.59	43	10773	6.919	ug/L	58
14) Carbon disulfide	2.82	76	174442	8.410	ug/L	99
16) Methylene chloride	3.07	84	30006	2.806	ug/L	93
18) trans-1,2-Dichloroethene	3.38	96	14891021	2016.220	ug/L	79
19) 1,1-Dichloroethane	3.92	63	34922	2.561	ug/L	98
25) Chloroform	5.17	83	61643	4.206	ug/L	95
27) 1,2-Dichloroethane	5.82	62	1997	0.198	ug/L #	71
33) Benzene	5.82	78	183563	6.366	ug/L	100
34) Trichloroethene	6.57	95	448248	59.855	ug/L	97
35) Methylcyclohexane	6.72	83	9694	0.811	ug/L #	20
37) 1,2-Dichloropropane	6.72	63	5679	0.741	ug/L #	86

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080620\
 Data File : VU039768.D
 Acq On : 06 Aug 2020 19:50
 Operator : SY/MD
 Sample : L3578-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 07 04:31:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 07 04:28:48 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
39) cis-1,3-Dichloropropene	7.58	75	1670	0.160	ug/L	98
40) 4-Methyl-2-pentanone	7.81	43	32648	5.704	ug/L	98
42) Toluene	8.00	91	12581428	415.189	ug/L	99
44) trans-1,3-Dichloropropene	8.00	75	105647	11.227	ug/L #	1
51) Chlorobenzene	9.46	112	27365	1.344	ug/L	97
52) Ethylbenzene	9.58	91	1521379	44.858	ug/L	97
53) m,p-Xylene	9.70	106	1618612	125.324	ug/L	90
54) o-Xylene	10.10	106	423450	33.483	ug/L	89
55) Styrene	10.10	104	22147	1.040	ug/L #	1
56) Isopropylbenzene	10.48	105	3469	0.103	ug/L	96
59) 1,2,3-Trichloropropane	10.10	75	11504	2.082	ug/L #	1
65) 1,2-Dichlorobenzene	12.21	146	11844	0.844	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080620\
Data File : VU039768.D
Acq On : 06 Aug 2020 19:50
Operator : SY/MD
Sample : L3578-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Aug 07 04:31:14 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 07 04:28:48 2020
Response via : Initial Calibration

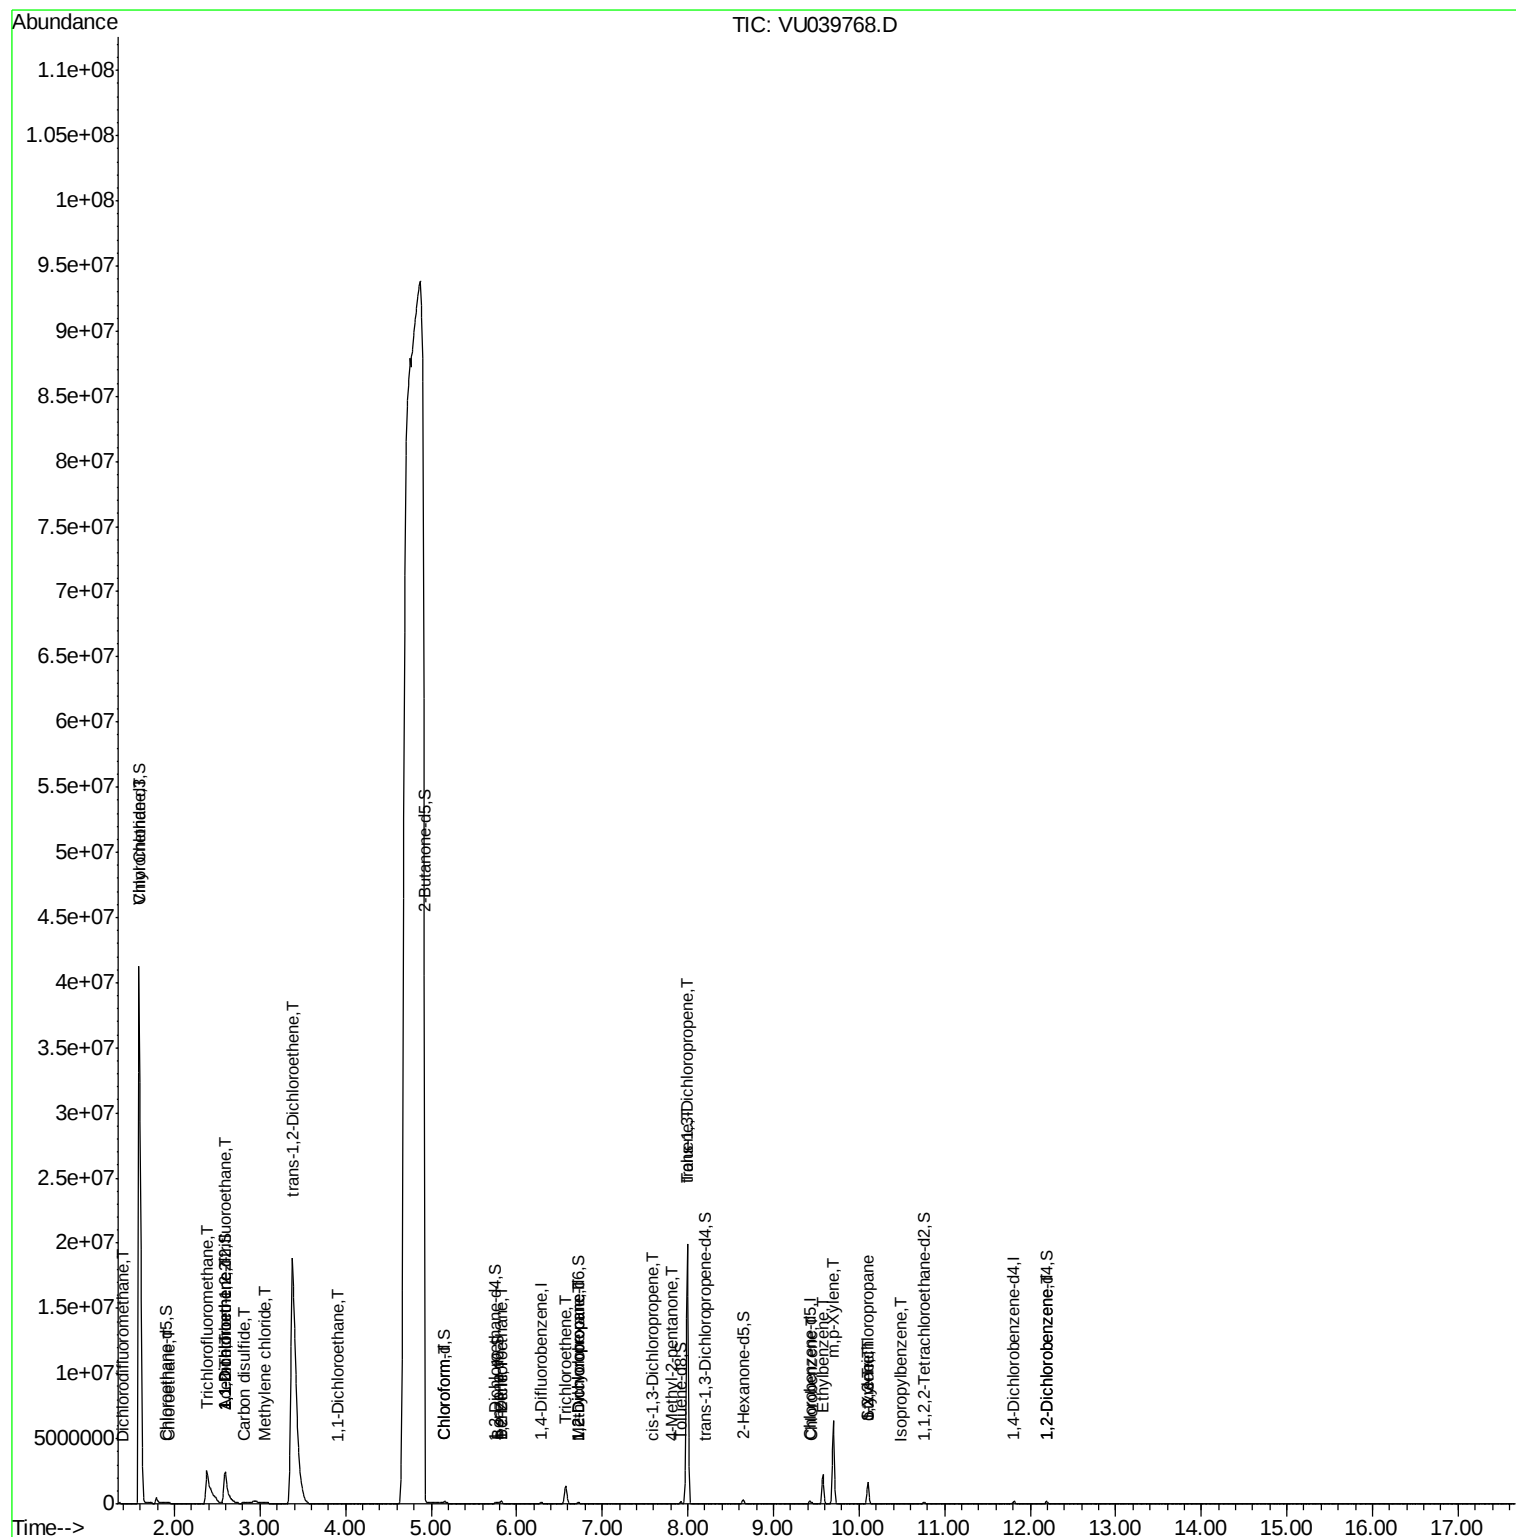

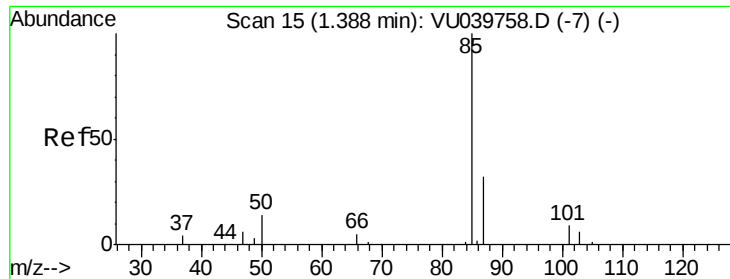

#2

Dichlorodifluoromethane

Concen: 0.102 ug/L

RT: 1.40 min Scan# 19

Delta R.T. 0.01 min

Lab File: VU039768.D

Acq: 06 Aug 2020 19:50

Instrument :

MSVOA_U


ClientSampleId :

Tot Ion: 85 Resp: 914

Ion Ratio Lower Upper




85 100

87 28.6 25.4 38.0

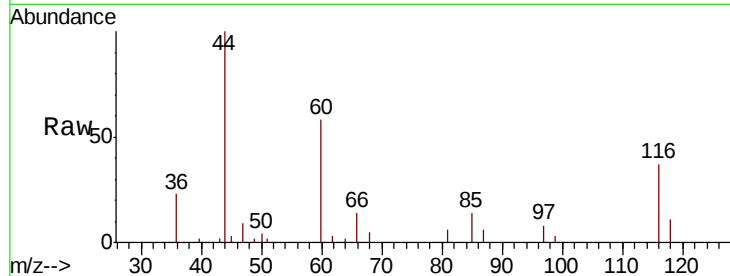

Abundance Ion 85.00 (84.70 to 85.70): VU039758.D (-7) (-)

Ion 87.00 (86.70 to 87.70): VU039758.D (-7) (-)

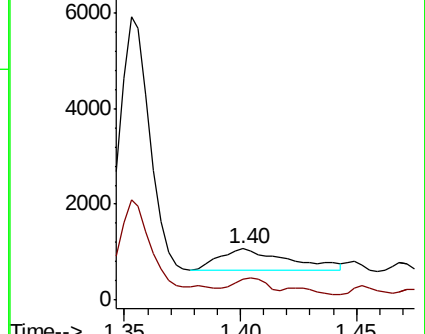

#3

Chloromethane

Concen: 46.970 ug/L

RT: 1.58 min Scan# 76

Delta R.T. 0.06 min

Lab File: VU039768.D


Acq: 06 Aug 2020 19:50

Tgt Ion: 50 Resp: 442975

Ion Ratio Lower Upper



50 100


52 0.4 21.6 40.0#



Abundance Ion 50.05 (49.75 to 50.75): VU039758.D (-49) (-)

Ion 52.05 (51.75 to 52.75): VU039758.D (-49) (-)




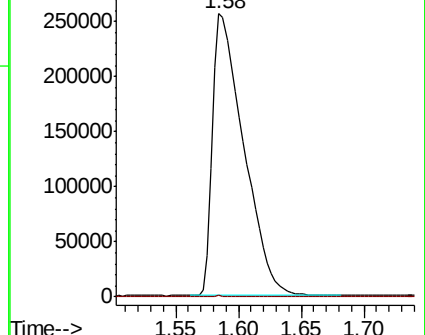




#8
Chloroethane
Concen: 1.016 ug/L
RT: 1.95 min Scan# 189
Delta R.T. 0.01 min
Lab File: VU039768.D
Acq: 06 Aug 2020 19:50




Instrument :
MSVOA_U
ClientSampleId :


Tot Ion: 64 Resp: 6735
Ion Ratio Lower Upper
64 100
66 5.2 22.3 41.3#

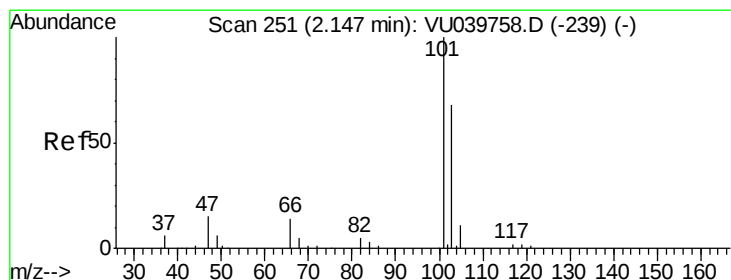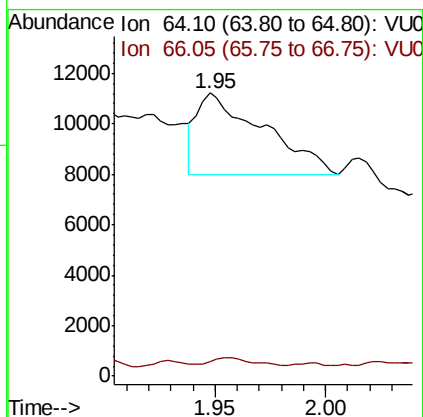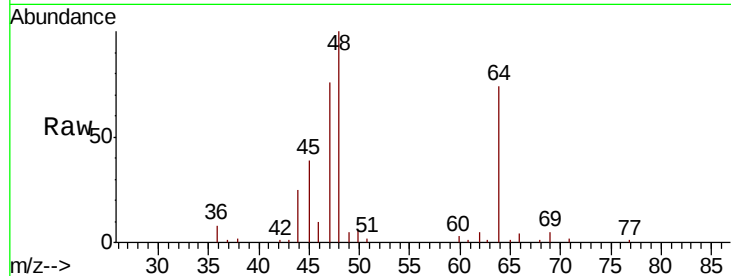

#9
Trichlorofluoromethane
Concen: 1.032 ug/L
RT: 2.38 min Scan# 325
Delta R.T. 0.24 min
Lab File: VU039768.D
Acq: 06 Aug 2020 19:50

Tgt Ion:101 Resp: 14511
Ion Ratio Lower Upper
101 100
103 65.0 51.4 77.2

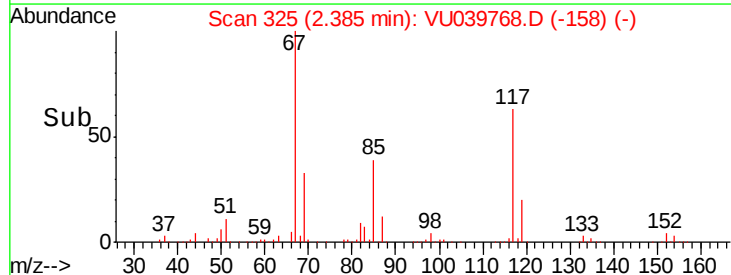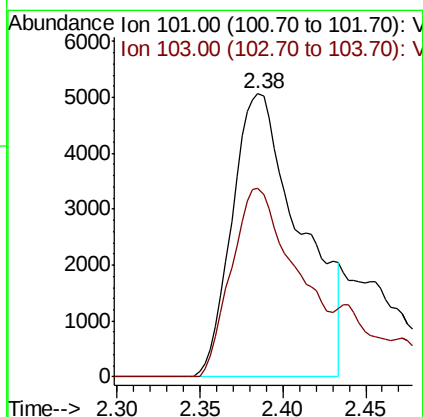



#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 118.665 ug/L

RT: 2.59 min Scan# 390

Delta R.T. -0.00 min

Lab File: VU039768.D

Acq: 06 Aug 2020 19:50

Instrument :

MSVOA_U

ClientSampled :


Tot Ion:101 Resp: 905474

Ion Ratio Lower Upper

101 100

85 46.3 37.9 56.9




151 72.6 54.7 82.1

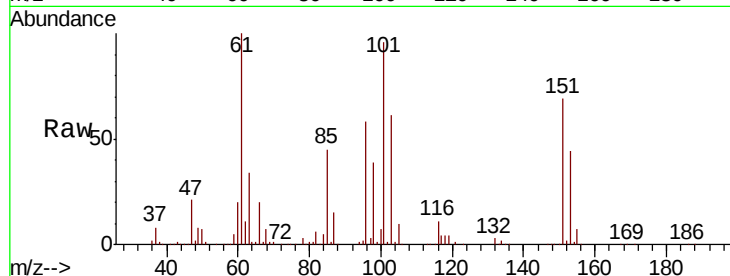

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VU0

Ion 151.00 (150.70 to 151.70): V

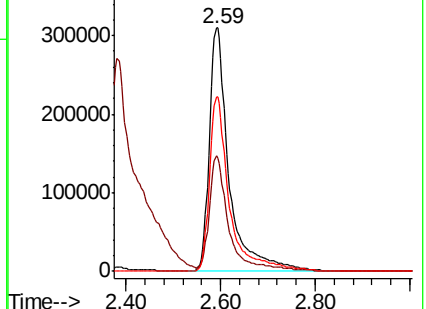

#12

1,1-Dichloroethene

Concen: 111.136 ug/L

RT: 2.60 min Scan# 391

Delta R.T. 0.01 min

Lab File: VU039768.D

Acq: 06 Aug 2020 19:50


Tgt Ion: 96 Resp: 737259

Ion Ratio Lower Upper

96 100

61 170.1 121.7 225.9



63 58.2 82.1 152.5#




Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.05 (60.75 to 61.75): VU0

Ion 63.00 (62.70 to 63.70): VU0

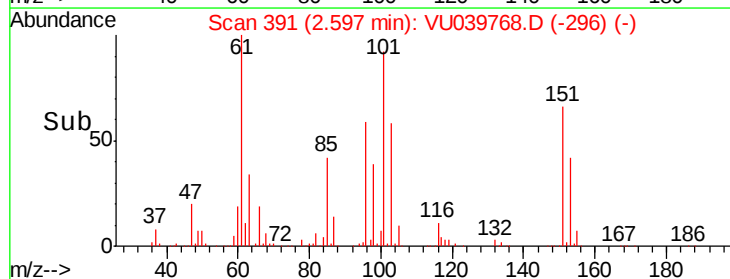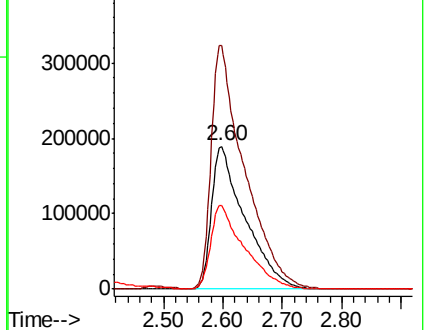

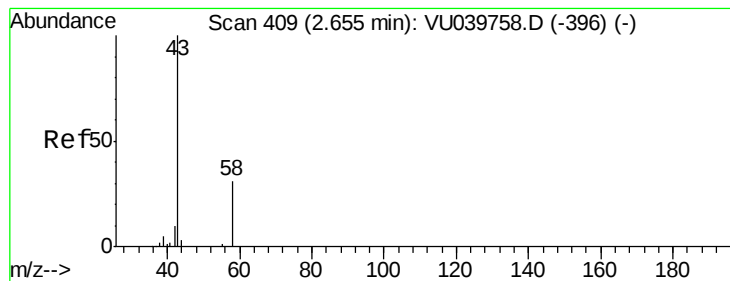

#13

Acetone

Concen: 6.919 ug/L

RT: 2.59 min Scan# 388

Delta R.T. -0.07 min

Lab File: VU039768.D

Acq: 06 Aug 2020 19:50





Instrument :
MSVOA_U
ClientSampled :

Tot Ion: 43 Resp: 10773

Ion Ratio Lower Upper

43 100

58 7.6 0.0 61.8

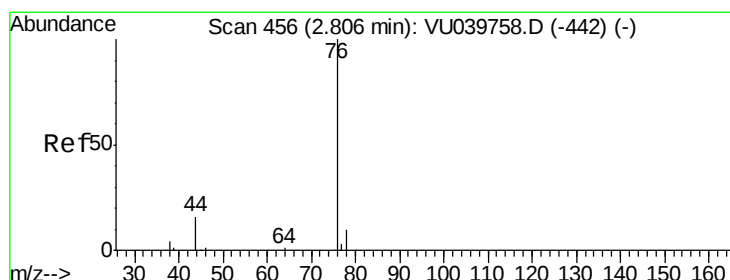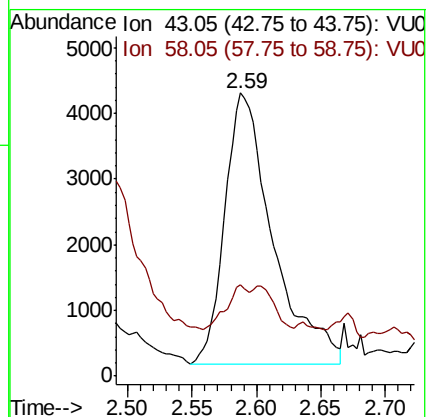

#14

Carbon disulfide

Concen: 8.410 ug/L

RT: 2.82 min Scan# 459

Delta R.T. 0.01 min

Lab File: VU039768.D




Acq: 06 Aug 2020 19:50


Tgt Ion: 76 Resp: 174442

Ion Ratio Lower Upper

76 100

78 9.2 7.8 11.6

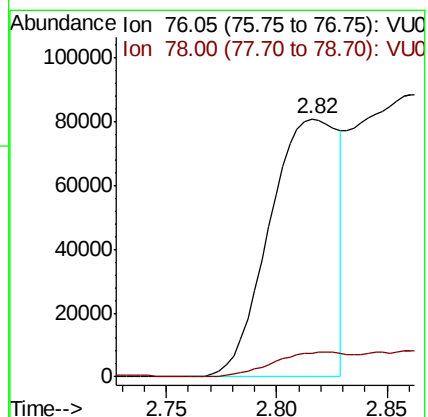







#16
Methvlene chloride
Concen: 2.806 ug/L
RT: 3.07 min Scan# 538
Delta R.T. 0.01 min
Lab File: VU039768.D
Acq: 06 Aug 2020 19:50

Instrument :
MSVOA_U
ClientSampleId :

Tot Ion: 84 Resp: 30006
Ion Ratio Lower Upper
84 100
86 70.0 43.9 81.5
49 127.1 94.4 175.4

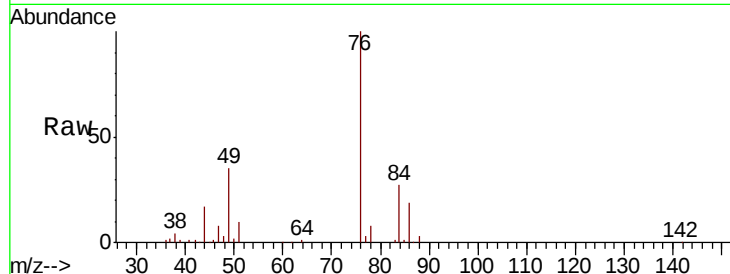


Abundance Ion 84.05 (83.75 to 84.75): VU0
Ion 86.00 (85.70 to 86.70): VU0
Ion 49.10 (48.80 to 49.80): VU0

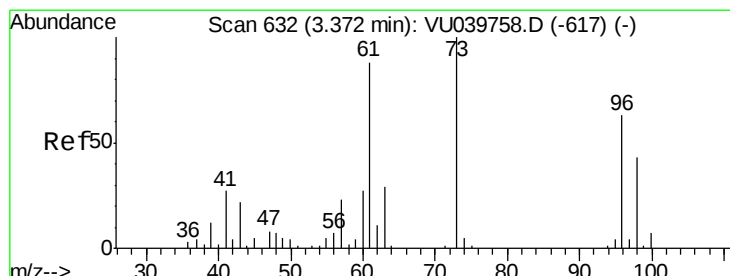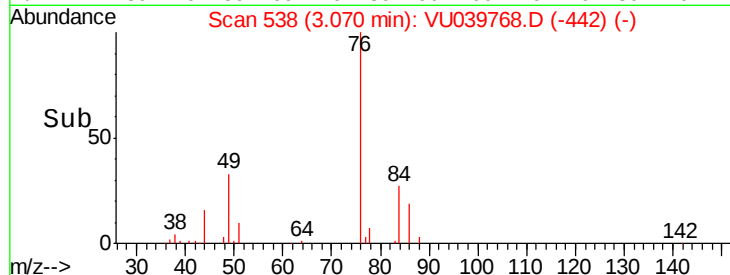
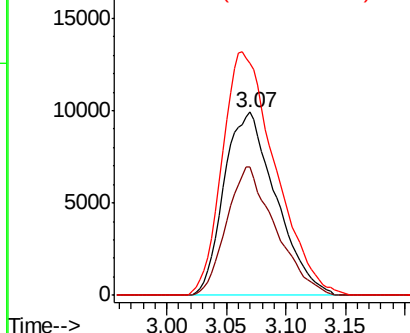



#18
trans-1,2-Dichloroethene
Concen: 2016.220 ug/L
RT: 3.38 min Scan# 634
Delta R.T. 0.01 min
Lab File: VU039768.D
Acq: 06 Aug 2020 19:50

Tgt Ion: 96 Resp:14891021
Ion Ratio Lower Upper
96 100
61 169.8 96.5 179.1
98 63.7 40.9 76.0

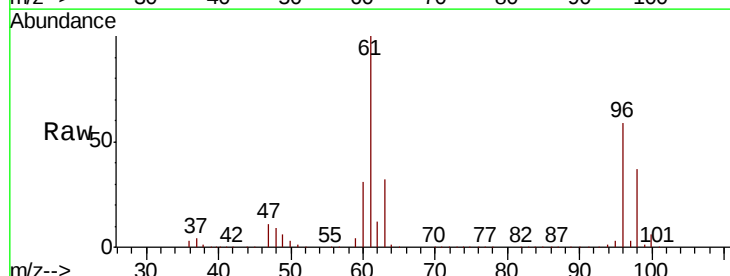

Abundance Ion 96.00 (95.70 to 96.70): VU0
Ion 61.05 (60.75 to 61.75): VU0
Ion 97.95 (97.65 to 98.65): VU0



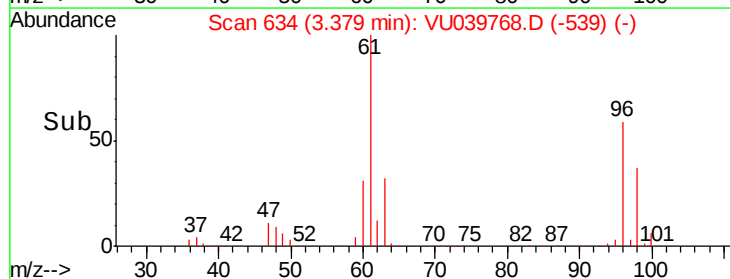
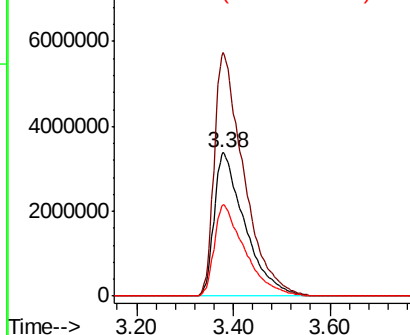




#19
 1,1-Dichloroethane
 Concen: 2.561 ug/L
 RT: 3.92 min Scan# 803
 Delta R.T. 0.03 min
 Lab File: VU039768.D
 Acq: 06 Aug 2020 19:50




Instrument :
 MSVOA_U
 ClientSampleId :


Tot Ion: 63 Resp: 34922
 Ion Ratio Lower Upper
 63 100
 65 30.7 22.0 41.0
 83 14.2 10.9 20.2

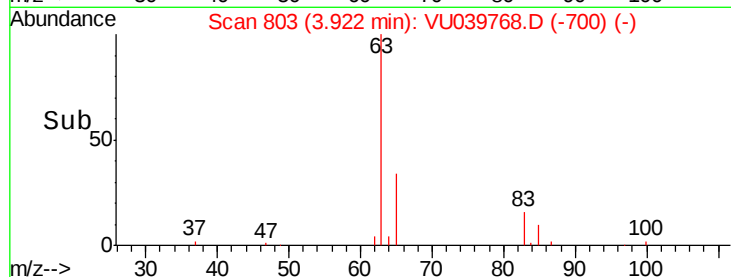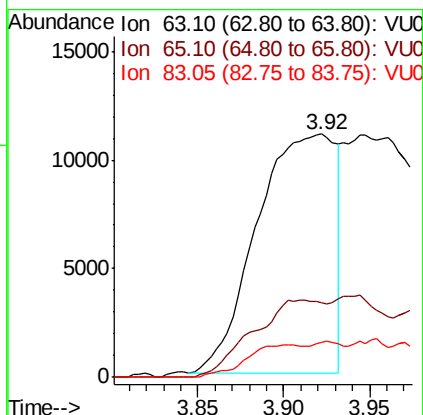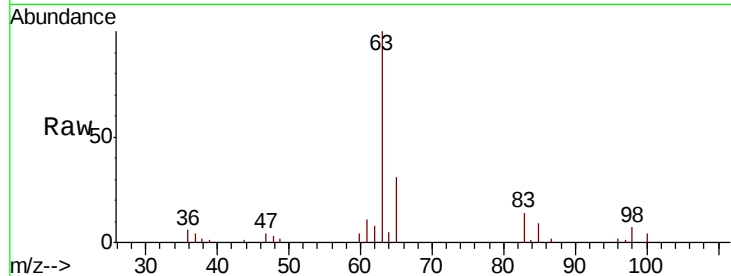

#25
 Chloroform
 Concen: 4.206 ug/L
 RT: 5.17 min Scan# 1190
 Delta R.T. 0.06 min
 Lab File: VU039768.D
 Acq: 06 Aug 2020 19:50

Tgt Ion: 83 Resp: 61643
 Ion Ratio Lower Upper
 83 100
 85 63.9 42.1 78.3



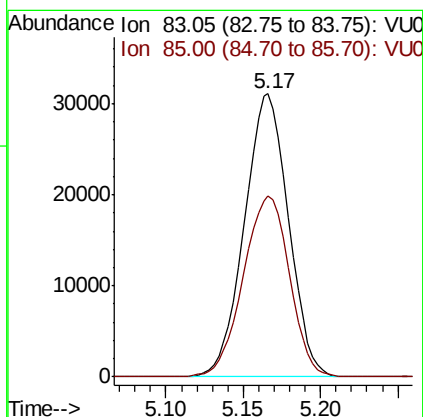



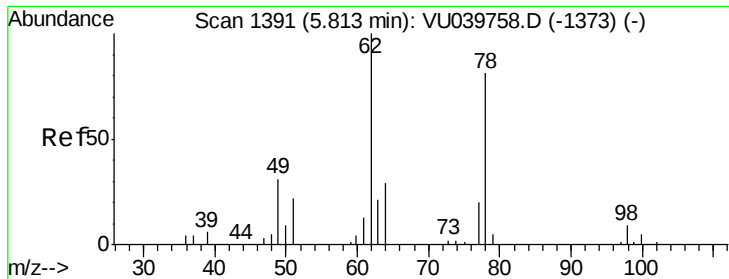




#27
 1,2-Dichloroethane
 Concen: 0.198 ug/L
 RT: 5.82 min Scan# 1393
 Delta R.T. 0.01 min
 Lab File: VU039768.D
 Acq: 06 Aug 2020 19:50


Instrument :
 MSVOA_U
 ClientSampled :

Tot Ion: 62 Resp: 1997
 Ion Ratio Lower Upper
 62 100
 98 19.8 7.3 10.9#

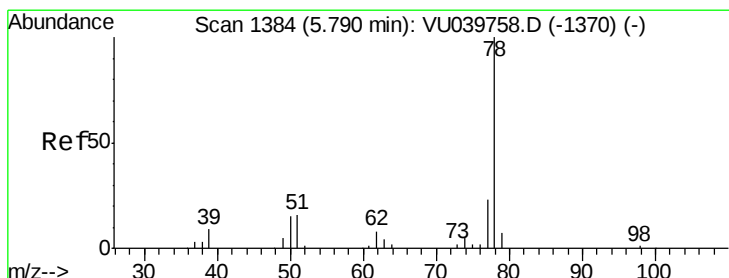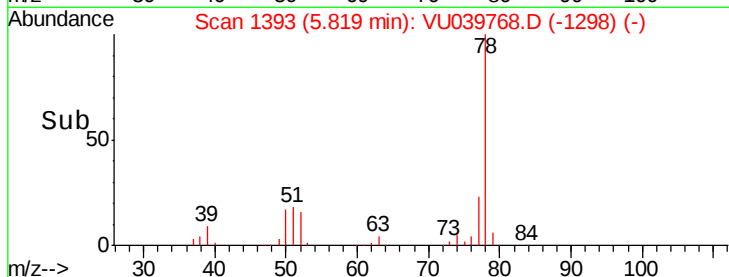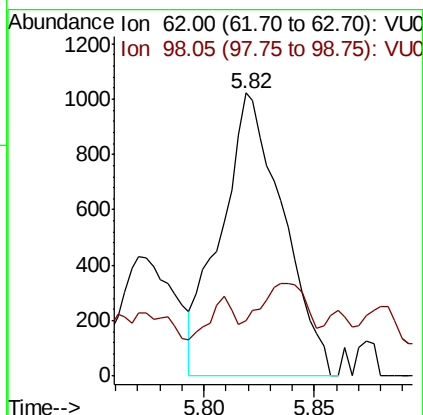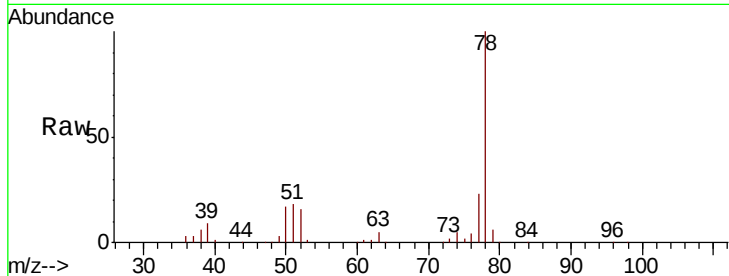

#33
 Benzene
 Concen: 6.366 ug/L
 RT: 5.82 min Scan# 1393
 Delta R.T. 0.03 min
 Lab File: VU039768.D
 Acq: 06 Aug 2020 19:50
 Tgt Ion: 78 Resp: 183563

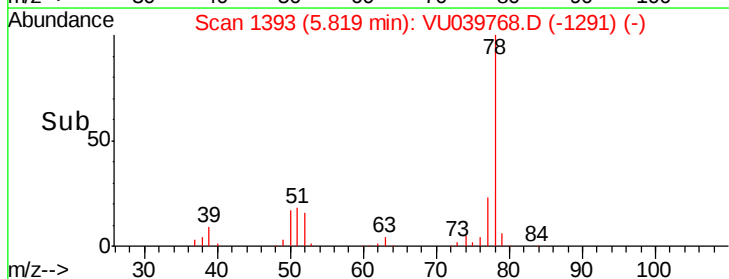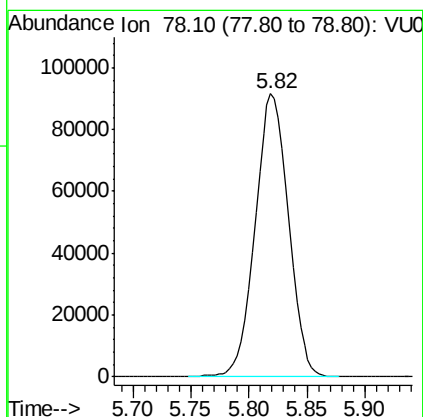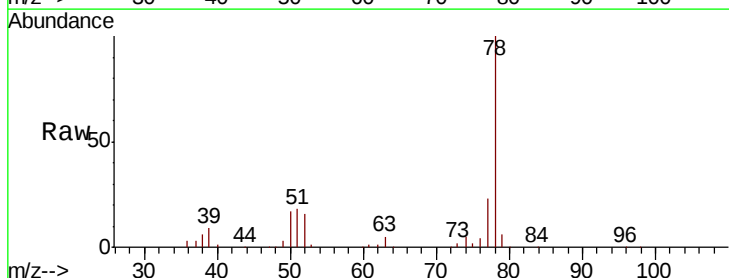







#34
 Trichloroethene
 Concen: 59.855 ug/L
 RT: 6.57 min Scan# 1627
 Delta R.T. 0.02 min
 Lab File: VU039768.D
 Acq: 06 Aug 2020 19:50

Instrument :
 MSVOA_U
 ClientSampled :

Tot Ion: 95 Resp: 448248
 Ion Ratio Lower Upper
 95 100
 97 65.2 44.0 81.8
 132 96.8 71.7 133.3
 130 100.7 71.1 132.1

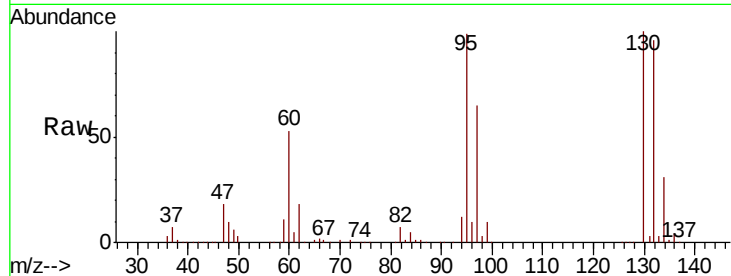


Abundance Ion 95.00 (94.70 to 95.70): VU0
 Ion 96.95 (96.65 to 97.65): VU0
 Ion 131.95 (131.65 to 132.65): V
 Ion 129.95 (129.65 to 130.65): V


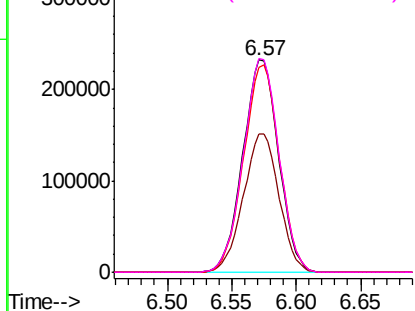



#35
 Methylcyclohexane
 Concen: 0.811 ug/L
 RT: 6.72 min Scan# 1674
 Delta R.T. -0.05 min
 Lab File: VU039768.D
 Acq: 06 Aug 2020 19:50

Tgt Ion: 83 Resp: 9694
 Ion Ratio Lower Upper
 83 100
 55 1.1 59.4 89.0#
 98 0.0 39.0 58.4#



Abundance Ion 83.15 (82.85 to 83.85): VU0
 Ion 55.10 (54.80 to 55.80): VU0
 Ion 98.15 (97.85 to 98.85): VU0



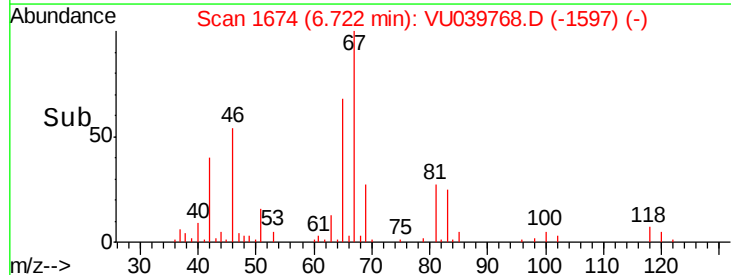
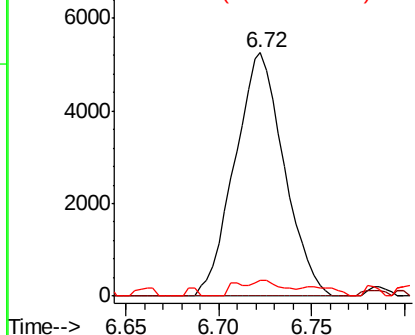




#37
 1,2-Dichloropropane
 Concen: 0.741 ug/L
 RT: 6.72 min Scan# 1674
 Delta R.T. -0.08 min
 Lab File: VU039768.D
 Acq: 06 Aug 2020 19:50




Instrument :
 MSVOA_U
 ClientSampleId :


Tot Ion: 63 Resp: 5679
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.8 5.6#

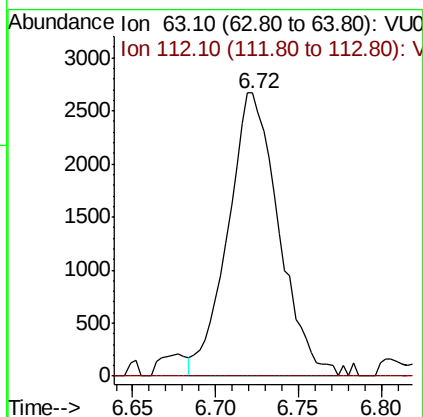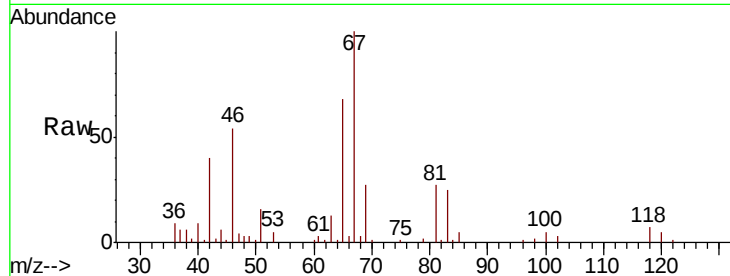

#39
 cis-1,3-Dichloropropene
 Concen: 0.160 ug/L
 RT: 7.58 min Scan# 1942
 Delta R.T. -0.03 min
 Lab File: VU039768.D
 Acq: 06 Aug 2020 19:50

Tgt Ion: 75 Resp: 1670
 Ion Ratio Lower Upper
 75 100
 77 32.9 22.4 41.6

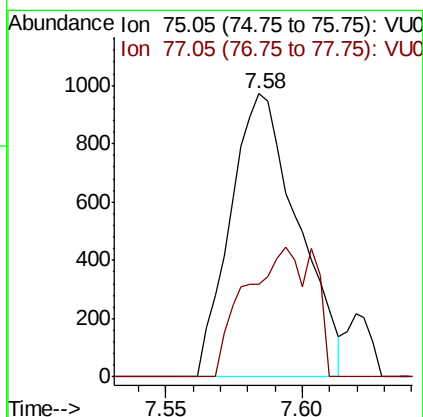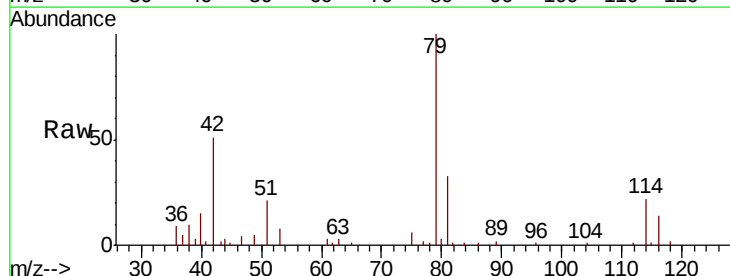







#40
 4-Methyl-2-pentanone
 Concen: 5.704 ug/L
 RT: 7.81 min Scan# 2013
 Delta R.T. 0.01 min
 Lab File: VU039768.D
 Acq: 06 Aug 2020 19:50

Instrument :
 MSVOA_U
 ClientSampleId :

Tot Ion: 43 Resp: 32648
 Ion Ratio Lower Upper
 43 100
 58 37.9 29.4 44.2
 100 14.3 11.7 17.5

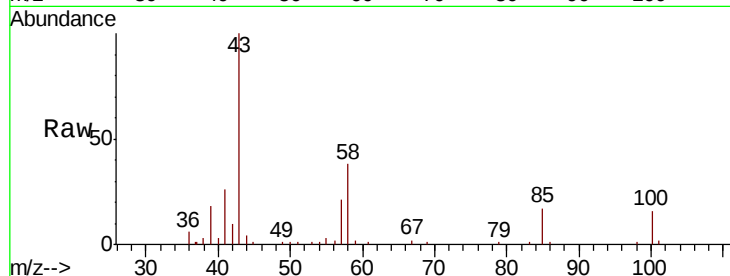


Abundance Ion 43.05 (42.75 to 43.75): VU0
 Ion 58.05 (57.75 to 58.75): VU0
 Ion 100.15 (99.85 to 100.85): VU0


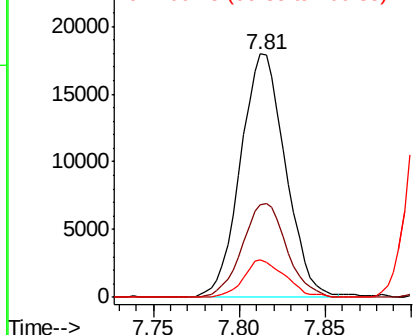



#42
 Toluene
 Concen: 415.189 ug/L
 RT: 8.00 min Scan# 2070
 Delta R.T. 0.02 min
 Lab File: VU039768.D
 Acq: 06 Aug 2020 19:50

Tgt Ion: 91 Resp: 12581428
 Ion Ratio Lower Upper
 91 100
 92 60.6 41.6 77.3



Abundance Ion 91.15 (90.85 to 91.85): VU0
 Ion 92.15 (91.85 to 92.85): VU0

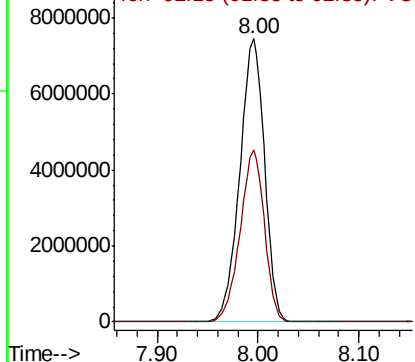



#44

trans-1,3-Dichloropropene

Concen: 11.227 ug/L

RT: 8.00 min Scan# 2070

Delta R.T. -0.22 min

Lab File: VU039768.D

Acq: 06 Aug 2020 19:50

Instrument :

MSVOA_U


ClientSampleId :

Tot Ion: 75 Resp: 105647

Ion Ratio Lower Upper




75 100

77 161.4 21.6 40.2#

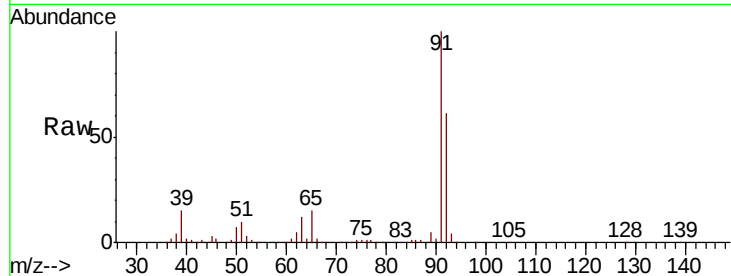

Abundance Ion 75.05 (74.75 to 75.75): VU039758.D (-2123) (-)

Ion 77.05 (76.75 to 77.75): VU039758.D (-2123) (-)

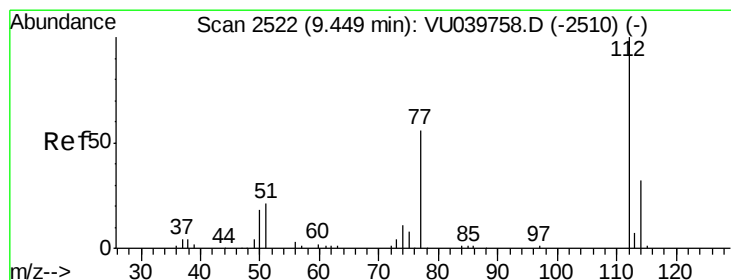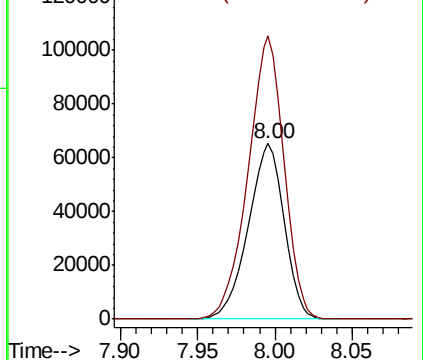

#51

Chlorobenzene

Concen: 1.344 ug/L

RT: 9.46 min Scan# 2524

Delta R.T. 0.01 min

Lab File: VU039768.D

Acq: 06 Aug 2020 19:50


Tgt Ion: 112 Resp: 27365

Ion Ratio Lower Upper

112 100

114 31.8 23.2 43.0



77 62.1 47.8 71.6




Abundance Ion 112.10 (111.80 to 112.80): VU039758.D (-2510) (-)

Ion 114.05 (113.75 to 114.75): VU039758.D (-2510) (-)

Ion 77.10 (76.80 to 77.80): VU039758.D (-2510) (-)

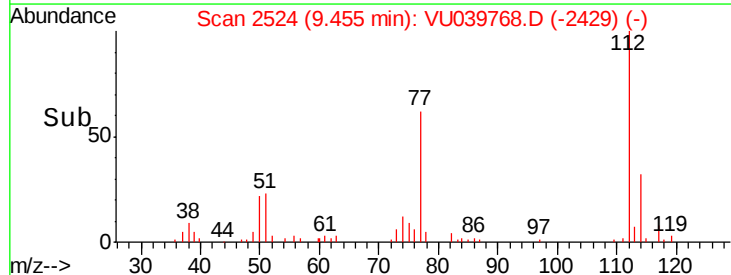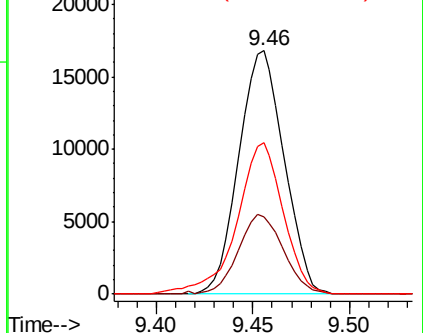



#52

Ethylbenzene

Concen: 44.858 ug/L

RT: 9.58 min Scan# 2562

Delta R.T. 0.00 min

Lab File: VU039768.D

Acq: 06 Aug 2020 19:50


Instrument :
MSVOA_U
ClientSampled :

Tot Ion: 91 Resp: 1521379




Ion Ratio Lower Upper

91 100

106 30.9 22.8 42.4

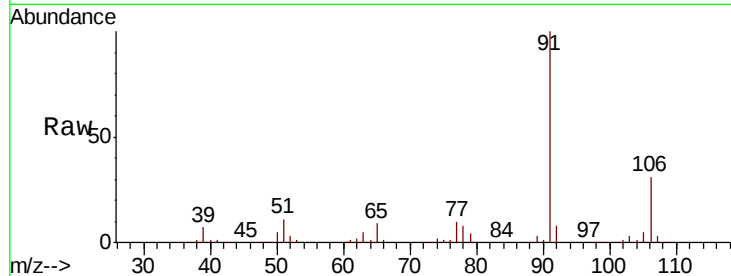

Abundance Ion 91.15 (90.85 to 91.85): VU039768.D (-2547) (-)

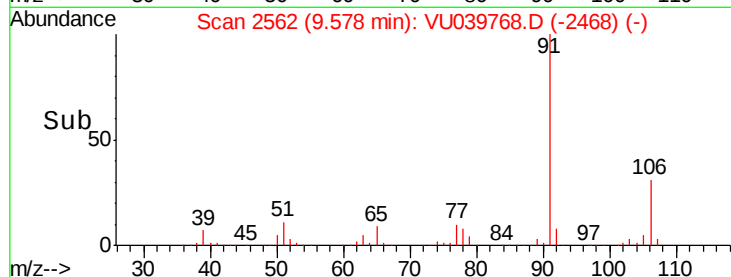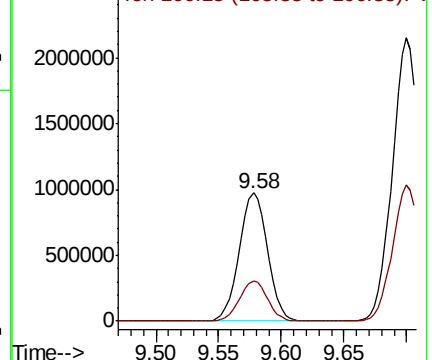

#53

m,p-Xylene

Concen: 125.324 ug/L

RT: 9.70 min Scan# 2600

Delta R.T. 0.00 min

Lab File: VU039768.D


Acq: 06 Aug 2020 19:50

Tgt Ion:106 Resp: 1618612



Ion Ratio Lower Upper


106 100

91 208.7 135.5 251.7



Abundance Ion 106.15 (105.85 to 106.85): VU039768.D (-2586) (-)

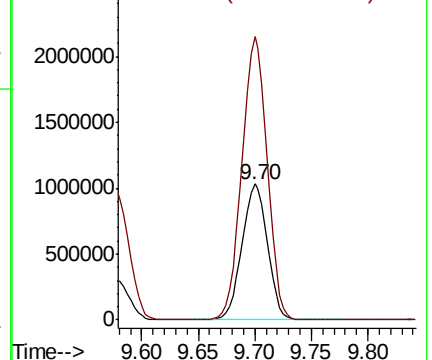


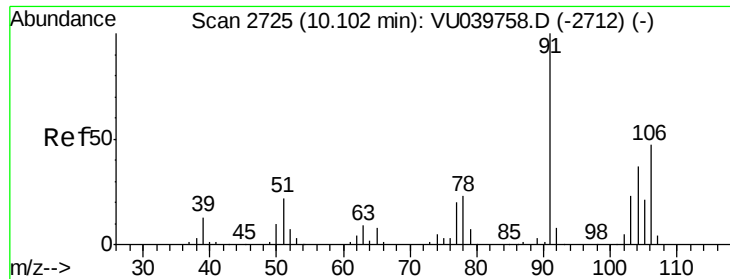




#54
o-Xylene
Concen: 33.483 ug/L
RT: 10.10 min Scan# 2726
Delta R.T. 0.00 min
Lab File: VU039768.D
Acq: 06 Aug 2020 19:50

Instrument :
MSVOA_U
ClientSampled :

Tot Ion:106 Resp: 423450
Ion Ratio Lower Upper
106 100
91 217.9 140.8 261.6

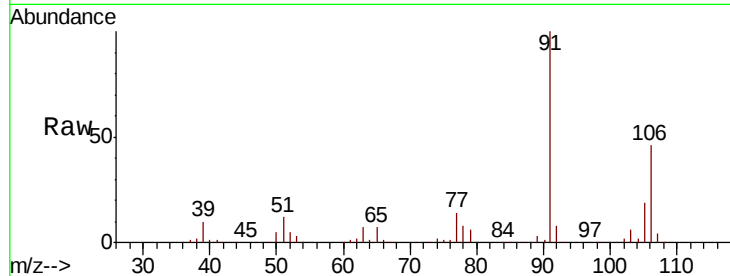


Abundance Ion 106.15 (105.85 to 106.85): V
Ion 91.15 (90.85 to 91.85): VU0

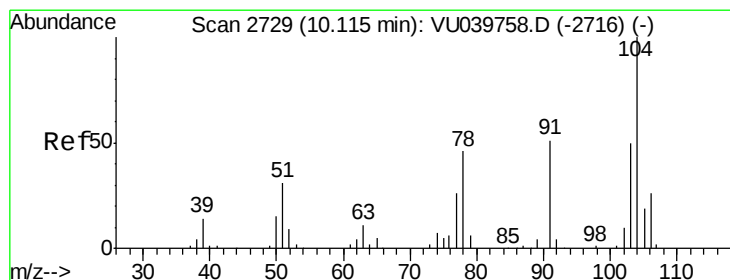
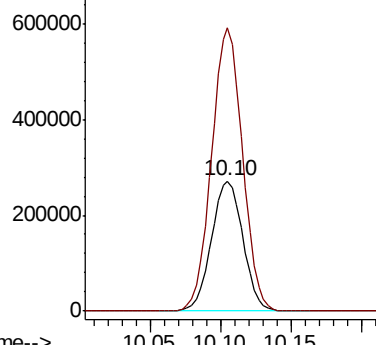



#55
Styrene
Concen: 1.040 ug/L
RT: 10.10 min Scan# 2726
Delta R.T. -0.01 min
Lab File: VU039768.D
Acq: 06 Aug 2020 19:50

Tgt Ion:104 Resp: 22147
Ion Ratio Lower Upper
104 100
78 327.4 32.3 60.1#



Abundance Ion 104.10 (103.80 to 104.80): V
Ion 78.10 (77.80 to 78.80): VU0

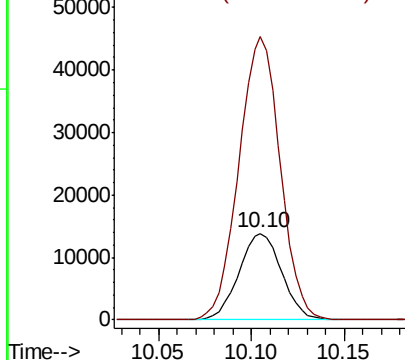



#56

Isopropylbenzene

Concen: 0.103 ug/L

RT: 10.48 min Scan# 2844

Delta R.T. -0.00 min

Lab File: VU039768.D

Acq: 06 Aug 2020 19:50

Instrument :

MSVOA_U

ClientSampleId :


Tot Ion: 105 Resp: 3469

Ion Ratio Lower Upper

105 100

120 29.2 21.0 31.6




77 16.7 12.9 19.3

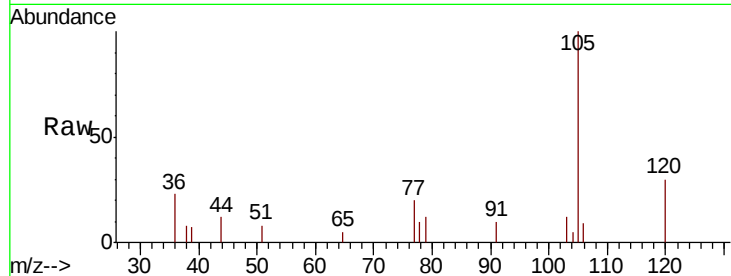

Abundance Ion 105.05 (104.75 to 105.75): V

Ion 120.10 (119.80 to 120.80): V

Ion 77.10 (76.80 to 77.80): VU

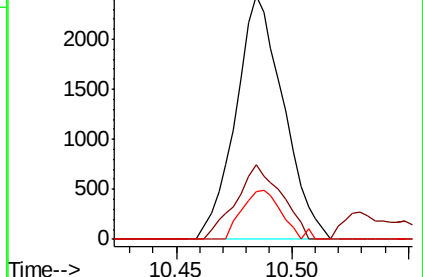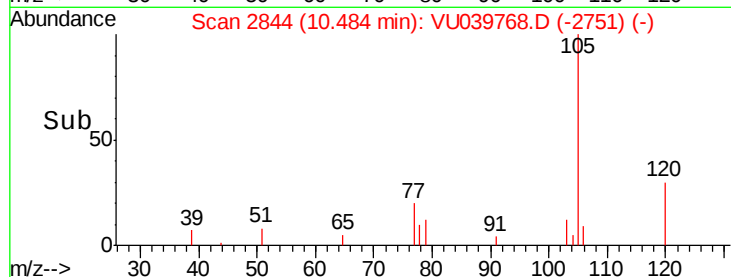

#59

1,2,3-Trichloropropane

Concen: 2.082 ug/L

RT: 10.10 min Scan# 2726

Delta R.T. -0.72 min

Lab File: VU039768.D


Acq: 06 Aug 2020 19:50

Tgt Ion: 75 Resp: 11504

Ion Ratio Lower Upper



75 100


77 1076.8 24.6 37.0#



Abundance Ion 75.00 (74.70 to 75.70): VU

Ion 77.00 (76.70 to 77.70): VU

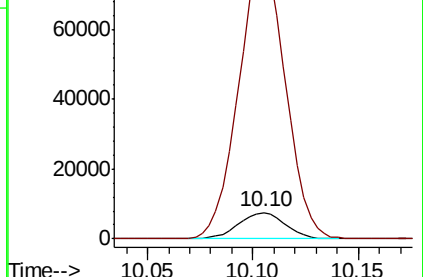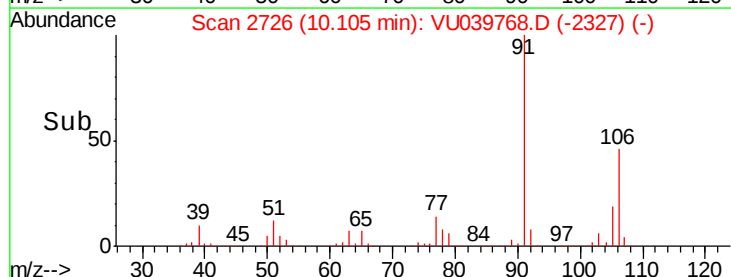


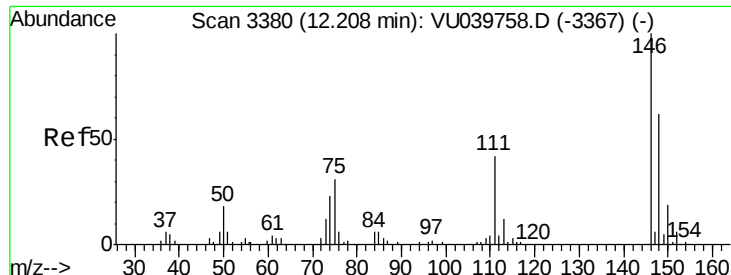

#65
 1,2-Dichlorobenzene
 Concen: 0.844 ug/L
 RT: 12.21 min Scan# 3380
 Delta R.T. -0.00 min
 Lab File: VU039768.D
 Acq: 06 Aug 2020 19:50

Instrument :
 MSVOA_U
 ClientSampleId :

Tot Ion:146 Resp: 11844
 Ion Ratio Lower Upper
 146 100
 111 42.6 33.1 49.7
 148 67.4 51.5 77.3



Abundance Ion 145.95 (145.65 to 146.65): V
 Ion 111.00 (110.70 to 111.70): V
 Ion 148.00 (147.70 to 148.70): V

