

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080620\
 Data File : VU039748.D
 Acq On : 06 Aug 2020 11:46
 Operator : SY/MD
 Sample : VU0806WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK13

Quant Time: Aug 07 03:31:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 07 03:23:19 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	81464	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	78001	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	34760	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	20362	4.63	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.60%
7) Chloroethane-d5	1.92	69	21381	4.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.80%
11) 1,1-Dichloroethene-d2	2.57	63	29948	3.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.60%
20) 2-Butanone-d5	4.66	46	84325	43.58	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.16%
24) Chloroform-d	5.08	84	48363	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.00%
26) 1,2-Dichloroethane-d4	5.72	65	29197	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.20%
32) Benzene-d6	5.74	84	86744	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
36) 1,2-Dichloropropane-d6	6.70	67	29392	4.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.40%
41) Toluene-d8	7.90	98	68384	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.00%
43) trans-1,3-Dichloropropene-	8.19	79	11324	4.65	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.00%
46) 2-Hexanone-d5	8.64	63	57098	43.30	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.60%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	25541	4.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	29284	4.92	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.40%


Target Compounds					Ovalue
16) Methylene chloride	3.06	84	1506	0.192 ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080620\
Data File : VU039748.D
Acq On : 06 Aug 2020 11:46
Operator : SY/MD
Sample : VU0806WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK13

Quant Time: Aug 07 03:31:28 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 07 03:23:19 2020
Response via : Initial Calibration

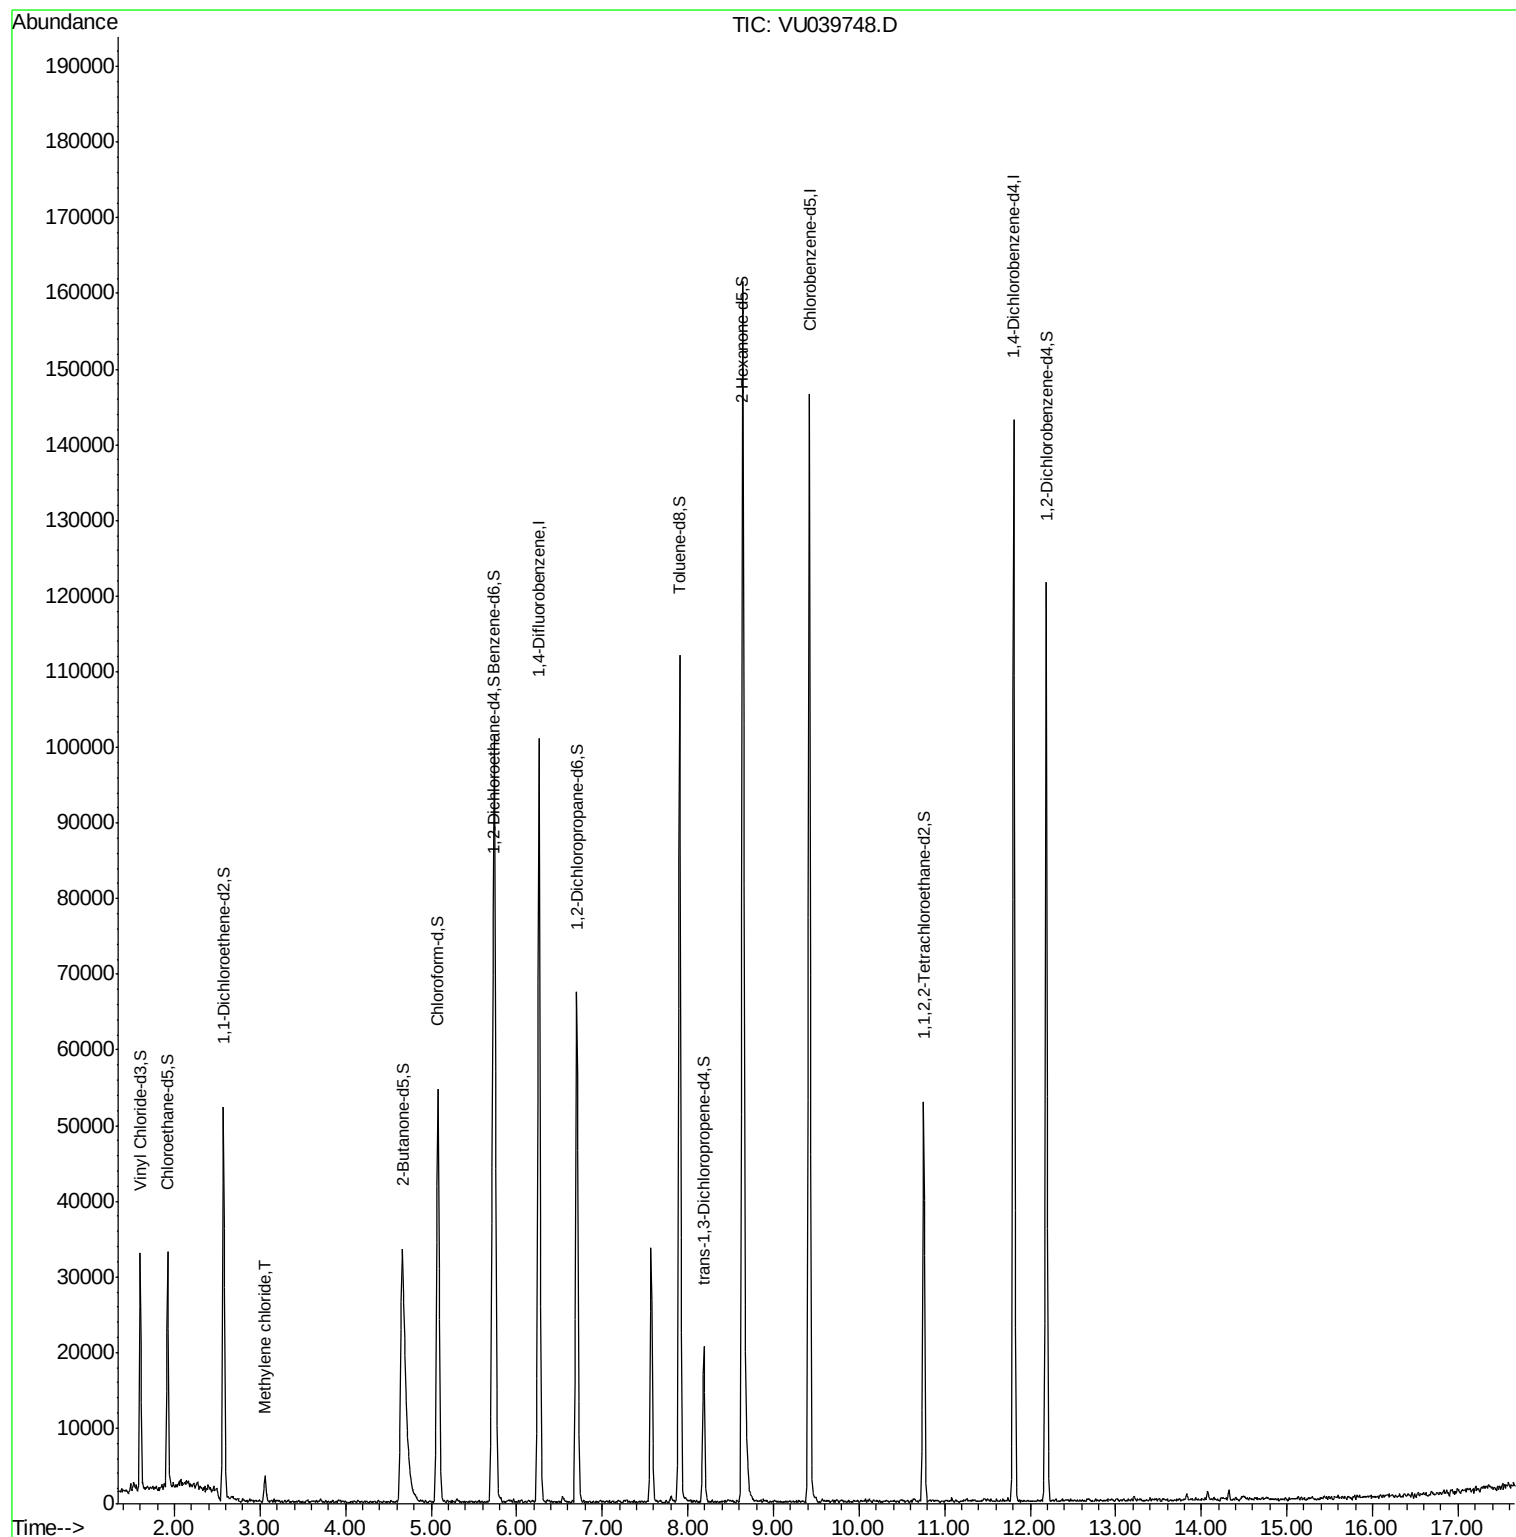

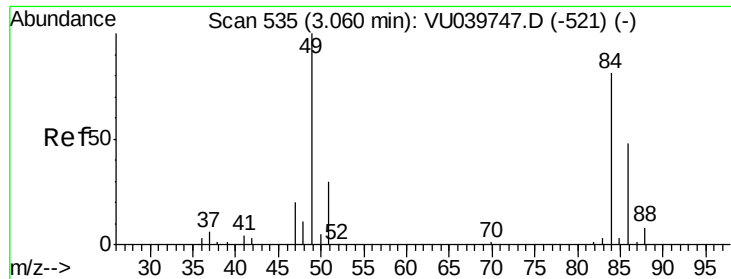

#16
Methylene chloride
Concen: 0.192 ug/L
RT: 3.06 min Scan# 534
Delta R.T. -0.00 min
Lab File: VU039748.D
Acq: 06 Aug 2020 11:46

Instrument :
MSVOA_U
ClientSampleId :
VBLK13

Tot Ion:	84	Resp:	1506
Ion	Ratio	Lower	Upper
84	100		
86	55.5	43.9	81.5
49	101.2	94.4	175.4

