


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080620\
 Data File : VU039746.D
 Acq On : 06 Aug 2020 10:25
 Operator : SY/MD
 Sample : BFB09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB09

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Aug 10 06:26:03 2020

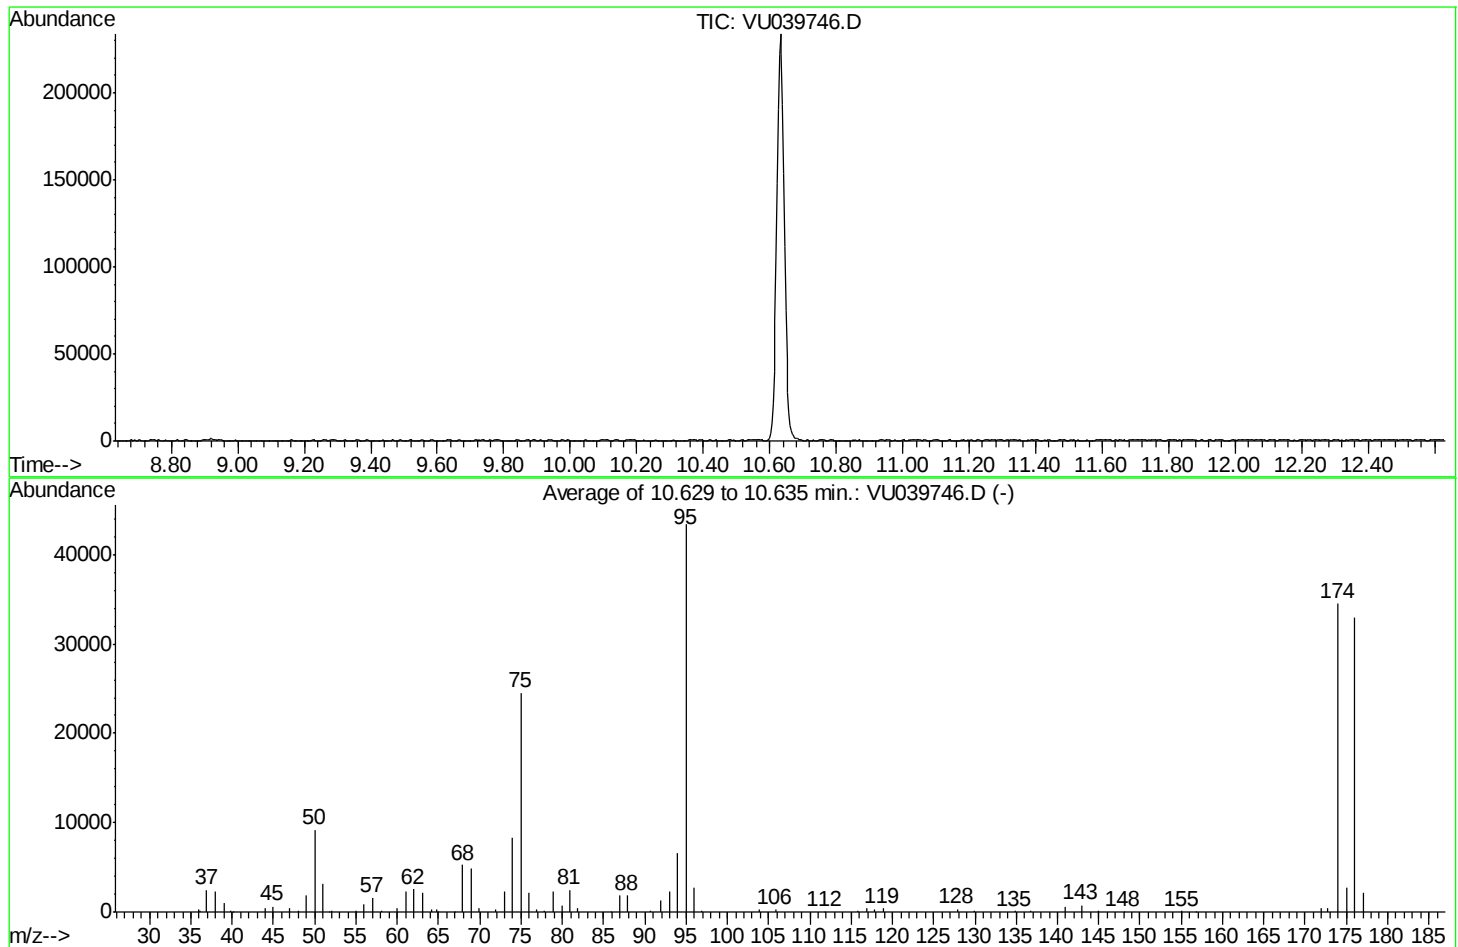

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	9218	PASS
75	95	30	80	56.5	24520	PASS
95	95	100	100	100.0	43394	PASS
96	95	5	9	6.2	2684	PASS
173	174	0.00	2	1.3	438	PASS
174	95	50	120	79.5	34517	PASS
175	174	5	9	8.1	2794	PASS
176	174	95	101	95.6	33010	PASS
177	176	5	9	6.4	2112	PASS

m/z	Abundance
44.00	272.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
35.90	449.0
36.90	2485.0
37.90	2368.0
39.00	1024.0
39.80	117.0
44.00	704.0
44.90	630.0
46.90	533.0
48.00	261.0
48.90	1837.0
50.00	9197.0
50.90	3171.0
52.00	134.0
55.00	128.0
55.90	862.0
57.00	1629.0
58.10	141.0
59.90	414.0
61.00	2234.0
62.00	2407.0
63.00	2182.0
64.20	224.0
64.80	412.0
67.00	109.0
67.90	5167.0
68.90	4762.0
69.90	427.0
72.00	342.0
72.90	2221.0
74.00	8305.0
75.00	24392.0
76.00	2205.0
76.90	301.0
77.80	230.0
78.90	2337.0
79.90	629.0
80.90	2459.0
81.90	485.0
85.80	132.0
86.90	1758.0
87.80	1720.0
90.70	197.0
91.90	1416.0
92.90	2269.0
94.00	6565.0
95.00	42216.0
96.00	2602.0
96.90	206.0
103.80	241.0
105.80	244.0
115.90	193.0
116.90	439.0
117.90	194.0
118.90	417.0
127.90	272.0
129.90	197.0
135.00	103.0
141.00	634.0
143.00	687.0
144.90	125.0
148.00	113.0
155.00	114.0
171.90	460.0
172.90	461.0
174.00	33032.0
175.00	2887.0
176.00	32008.0
177.00	2085.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
35.90	417.0
36.90	2587.0
37.90	2400.0
39.00	1105.0
39.80	134.0
43.90	697.0
44.90	604.0
46.90	503.0
48.00	219.0
48.90	1959.0
50.00	9517.0
50.90	3216.0
52.10	140.0
54.90	117.0
56.00	880.0
57.00	1704.0
58.10	143.0
59.90	406.0
61.00	2266.0
61.90	2603.0
63.00	2246.0
64.20	277.0
64.80	312.0
67.00	109.0
67.90	5478.0
69.00	5055.0
69.90	482.0
72.00	339.0
73.00	2386.0
74.00	8630.0
75.00	25232.0
76.00	2300.0
76.90	285.0
77.80	216.0
78.90	2466.0
79.90	692.0
80.90	2572.0
81.80	457.0
86.90	1925.0
87.80	1895.0
90.70	203.0
92.00	1401.0
93.00	2390.0
94.00	6919.0
95.00	44712.0
96.00	2667.0
96.90	173.0
103.80	264.0
105.90	276.0
111.80	103.0
115.90	178.0
116.90	391.0
117.90	261.0
118.90	423.0
127.90	363.0
129.90	219.0
134.80	122.0
136.80	141.0
141.00	616.0
142.90	761.0
144.90	123.0
148.00	106.0
155.10	133.0
172.00	522.0
172.80	468.0
174.00	35720.0
175.00	2849.0
176.00	34096.0
177.00	2228.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
36.10	324.0
36.90	2424.0
38.00	2153.0
39.00	1098.0
39.80	127.0
40.10	141.0
44.00	689.0
44.90	516.0
46.90	455.0
48.00	150.0
48.90	1843.0
50.00	8941.0
50.90	2914.0
51.80	116.0
52.20	103.0
54.90	107.0
56.00	784.0
57.00	1554.0
58.00	131.0
59.90	349.0
61.00	2255.0
62.00	2561.0
63.00	2181.0
64.10	239.0
65.00	229.0
67.90	5113.0
69.00	4848.0
69.90	534.0
71.90	329.0
73.00	2202.0
74.00	8094.0
75.00	23936.0
76.00	2139.0
76.90	264.0
78.90	2303.0
79.90	648.0
80.90	2382.0
81.80	451.0
86.90	1852.0
87.90	1967.0
90.80	179.0
92.00	1276.0
93.00	2353.0
94.00	6377.0
95.00	43256.0
96.00	2784.0
103.80	237.0
105.90	289.0
115.80	157.0
117.00	308.0
117.80	265.0
118.90	336.0
127.90	304.0
129.80	192.0
134.80	127.0
136.80	141.0
141.00	554.0
142.90	763.0
155.10	124.0
156.80	110.0
172.10	521.0
172.70	385.0
174.00	34800.0
175.00	2648.0
176.00	32928.0
177.00	2023.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09