

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080718\
 Data File : VU025963.D
 Acq On : 08 Aug 2018 01:45
 Operator : MD/SY
 Sample : J4361-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080718WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.622	7	10	11	rBV2	259	155	0.002%	0.0002%
2	0.645	15	17	21	rVV2	229	133	0.001%	0.0002%
3	0.661	21	22	24	rVB	159	35	0.000%	0.0000%
4	0.735	39	45	48	rBV3	359	401	0.04%	0.0005%
5	0.764	51	54	55	rBV3	165	88	0.01%	0.0001%
6	0.812	68	69	70	rBV3	75	21	0.000%	0.0000%
7	0.825	70	73	77	rBV2	301	245	0.002%	0.0003%
8	0.976	117	120	122	rBV3	476	338	0.003%	0.0004%
9	1.089	147	155	170	rBV	322604	359126	36.34%	4.299%
10	1.400	245	252	264	rBV	131038	136628	13.82%	1.635%
11	1.680	331	339	353	rVB	92528	122326	12.38%	1.464%
12	2.272	514	523	535	rBV	212270	318708	32.25%	3.815%
13	2.671	645	647	650	rVB2	389	200	0.002%	0.0002%
14	2.783	680	682	684	rBV2	314	227	0.002%	0.0003%
15	3.076	766	773	777	rBV3	479	544	0.006%	0.0007%
16	3.159	795	799	800	rBV	234	138	0.001%	0.0002%
17	3.169	800	802	803	rBV	200	85	0.001%	0.0001%
18	3.249	825	827	834	rVB3	456	325	0.003%	0.0004%
19	3.291	838	840	845	rVV2	286	276	0.003%	0.0003%
20	3.339	849	855	858	rBV2	331	359	0.004%	0.0004%
21	3.416	877	879	882	rBV2	339	244	0.002%	0.0003%
22	3.597	933	935	936	rBV2	142	43	0.000%	0.0001%
23	3.699	965	967	971	rBV	365	183	0.002%	0.0002%
24	3.725	971	975	977	rVB	321	191	0.002%	0.0002%
25	3.744	977	981	983	rBV2	477	372	0.004%	0.0004%
26	3.809	998	1001	1003	rBV	269	181	0.002%	0.0002%
27	3.828	1004	1007	1010	rVB	395	208	0.002%	0.0002%
28	3.863	1014	1018	1021	rVV3	501	427	0.004%	0.0005%
29	3.892	1025	1027	1030	rVB2	333	158	0.002%	0.0002%
30	3.918	1030	1035	1039	rBV3	384	419	0.004%	0.0005%
31	4.002	1059	1061	1063	rBV	288	123	0.001%	0.0001%
32	4.069	1080	1082	1085	rBV2	237	127	0.001%	0.0002%
33	4.092	1086	1089	1092	rVV2	238	172	0.002%	0.0002%
34	4.178	1102	1116	1147	rBV	80964	210699	21.32%	2.522%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080718\
 Data File : VU025963.D
 Acq On : 08 Aug 2018 01:45
 Operator : MD/SY
 Sample : J4361-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080718WMA.M
 Title : VOC Analysis

35	4.375	1173	1177	1179	rBV3	347	323	0.03%	0.004%
36	4.465	1202	1205	1209	rBV2	317	250	0.03%	0.003%
37	4.487	1210	1212	1214	rVV2	264	123	0.01%	0.001%
38	4.542	1227	1229	1230	rBV	181	81	0.01%	0.001%
39	4.568	1235	1237	1241	rBV	382	273	0.03%	0.003%
40	4.651	1245	1263	1288	rBV	172243	400732	40.55%	4.797%
41	4.805	1305	1311	1315	rVB3	373	381	0.04%	0.005%
42	4.828	1315	1318	1319	rBV	344	238	0.02%	0.003%
43	4.979	1358	1365	1368	rBV4	659	791	0.08%	0.009%
44	5.034	1379	1382	1383	rBV2	245	144	0.01%	0.002%
45	5.085	1396	1398	1399	rBV2	201	73	0.01%	0.001%
46	5.124	1406	1410	1413	rVB2	481	406	0.04%	0.005%
47	5.143	1413	1416	1417	rBV	96	41	0.00%	0.000%
48	5.153	1417	1419	1421	rVB	212	92	0.01%	0.001%
49	5.166	1421	1423	1426	rBV2	187	132	0.01%	0.002%
50	5.182	1426	1428	1431	rBV2	215	130	0.01%	0.002%
51	5.220	1438	1440	1443	rVB2	332	160	0.02%	0.002%
52	5.246	1445	1448	1450	rBV2	286	186	0.02%	0.002%
53	5.259	1450	1452	1455	rVB	164	78	0.01%	0.001%
54	5.346	1455	1479	1497	rBV2	331345	988345	100.00%	11.830%
55	5.613	1559	1562	1563	rBV2	289	174	0.02%	0.002%
56	5.889	1633	1648	1676	rBV	358664	705855	71.42%	8.449%
57	6.085	1704	1709	1712	rBV3	560	573	0.06%	0.007%
58	6.159	1728	1732	1733	rBV2	316	201	0.02%	0.002%
59	6.175	1733	1737	1739	rBV	337	287	0.03%	0.003%
60	6.336	1772	1787	1807	rBV	222081	444352	44.96%	5.319%
61	6.645	1881	1883	1885	rVB	173	80	0.01%	0.001%
62	6.661	1885	1888	1893	rBV2	576	543	0.05%	0.006%
63	6.776	1919	1924	1931	rVB3	522	752	0.08%	0.009%
64	6.809	1931	1934	1936	rBV2	235	129	0.01%	0.002%
65	6.828	1936	1940	1941	rBV3	283	185	0.02%	0.002%
66	6.931	1969	1972	1974	rVB	494	307	0.03%	0.004%
67	6.950	1974	1978	1981	rBV2	404	365	0.04%	0.004%
68	7.021	1996	2000	2001	rBV	365	185	0.02%	0.002%
69	7.034	2002	2004	2006	rVB	325	140	0.01%	0.002%
70	7.085	2018	2020	2024	rVB3	262	118	0.01%	0.001%
71	7.230	2053	2065	2086	rBV	120609	217121	21.97%	2.599%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080718\
 Data File : VU025963.D
 Acq On : 08 Aug 2018 01:45
 Operator : MD/SY
 Sample : J4361-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080718WMA.M
 Title : VOC Analysis

72	7.420	2121	2124	2129	rBV2	385	341	0.03%	0.004%
73	7.567	2157	2170	2190	rBV	445224	781333	79.05%	9.352%
74	7.854	2248	2259	2276	rBV	85901	146722	14.85%	1.756%
75	8.313	2385	2402	2430	rBV	243763	435444	44.06%	5.212%
76	8.468	2443	2450	2470	rVB3	16569	30036	3.04%	0.360%
77	8.558	2476	2478	2481	rBV2	433	291	0.03%	0.003%
78	8.760	2536	2541	2542	rBV2	380	275	0.03%	0.003%
79	8.812	2554	2557	2565	rVB2	504	486	0.05%	0.006%
80	8.953	2596	2601	2604	rBV3	336	318	0.03%	0.004%
81	9.091	2631	2644	2671	rBV	496995	876662	88.70%	10.493%
82	9.249	2690	2693	2694	rBV2	375	201	0.02%	0.002%
83	9.378	2729	2733	2734	rBV3	573	420	0.04%	0.005%
84	9.474	2757	2763	2765	rBV2	328	351	0.04%	0.004%
85	9.619	2804	2808	2810	rBV2	441	316	0.03%	0.004%
86	9.651	2816	2818	2820	rVB2	450	192	0.02%	0.002%
87	10.294	3015	3018	3019	rBV2	284	158	0.02%	0.002%
88	10.435	3050	3062	3082	rVB	299389	478817	48.45%	5.731%
89	10.870	3192	3197	3200	rBV3	459	457	0.05%	0.005%
90	11.027	3243	3246	3248	rBV3	549	314	0.03%	0.004%
91	11.288	3324	3327	3331	rBV2	460	423	0.04%	0.005%
92	11.423	3361	3369	3377	rBV4	4181	6076	0.61%	0.073%
93	11.487	3377	3389	3412	rVV	453333	800661	81.01%	9.584%
94	11.863	3494	3506	3532	rBV	426123	752441	76.13%	9.006%
95	12.117	3582	3585	3586	rBV	500	266	0.03%	0.003%
96	13.509	4007	4018	4035	rBV	73116	123287	12.47%	1.476%


Sum of corrected areas: 8354539

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080718\
Data File : VU025963.D
Acq On : 08 Aug 2018 01:45
Operator : MD/SY
Sample : J4361-21
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
A4ZA3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

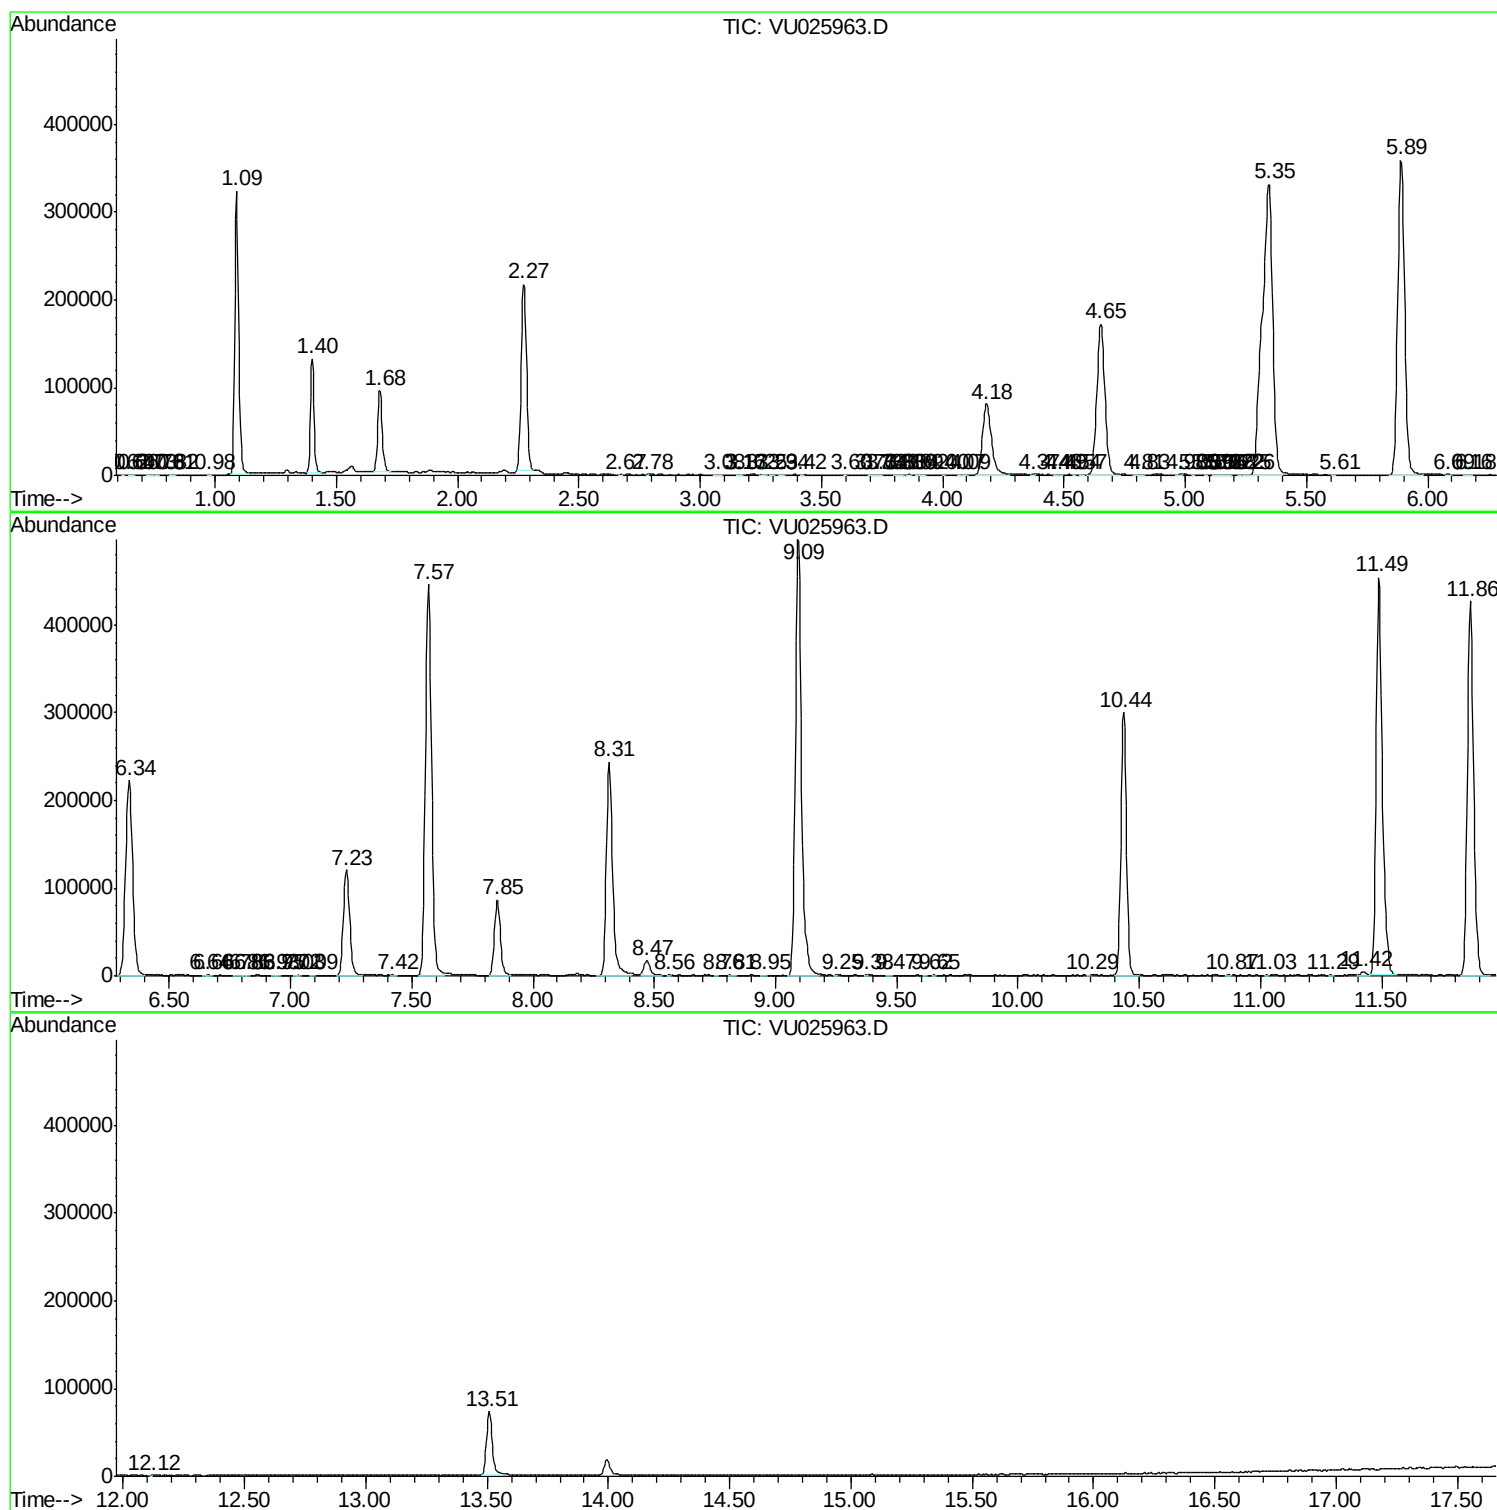

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080718\
Data File : VU025963.D
Acq On : 08 Aug 2018 01:45
Operator : MD/SY
Sample : J4361-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZA3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080718\
Data File : VU025963.D
Acq On : 08 Aug 2018 01:45
Operator : MD/SY
Sample : J4361-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZA3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc