


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU080718\
Data File : VU025932.D
Acq On : 07 Aug 2018 10:11
Operator : MD/SY
Sample : BFB40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB40

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080718WMA.M
Title : VOC Analysis
Last Update : Thu Aug 09 01:19:52 2018

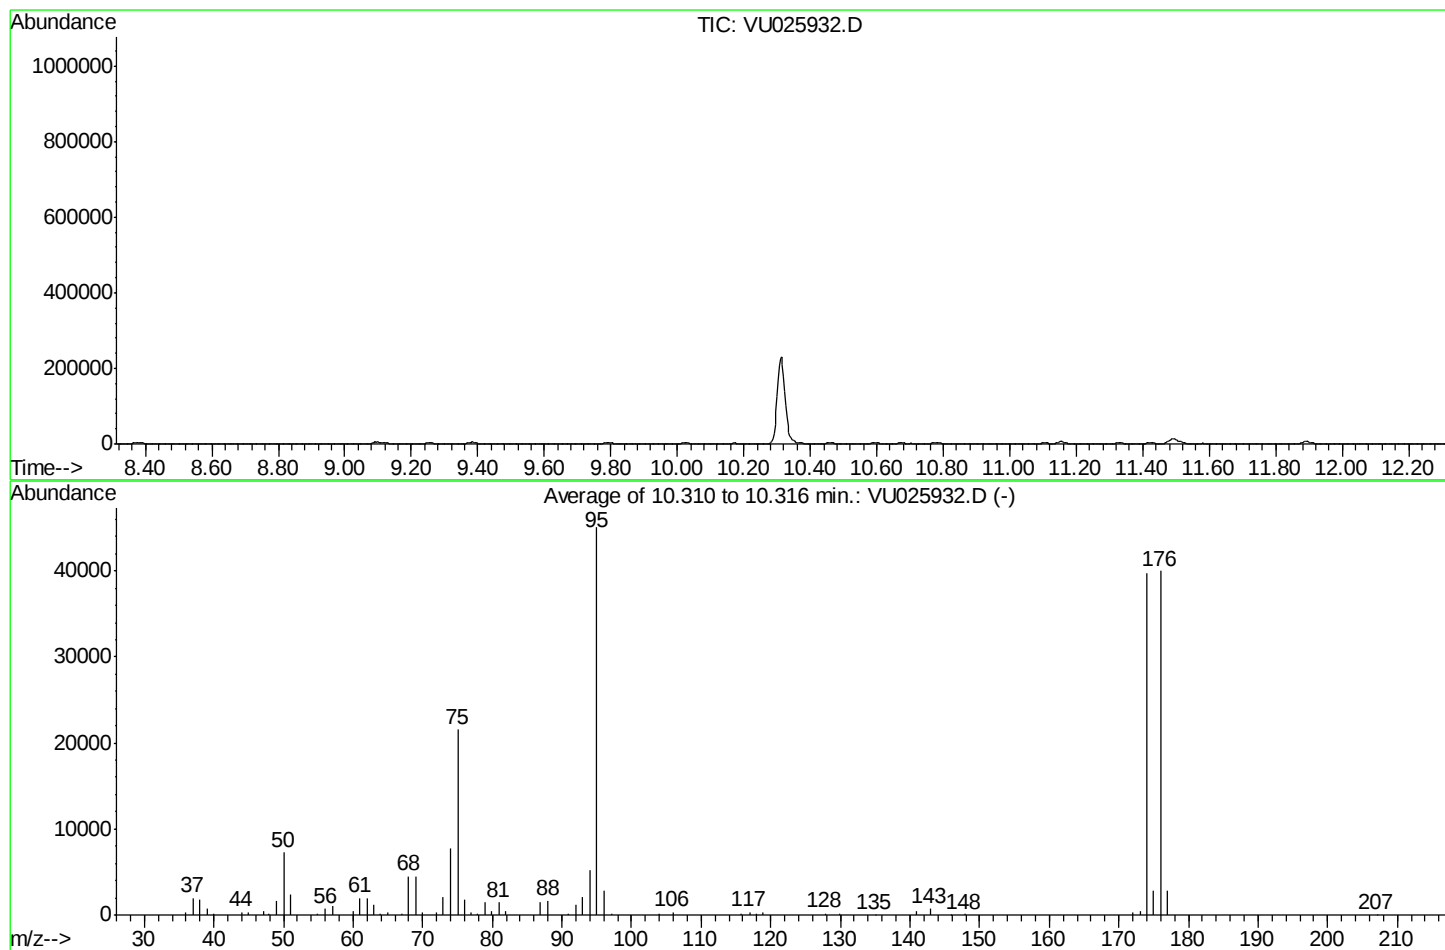

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	7229	PASS
75	95	30	80	47.8	21544	PASS
95	95	100	100	100.0	45064	PASS
96	95	5	9	6.2	2816	PASS
173	174	0.00	2	1.0	417	PASS
174	95	50	120	88.2	39733	PASS
175	174	5	9	7.1	2821	PASS
176	174	95	101	100.7	40002	PASS
177	176	5	9	7.0	2792	PASS

Scan 3011 (10.271 min): VU025932.D
BFB40

m/z	Abundance
40.00	126.0
43.90	442.0
207.00	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	322.0
37.00	2166.0
38.00	1693.0
39.00	743.0
40.00	246.0
44.00	804.0
45.00	374.0
47.00	430.0
47.90	159.0
49.00	1735.0
50.00	7619.0
51.10	2556.0
55.00	100.0
56.10	734.0
57.10	1192.0
59.90	456.0
61.00	2076.0
62.00	2046.0
63.00	1201.0
63.80	155.0
65.10	245.0
67.00	176.0
68.00	4559.0
69.00	4593.0
69.90	361.0
71.90	254.0
73.00	2153.0
74.00	7938.0
75.00	22528.0
76.00	1875.0
76.90	306.0
77.90	100.0
78.90	1439.0
79.90	522.0
80.90	1607.0
81.90	465.0
86.90	1465.0
88.00	1820.0
91.00	248.0
91.90	1090.0
93.00	2144.0
94.00	5320.0
95.00	45560.0
96.00	2966.0
97.10	105.0
104.00	179.0
105.90	305.0
115.80	178.0
117.00	344.0
117.90	204.0
118.80	276.0
127.90	193.0
129.90	151.0
135.00	101.0
141.00	489.0
142.90	720.0
147.80	206.0
171.90	286.0
173.10	471.0
174.00	39624.0
175.00	2902.0
176.00	40136.0
176.90	2747.0
207.10	189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	380.0
37.00	2049.0
38.00	1828.0
39.00	720.0
40.10	257.0
44.00	858.0
45.00	360.0
47.10	468.0
47.90	161.0
49.00	1627.0
50.00	7400.0
51.10	2419.0
54.90	123.0
56.10	718.0
57.10	1147.0
59.90	442.0
61.00	2045.0
62.00	1969.0
63.00	1239.0
63.90	145.0
65.00	237.0
66.90	133.0
68.00	4639.0
69.00	4518.0
70.00	342.0
71.90	258.0
73.00	2213.0
74.00	8104.0
75.00	21976.0
76.00	1828.0
76.90	268.0
77.90	105.0
78.90	1481.0
79.90	459.0
80.90	1510.0
81.90	515.0
86.90	1441.0
88.00	1778.0
91.00	191.0
92.00	1162.0
93.00	2169.0
94.00	5377.0
95.00	46496.0
96.00	2827.0
97.10	133.0
104.00	208.0
105.90	310.0
115.80	191.0
117.00	373.0
117.80	176.0
118.90	268.0
127.90	173.0
130.00	178.0
135.00	107.0
141.00	523.0
142.90	716.0
147.90	183.0
171.90	309.0
173.10	425.0
174.00	40920.0
175.00	2897.0
176.00	41312.0
177.00	2890.0
207.10	193.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	362.0
37.00	1763.0
38.00	1732.0
39.00	657.0
40.10	204.0
44.00	764.0
45.00	311.0
47.10	460.0
47.90	164.0
49.00	1487.0
50.00	6670.0
51.00	2136.0
54.90	131.0
56.00	585.0
57.00	960.0
60.00	355.0
60.90	1913.0
62.00	1751.0
63.00	1208.0
64.00	124.0
65.00	207.0
68.00	4365.0
69.00	4170.0
70.00	322.0
72.00	233.0
72.90	2002.0
74.00	7245.0
75.00	20128.0
76.00	1626.0
77.00	247.0
77.80	127.0
78.90	1342.0
79.90	354.0
81.00	1329.0
81.90	440.0
86.90	1372.0
88.00	1510.0
90.90	155.0
92.10	1164.0
93.00	1989.0
94.00	5123.0
95.00	43136.0
96.00	2656.0
97.10	132.0
104.00	203.0
105.90	286.0
115.80	173.0
116.90	386.0
117.80	133.0
118.90	261.0
127.80	173.0
130.00	186.0
140.90	499.0
142.90	634.0
145.90	117.0
172.00	302.0
173.10	357.0
174.00	38656.0
175.00	2665.0
176.00	38560.0
177.00	2741.0
207.10	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40