

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080719\
 Data File : VU033622.D
 Acq On : 07 Aug 2019 17:17
 Operator : JC/SP
 Sample : K4202-06DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2B23DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	87	94	107	rBV	139564	156120	15.04%	1.811%
2	1.672	173	181	195	rVB	126660	159547	15.37%	1.851%
3	2.260	353	364	377	rVB	222447	337063	32.47%	3.910%
4	2.534	446	449	452	rBV2	406	259	0.02%	0.003%
5	2.643	480	483	487	rBV2	268	195	0.02%	0.002%
6	2.688	491	497	504	rVB3	713	1093	0.11%	0.013%
7	2.820	526	538	550	rBV2	3358	6906	0.67%	0.080%
8	2.874	552	555	559	rVB	277	195	0.02%	0.002%
9	2.968	577	584	595	rVB4	1125	2003	0.19%	0.023%
10	3.019	596	600	603	rVB	210	159	0.02%	0.002%
11	3.337	693	699	703	rBV2	148	197	0.02%	0.002%
12	3.466	736	739	743	rBV2	246	157	0.02%	0.002%
13	3.530	753	759	762	rBV2	212	202	0.02%	0.002%
14	3.550	762	765	768	rBV2	153	140	0.01%	0.002%
15	4.154	940	953	960	rBV	111781	260783	25.12%	3.025%
16	4.556	1074	1078	1081	rBV3	157	168	0.02%	0.002%
17	4.624	1082	1099	1123	rVV2	182679	433947	41.80%	5.033%
18	4.845	1165	1168	1169	rBV2	238	159	0.02%	0.002%
19	4.964	1197	1205	1208	rBV3	390	456	0.04%	0.005%
20	5.087	1239	1243	1247	rBV2	271	243	0.02%	0.003%
21	5.119	1250	1253	1255	rVV	209	157	0.02%	0.002%
22	5.161	1263	1266	1271	rVB2	245	231	0.02%	0.003%
23	5.190	1271	1275	1277	rBV2	184	142	0.01%	0.002%
24	5.318	1291	1315	1348	rBV2	343165	1038163	100.00%	12.042%
25	5.472	1359	1363	1365	rBV2	499	374	0.04%	0.004%
26	5.649	1414	1418	1432	rVB3	575	921	0.09%	0.011%
27	5.730	1440	1443	1445	rBV	480	273	0.03%	0.003%
28	5.743	1445	1447	1449	rVV	266	153	0.01%	0.002%
29	5.759	1449	1452	1456	rVB2	253	180	0.02%	0.002%
30	5.865	1472	1485	1514	rBV	341237	672174	64.75%	7.796%
31	6.035	1536	1538	1542	rVB2	361	177	0.02%	0.002%
32	6.167	1566	1579	1603	rBV2	91181	184835	17.80%	2.144%
33	6.247	1603	1604	1608	rVB	366	172	0.02%	0.002%
34	6.308	1609	1623	1644	rBV	238481	481494	46.38%	5.585%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080719\
 Data File : VU033622.D
 Acq On : 07 Aug 2019 17:17
 Operator : JC/SP
 Sample : K4202-06DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2B23DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080519WMA.M
 Title : VOC Analysis

35	6.440	1660	1664	1665	rBV2	348	269	0.03%	0.003%
36	6.476	1672	1675	1678	rVB4	647	444	0.04%	0.005%
37	6.514	1685	1687	1692	rVV2	244	189	0.02%	0.002%
38	6.591	1708	1711	1716	rVV2	175	189	0.02%	0.002%
39	6.614	1716	1718	1724	rVB	233	154	0.01%	0.002%
40	6.845	1787	1790	1791	rVV2	262	178	0.02%	0.002%
41	6.861	1792	1795	1799	rVV2	668	607	0.06%	0.007%
42	6.878	1799	1800	1806	rVV2	382	368	0.04%	0.004%
43	6.906	1806	1809	1812	rVV2	312	260	0.03%	0.003%
44	6.952	1818	1823	1828	rVB2	248	242	0.02%	0.003%
45	7.209	1892	1903	1928	rBV2	124625	230695	22.22%	2.676%
46	7.546	1995	2008	2026	rBV	430337	753362	72.57%	8.738%
47	7.723	2060	2063	2065	rBV	344	236	0.02%	0.003%
48	7.832	2086	2097	2119	rBV	89745	159410	15.36%	1.849%
49	8.093	2175	2178	2180	rVV	288	209	0.02%	0.002%
50	8.122	2184	2187	2190	rVV2	201	164	0.02%	0.002%
51	8.164	2193	2200	2203	rVV2	969	1200	0.12%	0.014%
52	8.212	2206	2215	2225	rVB3	11388	19920	1.92%	0.231%
53	8.296	2230	2241	2276	rBV	348891	636896	61.35%	7.387%
54	8.607	2331	2338	2345	rBV4	1390	1953	0.19%	0.023%
55	8.713	2369	2371	2375	rBV2	153	151	0.01%	0.002%
56	8.823	2402	2405	2409	rBV2	261	188	0.02%	0.002%
57	8.903	2424	2430	2432	rBV2	233	253	0.02%	0.003%
58	9.000	2455	2460	2463	rBV2	228	248	0.02%	0.003%
59	9.070	2470	2482	2525	rBV	516568	871156	83.91%	10.104%
60	9.270	2542	2544	2548	rVB	373	209	0.02%	0.002%
61	9.331	2558	2563	2564	rBV	325	218	0.02%	0.003%
62	9.366	2571	2574	2577	rBV	482	228	0.02%	0.003%
63	9.456	2596	2602	2608	rBV2	345	428	0.04%	0.005%
64	9.540	2624	2628	2639	rVB2	238	251	0.02%	0.003%
65	9.585	2639	2642	2647	rBV2	292	221	0.02%	0.003%
66	9.640	2654	2659	2664	rBV2	254	288	0.03%	0.003%
67	9.723	2683	2685	2692	rVB2	159	163	0.02%	0.002%
68	9.758	2692	2696	2698	rBV2	212	153	0.01%	0.002%
69	10.080	2793	2796	2799	rVB3	338	201	0.02%	0.002%
70	10.244	2843	2847	2853	rBV	367	385	0.04%	0.004%
71	10.347	2875	2879	2883	rBV	298	243	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080719\
 Data File : VU033622.D
 Acq On : 07 Aug 2019 17:17
 Operator : JC/SP
 Sample : K4202-06DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2B23DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080519WMA.M
 Title : VOC Analysis

72	10.414	2887	2900	2920	rVV	393092	624616	60.17%	7.245%
73	10.585	2951	2953	2956	rBV	366	296	0.03%	0.003%
74	10.649	2970	2973	2975	rBV3	260	177	0.02%	0.002%
75	10.675	2979	2981	2986	rVB2	327	164	0.02%	0.002%
76	10.701	2986	2989	2991	rBV2	194	149	0.01%	0.002%
77	10.746	2998	3003	3006	rVB2	283	213	0.02%	0.002%
78	10.794	3015	3018	3020	rBV2	246	157	0.02%	0.002%
79	11.022	3086	3089	3097	rBV2	245	221	0.02%	0.003%
80	11.083	3104	3108	3112	rBV	267	236	0.02%	0.003%
81	11.164	3131	3133	3138	rVB2	244	209	0.02%	0.002%
82	11.202	3140	3145	3152	rBV2	305	425	0.04%	0.005%
83	11.244	3156	3158	3160	rVV2	325	185	0.02%	0.002%
84	11.273	3164	3167	3169	rBV	248	167	0.02%	0.002%
85	11.305	3174	3177	3179	rVB	312	168	0.02%	0.002%
86	11.411	3208	3210	3214	rBV2	255	175	0.02%	0.002%
87	11.466	3215	3227	3257	rBV	489028	785519	75.66%	9.111%
88	11.787	3325	3327	3330	rVB2	351	181	0.02%	0.002%
89	11.842	3330	3344	3363	rBV	480365	783630	75.48%	9.089%
90	12.080	3416	3418	3423	rVB4	651	429	0.04%	0.005%
91	12.231	3461	3465	3467	rBV2	530	307	0.03%	0.004%
92	12.266	3473	3476	3480	rBV2	475	323	0.03%	0.004%
93	12.286	3480	3482	3485	rVB2	431	262	0.03%	0.003%
94	12.308	3485	3489	3490	rBV2	361	261	0.03%	0.003%
95	12.459	3533	3536	3541	rBV2	356	294	0.03%	0.003%
96	12.630	3586	3589	3593	rBV	295	243	0.02%	0.003%
97	12.999	3702	3704	3707	rBV	311	164	0.02%	0.002%
98	13.057	3719	3722	3726	rBV3	370	300	0.03%	0.003%
99	13.762	3939	3941	3947	rBV	406	342	0.03%	0.004%
100	15.006	4326	4328	4330	rBV2	604	342	0.03%	0.004%


Sum of corrected areas: 8621522

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080719\
Data File : VU033622.D
Acq On : 07 Aug 2019 17:17
Operator : JC/SP
Sample : K4202-06DL 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B23DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

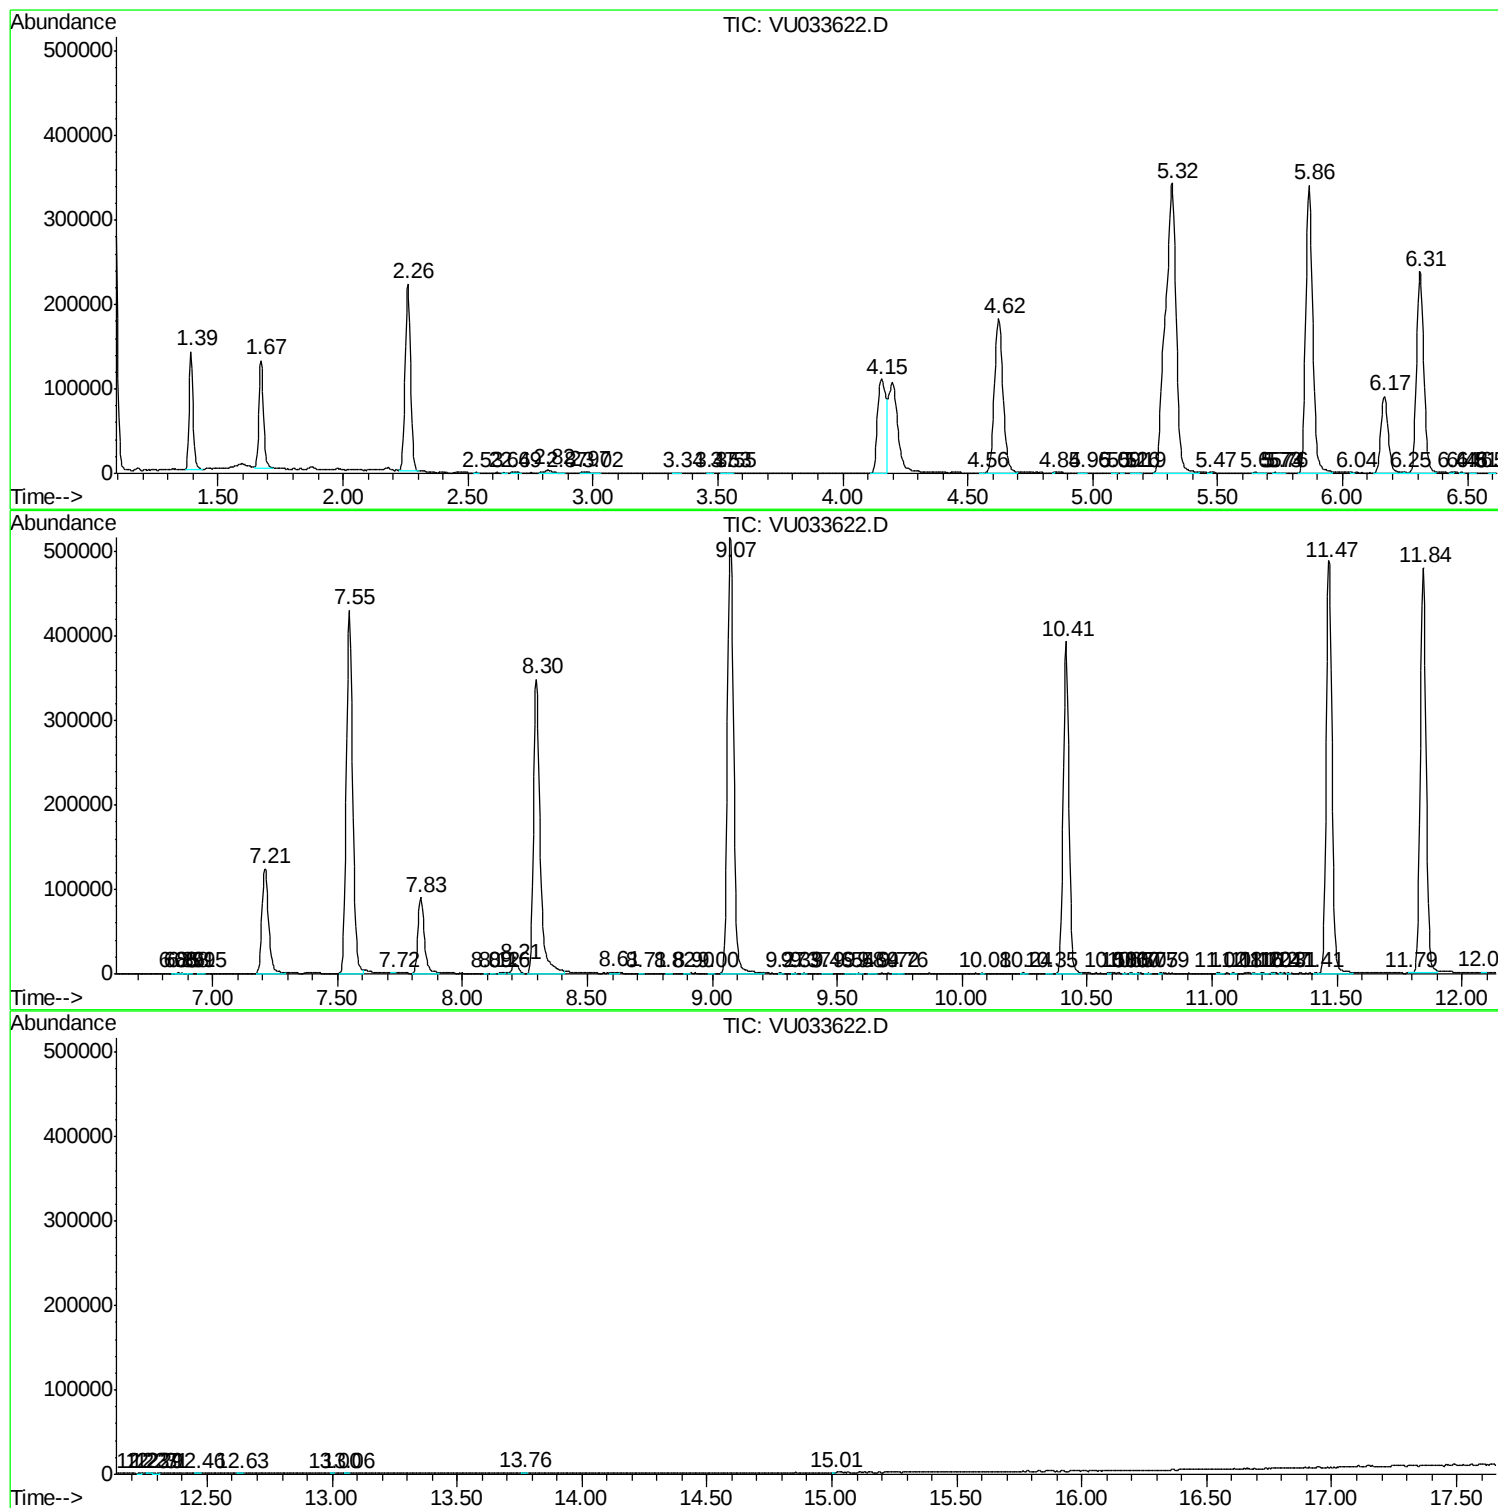

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080719\
Data File : VU033622.D
Acq On : 07 Aug 2019 17:17
Operator : JC/SP
Sample : K4202-06DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B23DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080719\
Data File : VU033622.D
Acq On : 07 Aug 2019 17:17
Operator : JC/SP
Sample : K4202-06DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B23DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc