


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080719\
 Data File : VU033612.D
 Acq On : 07 Aug 2019 08:27
 Operator : JC/SP
 Sample : BFB49
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB49

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080519WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 08 13:44:11 2019

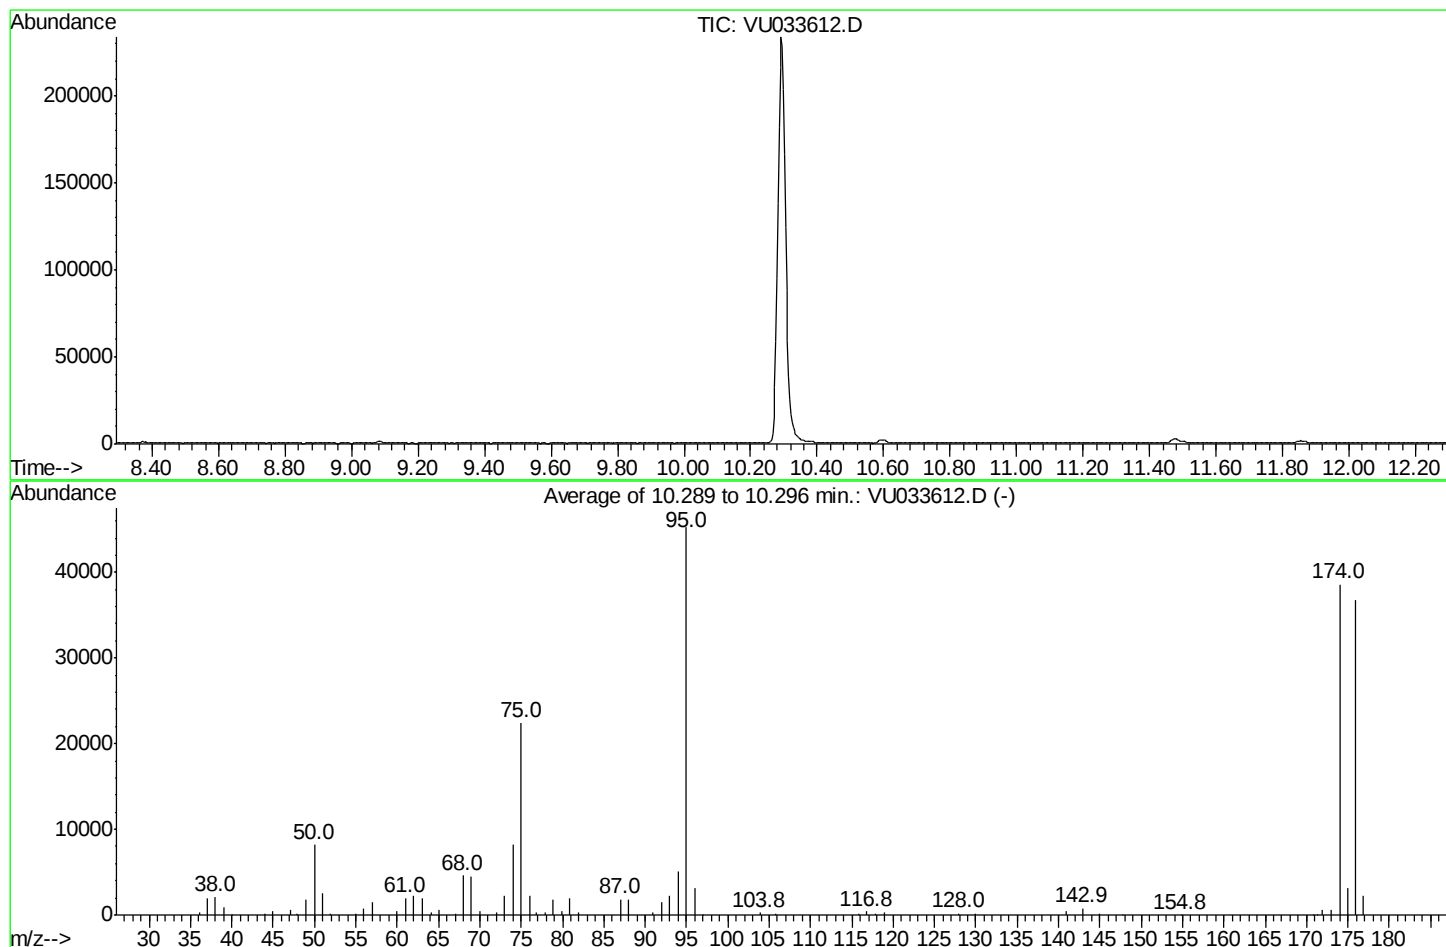

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	8173	PASS
75	95	30	80	49.6	22461	PASS
95	95	100	100	100.0	45256	PASS
96	95	5	9	7.0	3146	PASS
173	174	0.00	2	1.6	614	PASS
174	95	50	120	85.3	38584	PASS
175	174	5	9	8.2	3161	PASS
176	174	95	101	95.3	36757	PASS
177	176	5	9	6.3	2301	PASS

m/z	Abundance
36.10	339.0
37.00	1970.0
38.00	2148.0
39.00	967.0
40.00	160.0
44.00	640.0
45.00	557.0
47.00	536.0
47.90	212.0
49.00	1770.0
50.00	8442.0
51.00	2561.0
52.00	145.0
54.90	183.0
56.00	859.0
57.00	1575.0
60.00	466.0
61.00	2019.0
62.00	2255.0
63.00	2027.0
64.10	314.0
65.00	593.0
67.00	169.0
68.00	4811.0
69.00	4625.0
70.10	425.0
72.00	260.0
73.00	2314.0
74.00	8537.0
75.00	23184.0
76.00	2251.0
76.90	293.0
77.90	266.0
78.90	1854.0
79.90	452.0
80.90	1975.0
82.00	280.0
87.00	1841.0
88.00	1727.0
90.90	284.0
92.00	1526.0
93.00	2348.0
94.00	5201.0
95.00	46768.0
96.00	3237.0
103.90	299.0
105.90	179.0
115.80	180.0
116.80	480.0
117.80	188.0
118.90	305.0
128.00	227.0
129.90	180.0
140.90	408.0
142.90	835.0
145.00	232.0
154.80	103.0
170.80	106.0
171.90	559.0
173.00	862.0
174.00	39736.0
175.00	3278.0
175.90	37944.0
176.90	2372.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.10	340.0
37.00	1750.0
38.00	1905.0
39.00	895.0
39.90	178.0
44.00	588.0
45.00	505.0
47.10	587.0
47.90	188.0
49.00	1732.0
50.00	8176.0
51.00	2400.0
52.00	141.0
54.90	185.0
56.00	778.0
57.00	1391.0
60.00	401.0
61.00	1997.0
62.00	2169.0
63.00	1975.0
64.10	287.0
65.00	513.0
67.00	185.0
68.00	4335.0
69.00	4338.0
70.10	368.0
72.00	226.0
73.00	2129.0
74.00	8179.0
75.00	21712.0
76.00	2158.0
76.90	258.0
77.90	248.0
78.90	1678.0
79.90	392.0
80.90	1713.0
82.00	315.0
87.00	1939.0
88.00	1800.0
91.00	266.0
92.00	1360.0
93.00	2088.0
94.00	4863.0
95.00	43496.0
96.00	3053.0
97.00	125.0
103.80	292.0
105.90	158.0
115.80	201.0
116.80	369.0
117.80	182.0
119.00	327.0
128.00	186.0
130.00	131.0
140.90	418.0
142.90	751.0
145.00	197.0
154.80	109.0
170.70	108.0
171.90	454.0
174.00	36208.0
175.00	3009.0
175.90	34912.0
176.90	2204.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

Scan 2850 (10.254 min): VU033612.D
BFB49

m/z	Abundance
40.00	159.0
44.00	483.0
207.00	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.00	347.0
37.00	2004.0
38.00	2263.0
39.00	946.0
40.10	152.0
44.00	627.0
45.00	471.0
47.00	479.0
47.90	231.0
49.00	1683.0
50.00	7901.0
51.00	2568.0
51.90	126.0
55.00	139.0
56.00	827.0
57.00	1457.0
60.00	500.0
61.00	2001.0
62.00	2269.0
63.00	1820.0
64.10	330.0
65.00	639.0
67.00	148.0
68.00	4666.0
69.00	4387.0
70.00	420.0
72.00	257.0
73.00	2238.0
74.00	7931.0
75.00	22488.0
76.00	2110.0
76.90	260.0
77.90	253.0
78.90	1833.0
79.90	463.0
80.90	1950.0
81.90	241.0
87.00	1766.0
88.00	1661.0
90.90	245.0
91.90	1512.0
93.00	2312.0
94.00	5149.0
95.00	45504.0
96.00	3149.0
103.90	293.0
105.80	194.0
115.90	172.0
116.80	464.0
117.80	176.0
118.90	264.0
127.90	227.0
129.80	193.0
140.90	412.0
142.90	762.0
145.00	231.0
147.70	112.0
171.20	171.0
172.00	660.0
173.00	980.0
174.00	39808.0
175.00	3198.0
176.00	37416.0
176.90	2327.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49