

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080720\
 Data File : VU039789.D
 Acq On : 07 Aug 2020 16:06
 Operator : SY/MD
 Sample : L3572-05DL 4X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 08 03:34:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 08 03:30:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	72359	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	69802	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	31207	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	16209	4.15	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.00%
7) Chloroethane-d5	1.92	69	18019	4.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.20%
11) 1,1-Dichloroethene-d2	2.58	63	22755	2.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.80%#
20) 2-Butanone-d5	4.65	46	85618	49.82	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.64%
24) Chloroform-d	5.08	84	43889	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.00%
26) 1,2-Dichloroethane-d4	5.72	65	26466	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
32) Benzene-d6	5.74	84	71532	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.20%
36) 1,2-Dichloropropane-d6	6.70	67	26243	4.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.20%
41) Toluene-d8	7.91	98	54342	3.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.80%
43) trans-1,3-Dichloropropene-	8.19	79	8704	3.99	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.80%
46) 2-Hexanone-d5	8.64	63	58572	49.64	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.28%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	25012	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	26506	4.96	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.20%

Target Compounds


					Ovalue
3) Chloromethane	1.53	50	603	0.098	ug/L 91
5) Vinyl chloride	1.61	62	32449	5.515	ug/L 99
16) Methylene chloride	3.06	84	5599	0.805	ug/L 94
22) cis-1,2-Dichloroethene	4.69	96	35154	6.726	ug/L 94
35) Methylcyclohexane	6.70	83	6325	0.802	ug/L # 20
37) 1,2-Dichloropropane	6.70	63	3353	0.664	ug/L # 86
39) cis-1,3-Dichloropropene	7.58	75	781	0.113	ug/L # 70
59) 1,2,3-Trichloropropane	11.81	75	4073	1.118	ug/L # 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080720\
Data File : VU039789.D
Acq On : 07 Aug 2020 16:06
Operator : SY/MD
Sample : L3572-05DL 4X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Aug 08 03:34:06 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 08 03:30:58 2020
Response via : Initial Calibration




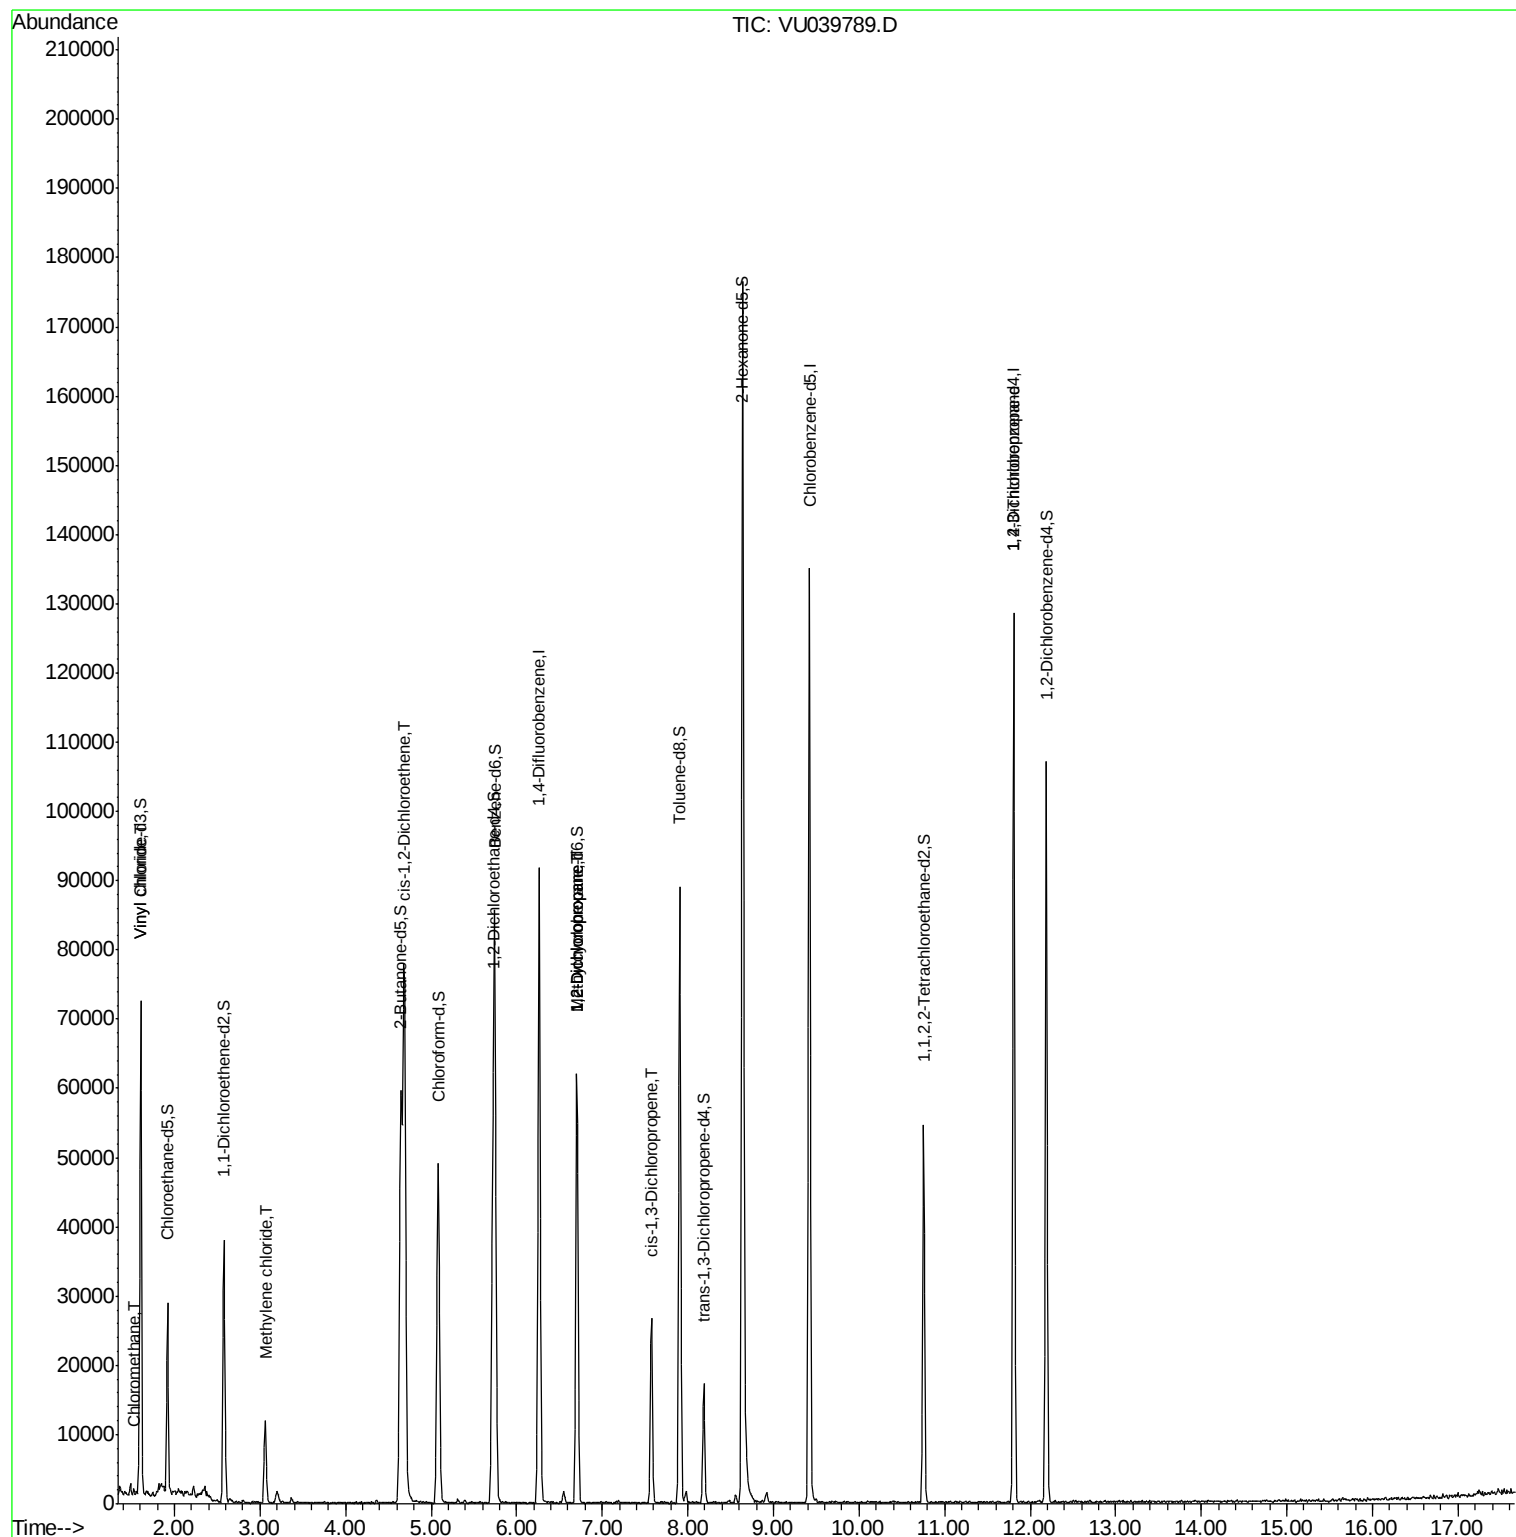


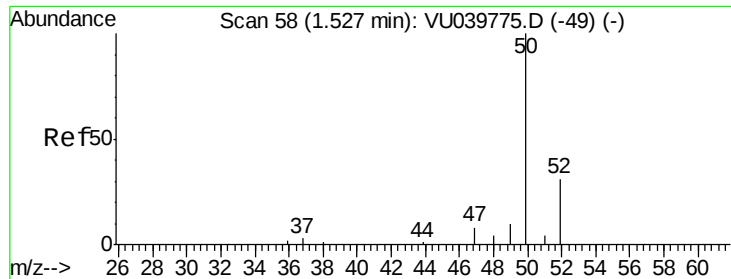

#3
Chloromethane
Concen: 0.098 ug/L
RT: 1.53 min Scan# 58
Delta R.T. -0.00 min
Lab File: VU039789.D
Acq: 07 Aug 2020 16:06




Instrument :
MSVOA_U
ClientSampleId :


Tot Ion: 50 Resp: 603
Ion Ratio Lower Upper
50 100
52 25.6 21.6 40.0

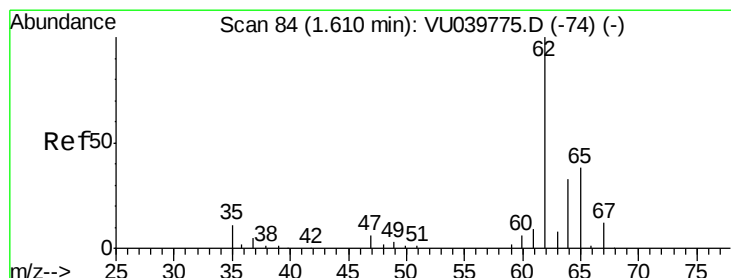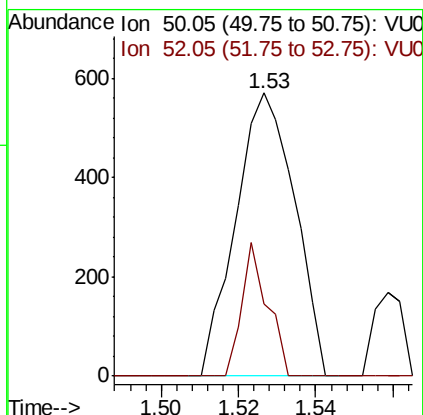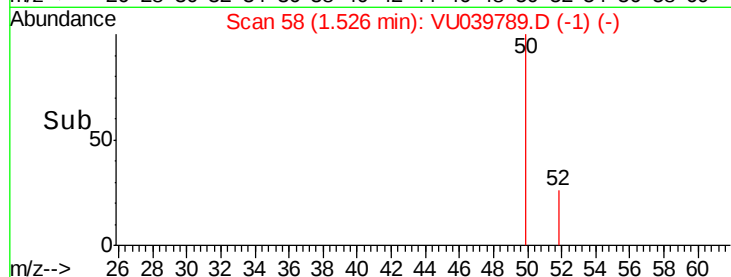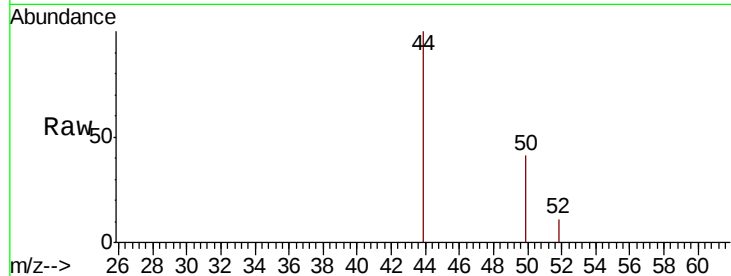

#5
Vinyl chloride
Concen: 5.515 ug/L
RT: 1.61 min Scan# 84
Delta R.T. -0.00 min
Lab File: VU039789.D
Acq: 07 Aug 2020 16:06

Tgt Ion: 62 Resp: 32449
Ion Ratio Lower Upper
62 100
64 33.7 24.1 44.7

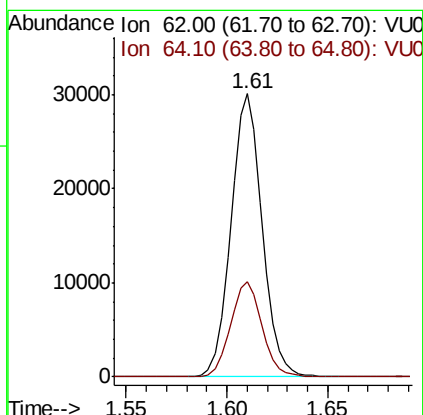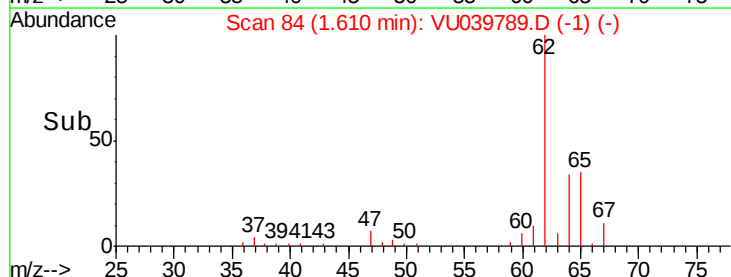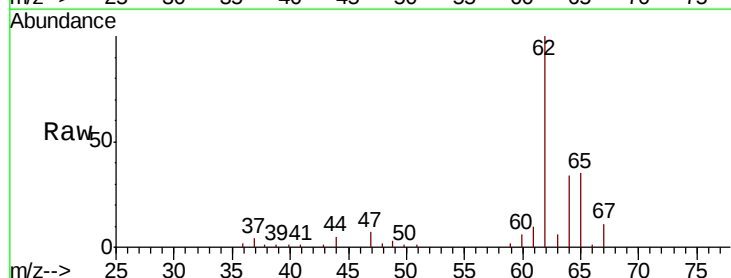

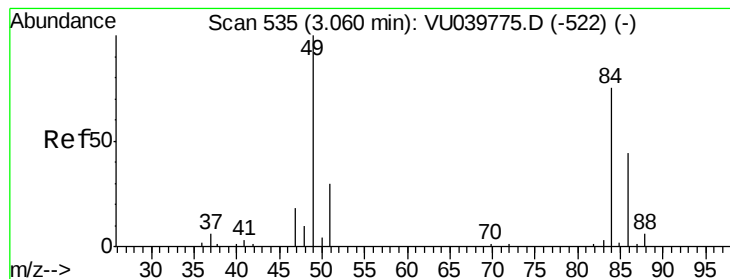

#16

Methylene chloride

Concen: 0.805 ug/L

RT: 3.06 min Scan# 535

Delta R.T. -0.00 min

Lab File: VU039789.D

Acq: 07 Aug 2020 16:06

Instrument :

MSVOA_U

ClientSampleId :


Tot Ion: 84 Resp: 5599

Ion Ratio Lower Upper

84 100

86 58.6 43.9 81.5




49 126.5 94.4 175.4

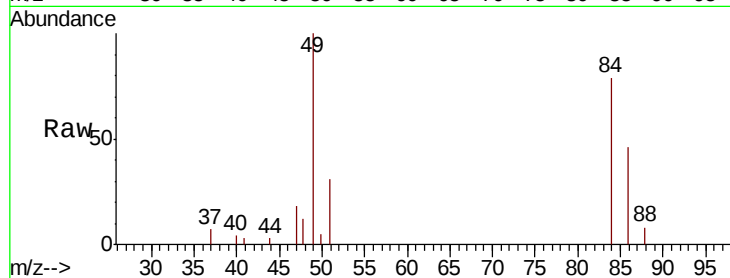

Abundance Ion 84.05 (83.75 to 84.75): VU039775.D (-522) (-)

Ion 86.00 (85.70 to 86.70): VU039775.D (-522) (-)

Ion 49.10 (48.80 to 49.80): VU039775.D (-522) (-)

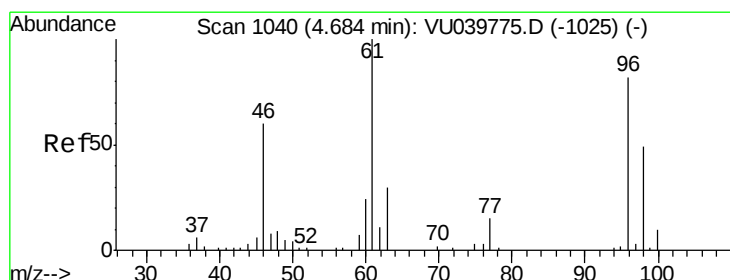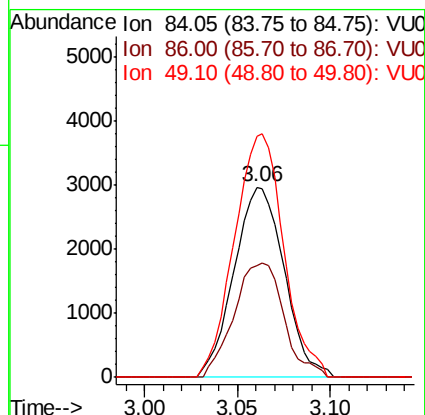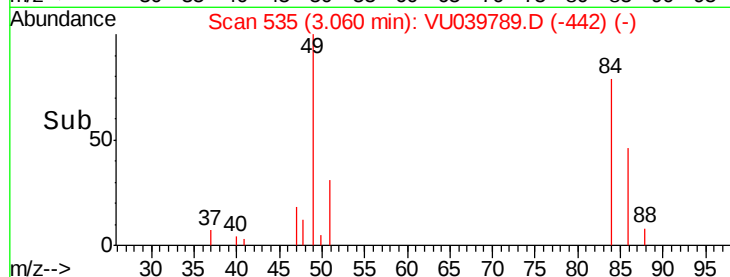

#22

cis-1,2-Dichloroethene

Concen: 6.726 ug/L

RT: 4.69 min Scan# 1041

Delta R.T. 0.00 min

Lab File: VU039789.D

Acq: 07 Aug 2020 16:06


Tgt Ion: 96 Resp: 35154

Ion Ratio Lower Upper

96 100

61 132.0 87.4 162.2



68 0.0 0.0 0.0

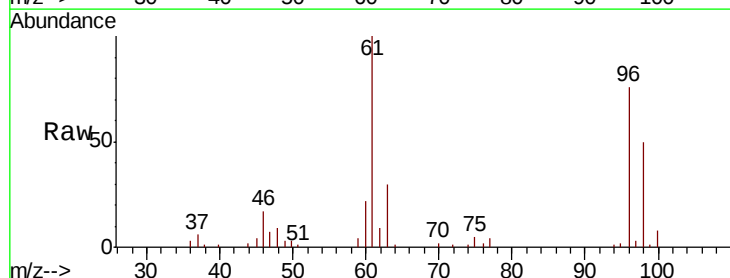


Abundance Ion 96.00 (95.70 to 96.70): VU039775.D (-1025) (-)

Ion 61.05 (60.75 to 61.75): VU039775.D (-1025) (-)

Ion 68.15 (67.85 to 68.85): VU039775.D (-1025) (-)

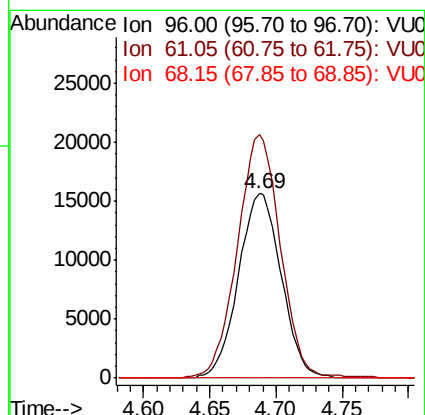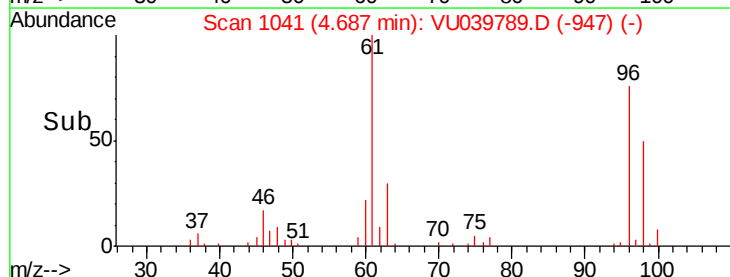


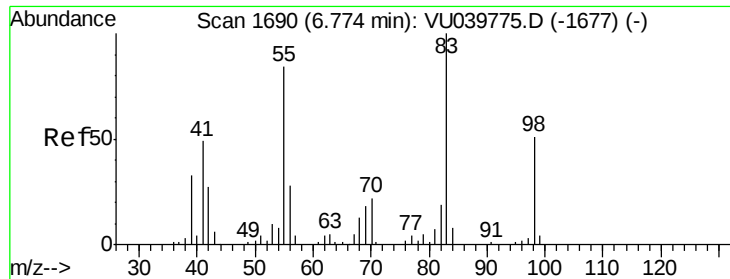




#35
Methylcyclohexane
Concen: 0.802 ug/L
RT: 6.70 min Scan# 1668
Delta R.T. -0.07 min
Lab File: VU039789.D
Acq: 07 Aug 2020 16:06

Instrument :
MSVOA_U
ClientSampleId :

Tot Ion: 83 Resp: 6325
Ion Ratio Lower Upper
83 100
55 0.0 59.4 89.0#
98 2.3 39.0 58.4#

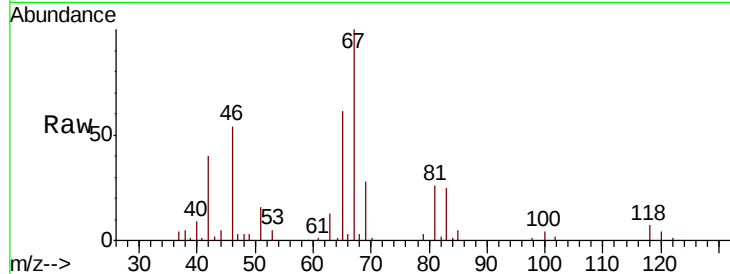


Abundance Ion 83.15 (82.85 to 83.85): VU0
Ion 55.10 (54.80 to 55.80): VU0
Ion 98.15 (97.85 to 98.85): VU0

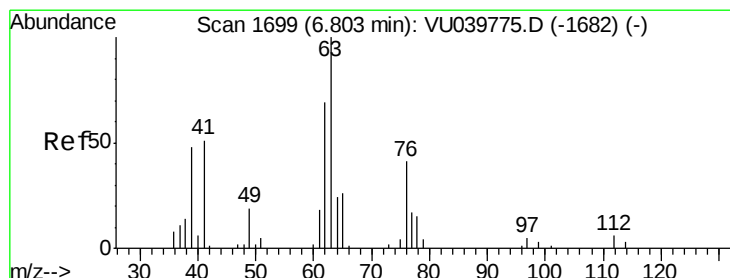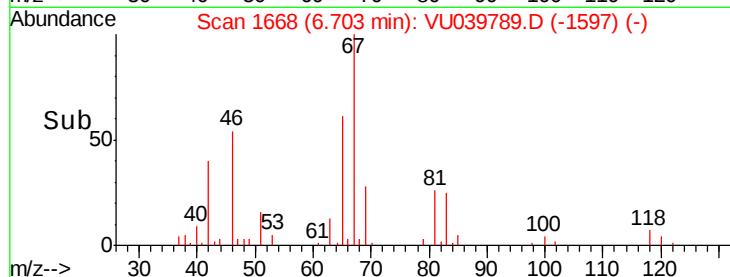
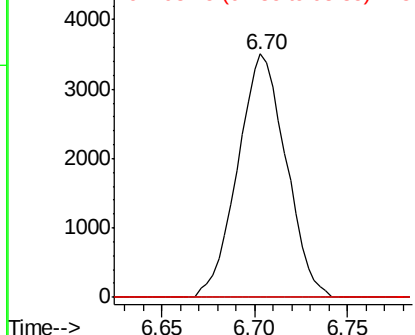



#37
1,2-Dichloropropane
Concen: 0.664 ug/L
RT: 6.70 min Scan# 1668
Delta R.T. -0.10 min
Lab File: VU039789.D
Acq: 07 Aug 2020 16:06

Tgt Ion: 63 Resp: 3353
Ion Ratio Lower Upper
63 100
112 0.0 3.8 5.6#

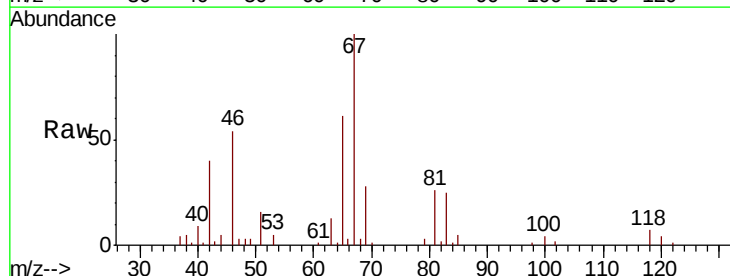

Abundance Ion 63.10 (62.80 to 63.80): VU0
Ion 112.10 (111.80 to 112.80): V



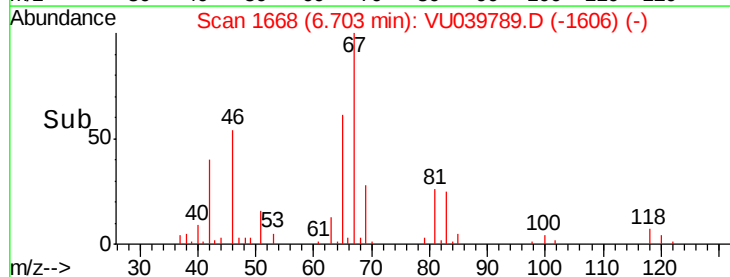
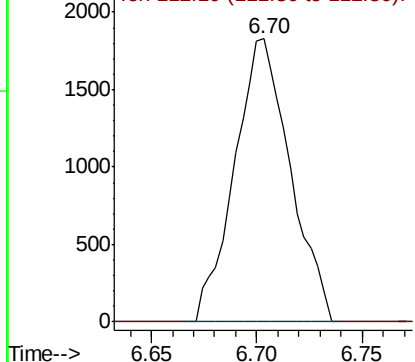


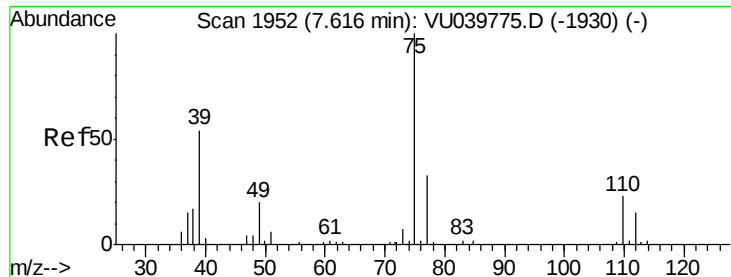

#39
 cis-1,3-Dichloropropene
 Concen: 0.113 ug/L
 RT: 7.58 min Scan# 1940
 Delta R.T. -0.04 min
 Lab File: VU039789.D
 Acq: 07 Aug 2020 16:06

Instrument :
 MSVOA_U
 ClientSampleId :

Tot Ion: 75 Resp: 781
 Ion Ratio Lower Upper
 75 100
 77 48.5 22.4 41.6#

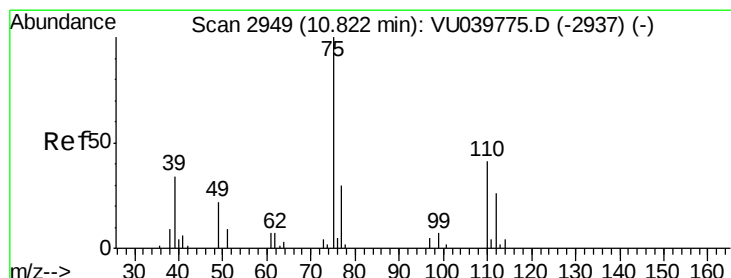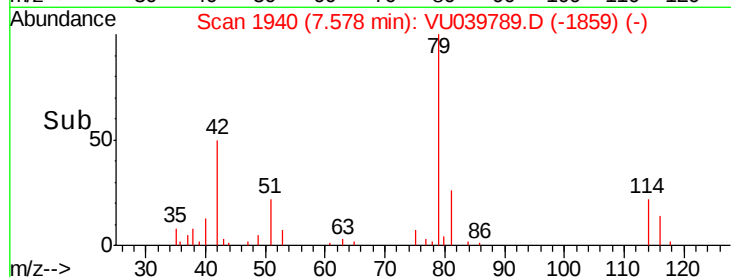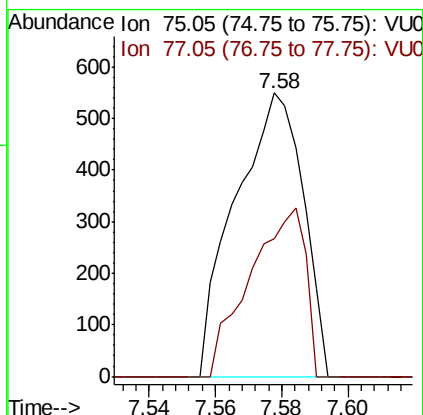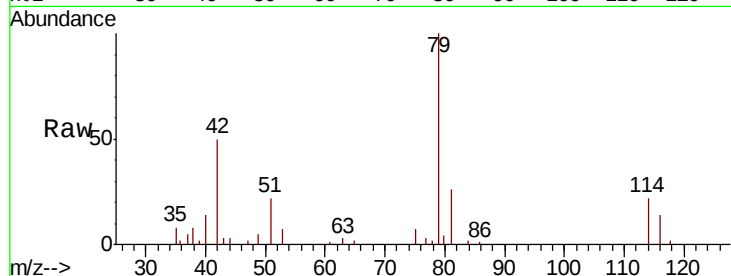

#59
 1,2,3-Trichloropropane
 Concen: 1.118 ug/L
 RT: 11.81 min Scan# 3255
 Delta R.T. 0.98 min
 Lab File: VU039789.D
 Acq: 07 Aug 2020 16:06

Tgt Ion: 75 Resp: 4073
 Ion Ratio Lower Upper
 75 100
 77 42.7 24.6 37.0#

