


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080720\
Data File : VU039779.D
Acq On : 07 Aug 2020 12:04
Operator : SY/MD
Sample : L3572-20
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Aug 08 03:59:10 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 08 03:30:58 2020
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
F2L87

Manual Integrations
APPROVED

sam
8/10/2020 8:18:25 AM

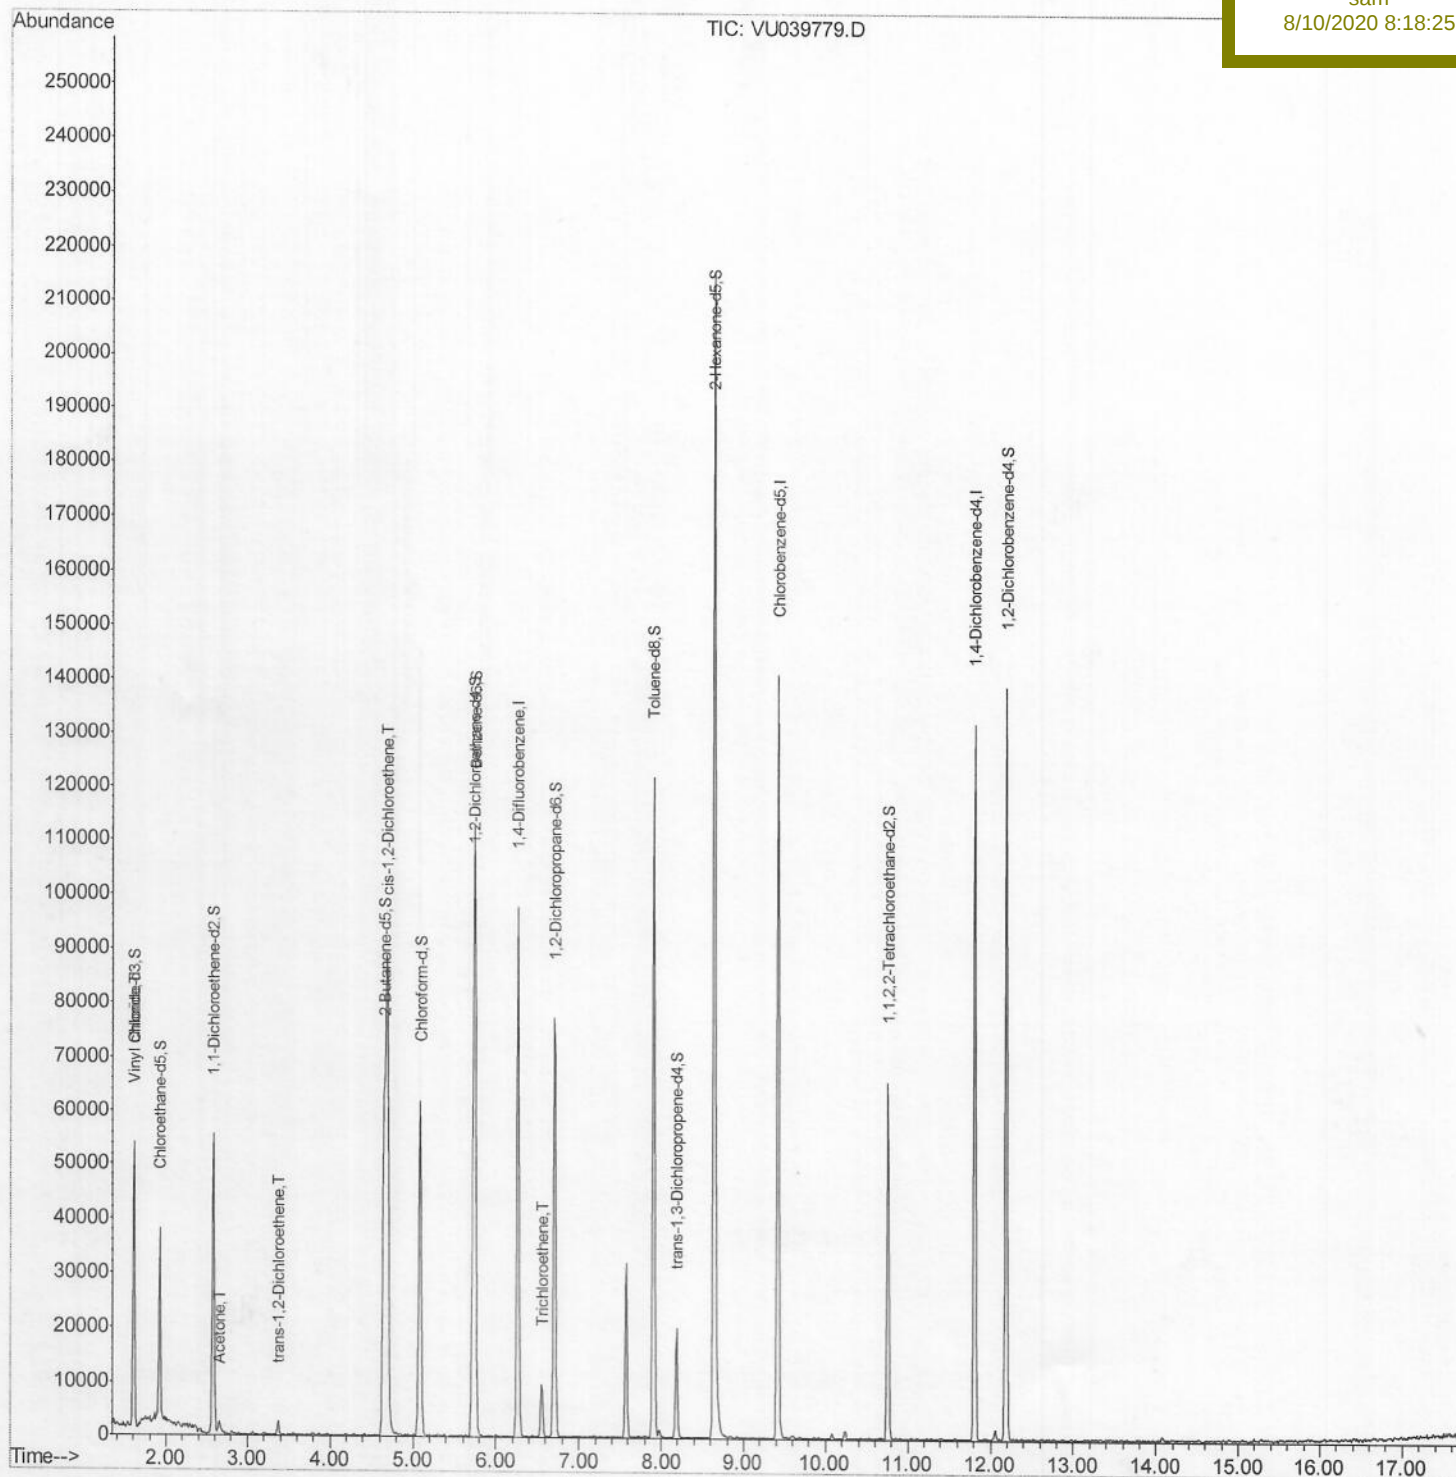

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080720\

Data File : VU039779.D

Acq On : 07 Aug 2020 12:04

Operator : SY/MD

Sample : L3572-20

Misc : 25.0mL/MSVOA U/WATER

ALS Vial : 6 Sample Multiplier: 1

Quant Time: Aug 08 03:32:48 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Sat Aug 08 03:30:58 2020

Response via : Initial Calibration

Instrument :

MSVOA_U

ClientSampleId :




F2L87

Manual Integrations

APPROVED

sam

8/10/2020 8:18:25 AM

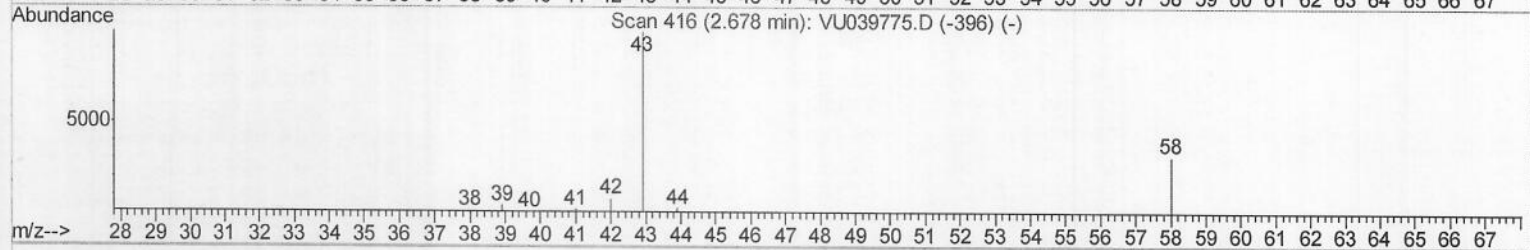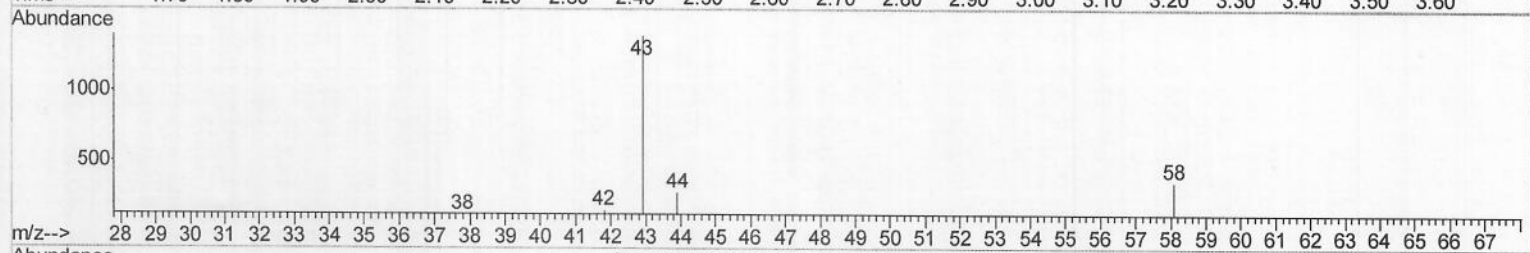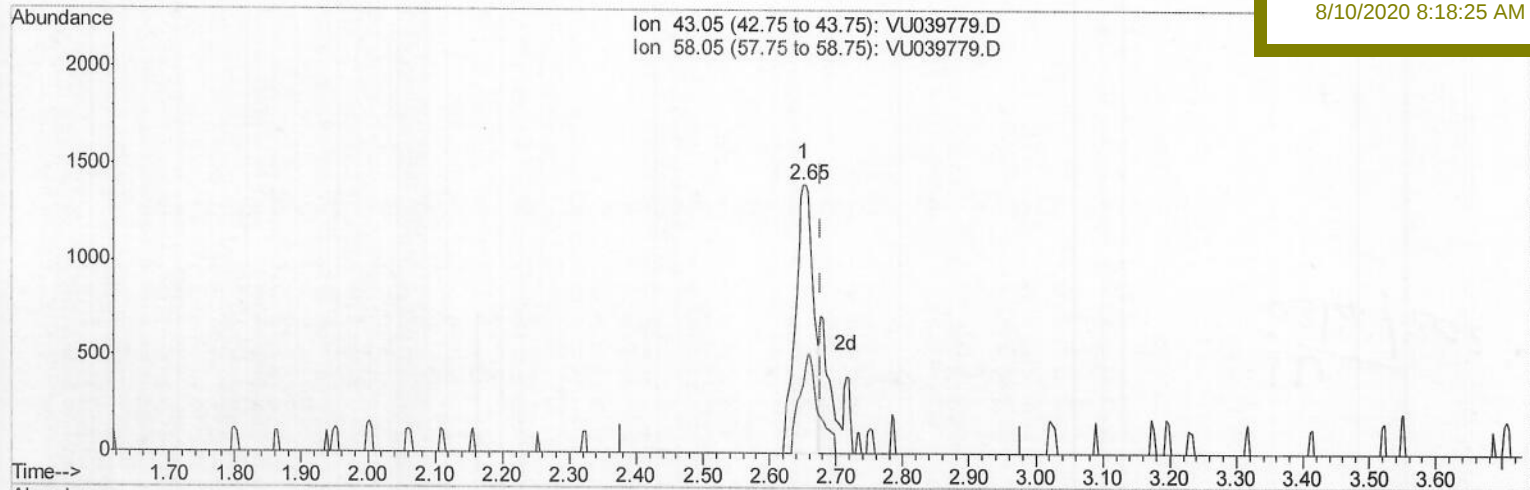

TIC: VU039779.D

(13) Acetone (T)

2.652min (-0.026) 2.46ug/L

response 2645

Ion	Exp%	Act%
43.05	100	100
58.05	30.90	37.62
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080720\

Data File : VU039779.D

Acq On : 07 Aug 2020 12:04

Operator : SY/MD

Sample : L3572-20

Misc : 25.0mL/MSVOA U/WATER

ALS Vial : 6 Sample Multiplier: 1

Quant Time: Aug 08 03:32:48 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Sat Aug 08 03:30:58 2020

Response via : Initial Calibration

Instrument :

MSVOA_U


ClientSampleId :

F2L87

Manual Integrations
APPROVED

sam

8/10/2020 8:18:25 AM

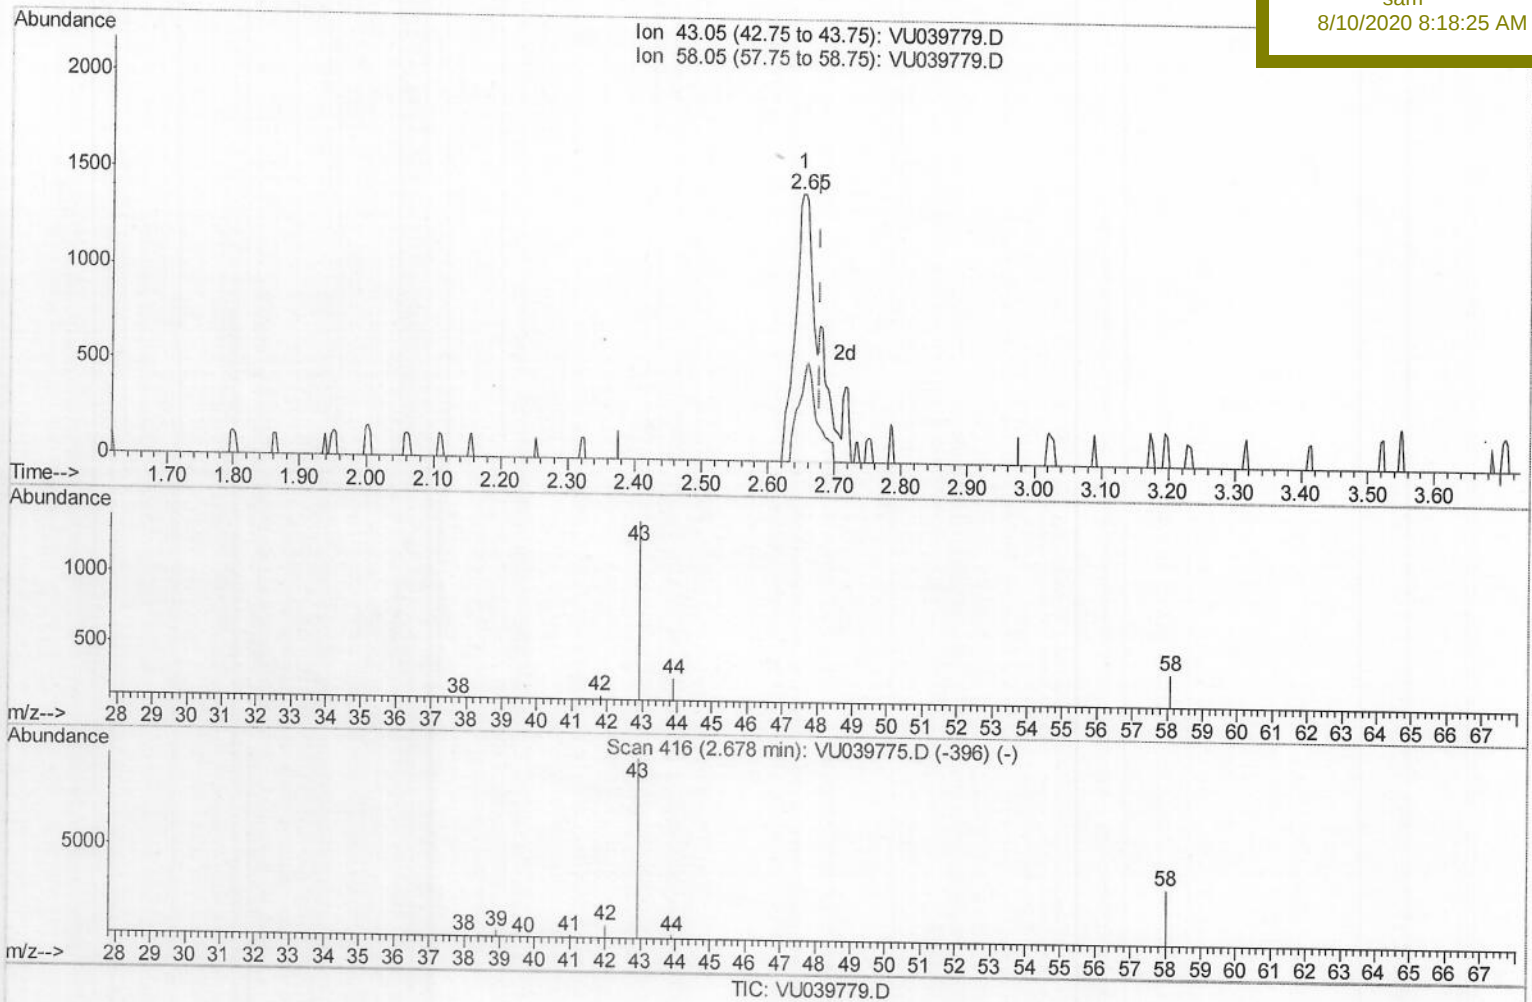

(13) Acetone (T)

2.652min (-0.026) 3.38ug/L m

response 3627

Ion	Exp%	Act%
43.05	100	100
58.05	30.90	27.43
0.00	0.00	0.00
0.00	0.00	0.00

-> MD
08/10/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080720\
 Data File : VU039779.D
 Acq On : 07 Aug 2020 12:04
 Operator : SY/MD
 Sample : L3572-20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2L87

Quant Time: Aug 08 03:59:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 08 03:30:58 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sam
 8/10/2020 8:18:25 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	76648	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	73157	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	33257	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	21326	5.15	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.00%
7) Chloroethane-d5	1.92	69	22974	5.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.60%
11) 1,1-Dichloroethene-d2	2.58	63	31426	3.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.40%
20) 2-Butanone-d5	4.65	46	102336	56.22	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.44%
24) Chloroform-d	5.09	84	54759	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.00%
26) 1,2-Dichloroethane-d4	5.72	65	33189	5.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.80%
32) Benzene-d6	5.74	84	95641	5.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.00%
36) 1,2-Dichloropropane-d6	6.70	67	33060	5.55	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	111.00%
41) Toluene-d8	7.91	98	75153	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
43) trans-1,3-Dichloropropene-	8.19	79	9976	4.36	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.20%
46) 2-Hexanone-d5	8.64	63	71966	58.19	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	116.38%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	30702	5.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.00%
64) 1,2-Dichlorobenzene-d4	12.19	152	34192	6.01	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	120.20%#

Target Compounds

5) Vinyl chloride	1.61	62	14612	2.345	ug/L	96
13) Acetone	2.65	43	3627m	→ 3.380	ug/L	
18) trans-1,2-Dichloroethene	3.37	96	1044	0.205	ug/L	79
22) cis-1,2-Dichloroethene	4.69	96	37453	6.765	ug/L	94
34) Trichloroethene	6.55	95	3127	0.604	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD
 08/10/20