


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080720\
 Data File : VU039774.D
 Acq On : 07 Aug 2020 09:04
 Operator : SY/MD
 Sample : BFB10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB10

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Aug 10 00:40:55 2020

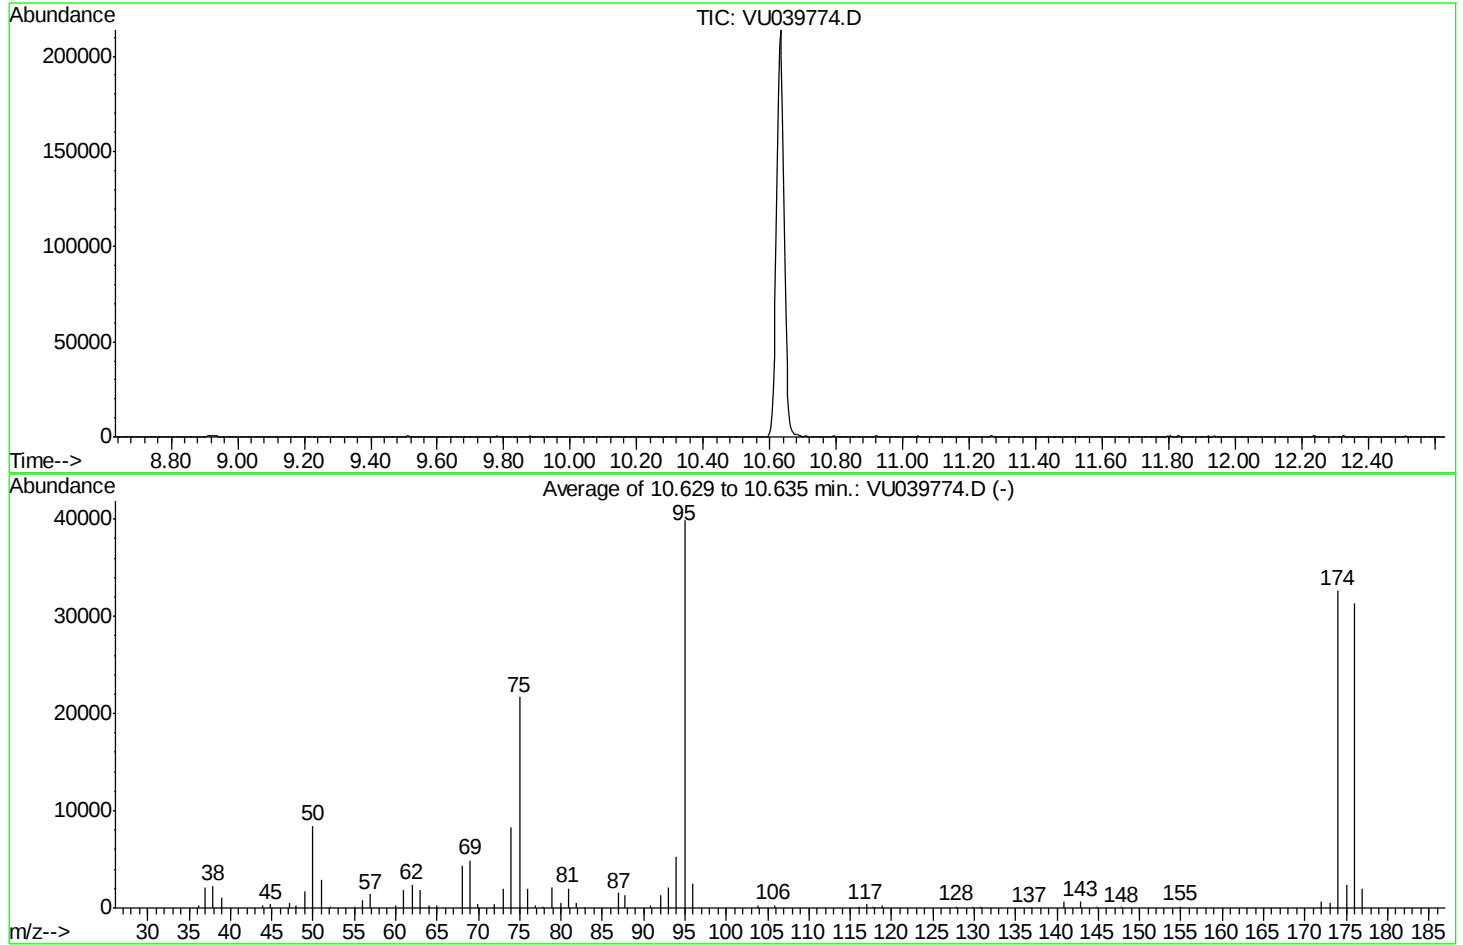

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	8440	PASS
75	95	30	80	54.3	21664	PASS
95	95	100	100	100.0	39869	PASS
96	95	5	9	6.1	2451	PASS
173	174	0.00	2	1.6	508	PASS
174	95	50	120	81.8	32632	PASS
175	174	5	9	7.1	2322	PASS
176	174	95	101	95.8	31274	PASS
177	176	5	9	6.1	1914	PASS

m/z	Abundance
44.00	268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.10	354.0
36.90	2067.0
37.90	2235.0
38.90	1071.0
43.90	553.0
44.90	316.0
47.10	502.0
48.00	232.0
49.00	1689.0
50.00	8657.0
51.00	3040.0
52.10	166.0
55.10	111.0
56.00	776.0
56.90	1565.0
60.10	279.0
61.00	1944.0
62.00	2377.0
63.00	2124.0
63.90	236.0
65.00	341.0
68.00	4546.0
69.00	4746.0
69.90	388.0
71.90	314.0
73.00	1721.0
74.00	8127.0
75.00	22224.0
76.00	1961.0
77.00	317.0
77.80	203.0
78.90	2030.0
80.00	455.0
80.90	2077.0
81.80	543.0
82.80	102.0
87.00	1511.0
87.80	1427.0
90.90	186.0
92.00	1347.0
93.00	1968.0
94.00	5425.0
95.00	40096.0
96.00	2380.0
103.90	249.0
105.80	281.0
116.00	192.0
117.00	361.0
117.70	252.0
118.80	337.0
127.90	173.0
129.90	139.0
136.80	100.0
140.90	562.0
142.90	598.0
144.80	107.0
147.80	138.0
155.00	156.0
172.00	554.0
173.00	457.0
174.00	31856.0
175.00	2314.0
176.00	30256.0
177.00	1804.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.10	350.0
36.90	2170.0
37.90	2429.0
38.90	1061.0
43.90	556.0
44.90	386.0
47.10	492.0
47.90	255.0
49.00	1744.0
50.00	8643.0
51.00	3064.0
52.10	167.0
55.10	118.0
56.00	802.0
57.00	1455.0
60.10	335.0
61.00	1820.0
61.90	2541.0
63.00	1904.0
64.00	230.0
64.90	324.0
68.00	4455.0
69.00	5109.0
69.90	396.0
71.90	388.0
73.00	1984.0
74.00	8535.0
75.00	22320.0
76.00	2030.0
77.00	258.0
77.80	187.0
78.90	2217.0
79.90	530.0
80.90	2023.0
81.90	541.0
87.00	1581.0
87.80	1380.0
90.90	270.0
92.00	1338.0
93.00	2178.0
94.00	5529.0
95.00	41320.0
96.00	2511.0
103.90	277.0
105.80	324.0
116.00	182.0
117.00	398.0
117.70	234.0
118.80	331.0
127.90	209.0
129.80	208.0
130.80	152.0
136.80	106.0
140.90	663.0
142.90	679.0
144.80	112.0
147.90	128.0
154.90	187.0
172.00	702.0
173.00	530.0
174.00	33752.0
175.00	2387.0
176.00	32320.0
177.00	1982.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.10	277.0
36.90	1962.0
37.90	2187.0
38.90	987.0
44.00	466.0
44.90	446.0
47.10	447.0
48.00	237.0
49.00	1634.0
50.00	8020.0
51.00	2718.0
52.00	148.0
55.90	748.0
56.90	1223.0
59.90	345.0
61.00	1650.0
61.90	2367.0
63.00	1640.0
64.10	252.0
65.10	302.0
68.00	3983.0
69.00	4840.0
70.00	378.0
71.90	377.0
73.00	2065.0
74.00	8093.0
75.00	20448.0
76.00	1932.0
76.90	225.0
77.90	157.0
78.90	2177.0
79.90	533.0
80.90	1856.0
81.90	520.0
87.00	1621.0
87.80	1208.0
90.90	289.0
92.00	1195.0
92.90	2138.0
94.00	5046.0
95.00	38192.0
96.00	2463.0
103.90	238.0
105.80	333.0
116.10	167.0
116.90	394.0
117.90	181.0
118.80	281.0
127.90	184.0
129.80	213.0
130.80	146.0
140.90	661.0
142.90	620.0
147.90	110.0
154.90	162.0
172.00	673.0
173.00	537.0
174.00	32288.0
175.00	2267.0
176.00	31248.0
177.00	1958.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10