


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080818\
 Data File : VU025971.D
 Acq On : 08 Aug 2018 10:24
 Operator : MD/SY
 Sample : BFB41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB41

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080718WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 09 01:19:52 2018

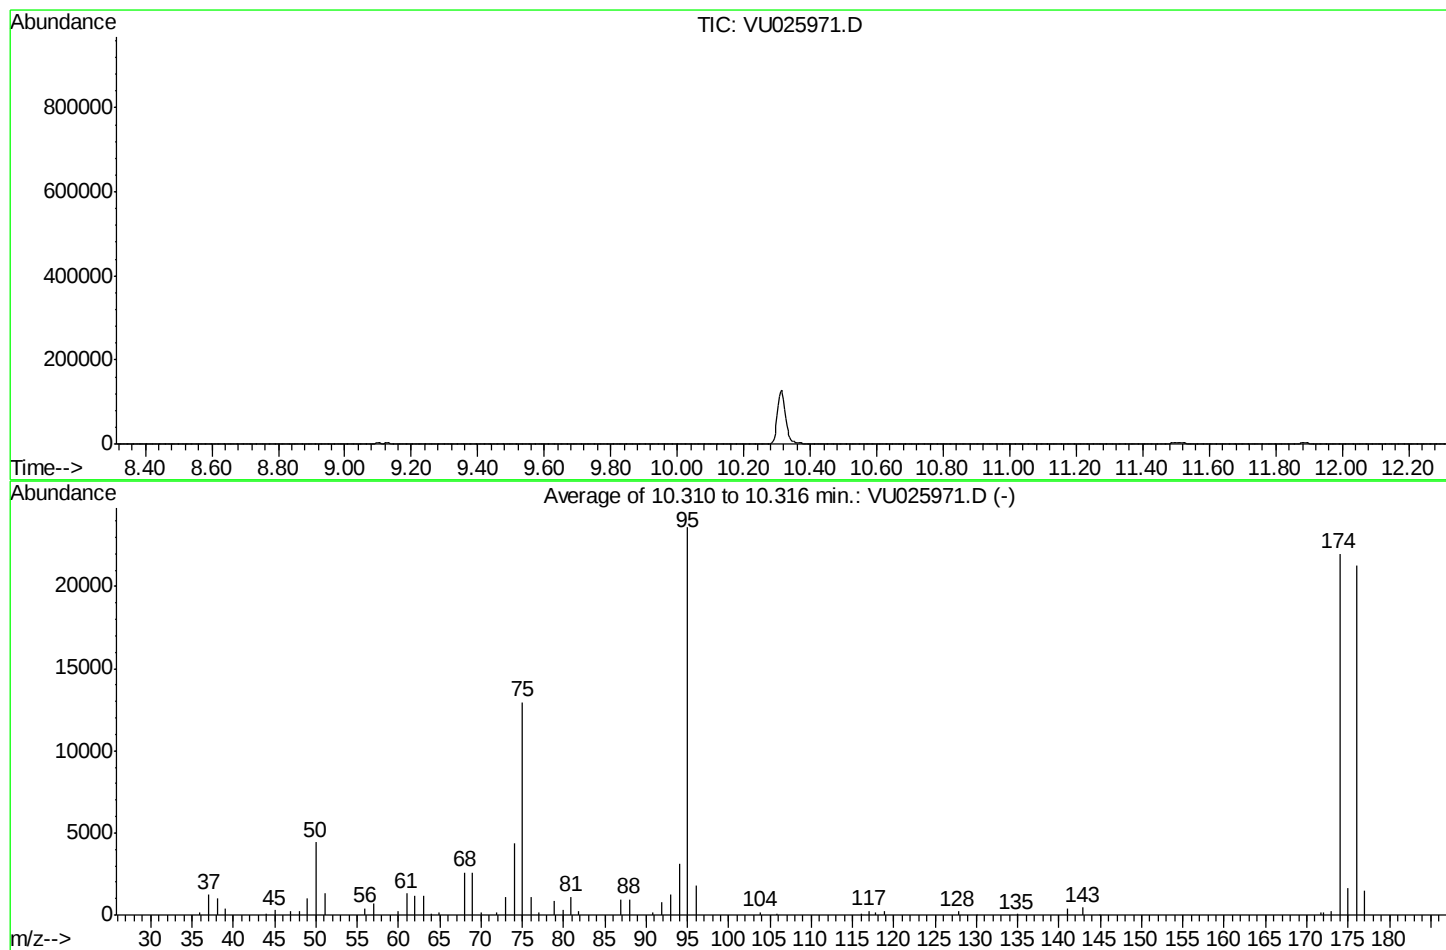

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3012

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	4439	PASS
75	95	30	80	55.0	12968	PASS
95	95	100	100	100.0	23597	PASS
96	95	5	9	7.7	1819	PASS
173	174	0.00	2	1.2	255	PASS
174	95	50	120	93.3	22005	PASS
175	174	5	9	7.5	1642	PASS
176	174	95	101	96.7	21272	PASS
177	176	5	9	6.8	1450	PASS

Scan 3012 (10.274 min): VU025971.D
BFB41

m/z	Abundance
35.90	101.0
39.90	201.0
43.90	397.0
207.00	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.90	245.0
37.00	1259.0
38.00	999.0
39.00	453.0
40.00	148.0
44.00	521.0
45.00	280.0
46.90	247.0
48.00	171.0
48.90	1060.0
50.00	4585.0
51.10	1259.0
56.00	433.0
57.00	754.0
60.00	224.0
61.00	1290.0
62.00	1242.0
63.10	1182.0
64.00	163.0
64.90	181.0
68.00	2568.0
69.00	2509.0
70.00	137.0
71.90	113.0
72.90	1116.0
74.00	4362.0
75.00	13355.0
76.00	1035.0
77.00	179.0
78.90	860.0
79.90	330.0
80.90	1129.0
81.80	243.0
86.90	921.0
87.90	903.0
90.90	143.0
92.00	674.0
93.00	1186.0
94.00	3186.0
95.00	23352.0
96.00	1856.0
103.90	161.0
105.80	180.0
116.10	100.0
117.00	224.0
117.70	140.0
118.90	242.0
127.80	185.0
140.90	327.0
142.90	451.0
144.90	104.0
172.00	268.0
172.90	400.0
174.00	21624.0
175.00	1781.0
176.00	21344.0
176.90	1419.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.90	234.0
37.00	1247.0
38.10	1038.0
39.00	432.0
39.90	157.0
44.00	459.0
45.00	312.0
46.90	243.0
47.90	205.0
49.00	1054.0
50.00	4557.0
51.00	1350.0
56.00	433.0
57.00	684.0
60.00	250.0
61.00	1345.0
62.00	1223.0
63.00	1222.0
64.00	139.0
65.00	199.0
68.00	2682.0
69.00	2612.0
69.90	136.0
72.00	133.0
72.90	1138.0
74.00	4511.0
75.00	13475.0
76.00	1118.0
77.00	186.0
78.90	861.0
79.90	298.0
80.90	1124.0
81.80	260.0
86.90	978.0
88.00	976.0
90.90	138.0
92.00	745.0
93.00	1272.0
94.00	3164.0
95.00	24160.0
96.00	1867.0
103.80	184.0
105.80	145.0
116.10	101.0
117.00	262.0
117.80	128.0
118.90	269.0
127.80	232.0
134.90	111.0
141.00	385.0
142.90	436.0
171.70	236.0
172.00	248.0
173.00	365.0
174.00	22632.0
174.90	1647.0
176.00	21864.0
176.90	1560.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	202.0
37.10	1132.0
38.10	1007.0
39.00	381.0
39.90	196.0
44.00	442.0
45.00	294.0
47.00	228.0
47.90	247.0
49.10	989.0
50.00	4176.0
51.00	1338.0
55.90	399.0
57.00	617.0
59.90	251.0
61.00	1312.0
62.00	1132.0
63.00	1110.0
65.00	210.0
68.10	2518.0
69.00	2491.0
69.90	161.0
72.00	167.0
72.90	1091.0
74.00	4167.0
75.00	12075.0
76.00	1126.0
77.00	158.0
78.90	839.0
79.90	233.0
80.90	1065.0
81.90	272.0
86.90	851.0
88.00	974.0
90.80	105.0
91.90	841.0
93.00	1204.0
94.00	2914.0
95.00	23280.0
96.00	1736.0
103.80	162.0
117.00	242.0
117.90	131.0
118.90	217.0
127.80	223.0
130.00	124.0
134.90	118.0
141.00	379.0
143.00	448.0
171.70	287.0
174.00	21760.0
174.90	1500.0
176.00	20608.0
176.90	1373.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41