


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080820\
 Data File : VU039798.D
 Acq On : 08 Aug 2020 09:18
 Operator : SY/MD
 Sample : BFB11
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB11

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Aug 10 05:56:42 2020

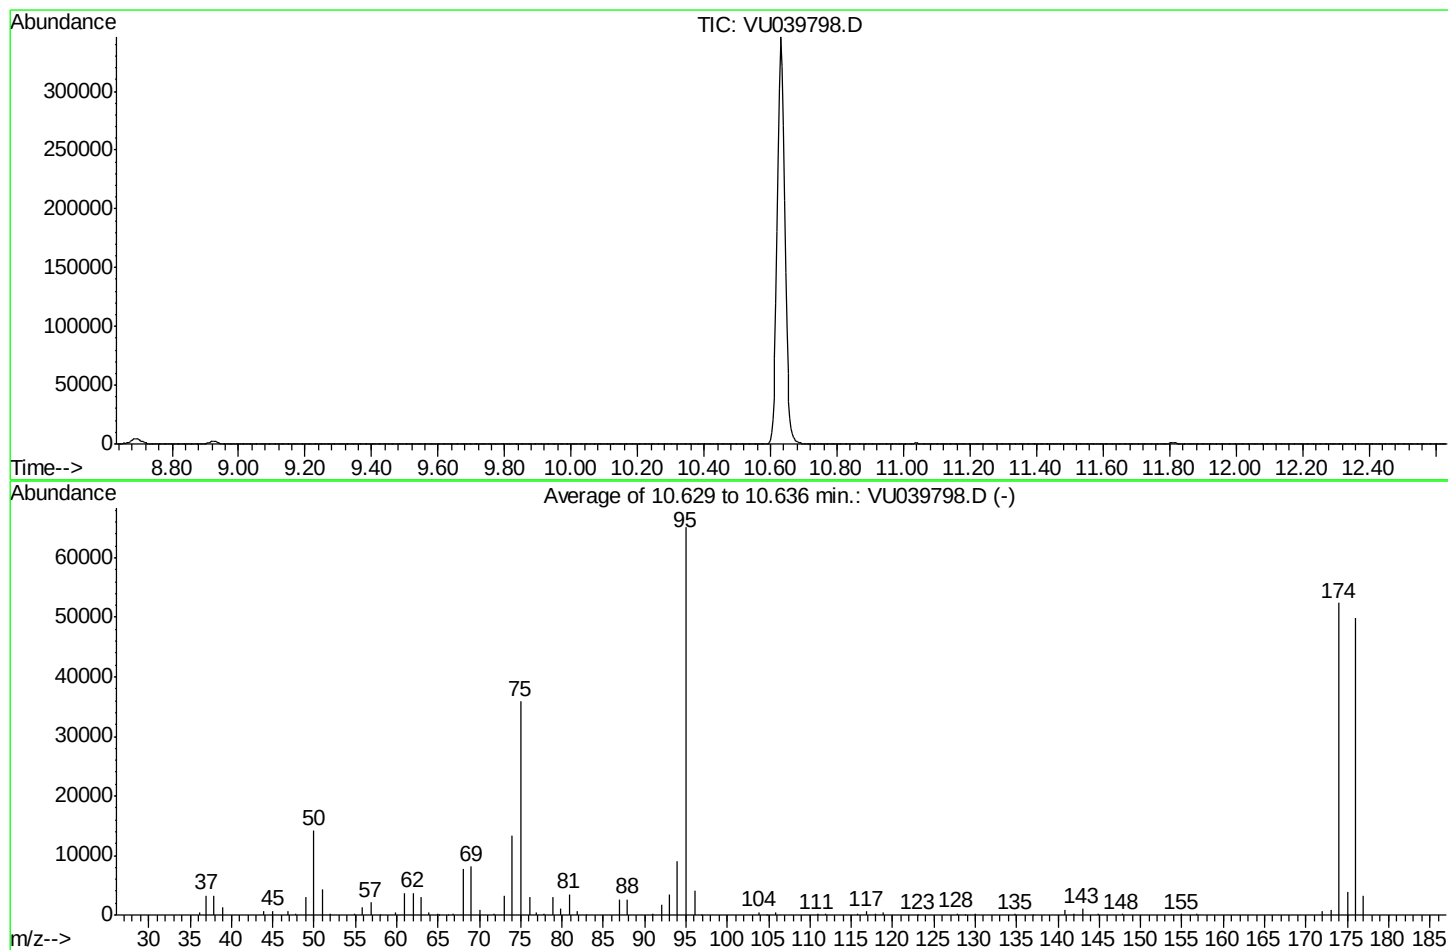

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	14114	PASS
75	95	30	80	55.1	35874	PASS
95	95	100	100	100.0	65120	PASS
96	95	5	9	6.2	4060	PASS
173	174	0.00	2	1.8	922	PASS
174	95	50	120	80.5	52426	PASS
175	174	5	9	7.2	3783	PASS
176	174	95	101	95.2	49933	PASS
177	176	5	9	6.6	3317	PASS

m/z	Abundance
43.80	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
36.10	457.0
37.00	3459.0
37.90	3478.0
38.90	1477.0
44.00	758.0
45.00	726.0
46.80	609.0
47.80	336.0
48.90	3168.0
50.00	14557.0
51.00	4543.0
52.00	247.0
54.90	239.0
55.90	1242.0
56.90	2096.0
59.90	453.0
61.00	3839.0
62.00	3788.0
62.90	3058.0
63.90	394.0
64.90	402.0
66.70	301.0
68.00	7880.0
69.00	8164.0
70.00	825.0
71.80	270.0
73.00	3215.0
74.00	13490.0
75.00	36520.0
76.00	3168.0
76.90	567.0
77.80	317.0
78.90	3169.0
79.90	977.0
80.90	3637.0
81.80	797.0
82.90	109.0
86.90	2589.0
87.90	2561.0
91.00	312.0
92.00	1916.0
93.00	3511.0
94.00	8876.0
95.00	66408.0
96.00	4276.0
96.80	158.0
103.80	530.0
104.70	134.0
105.90	370.0
110.90	113.0
111.90	117.0
115.80	336.0
116.90	599.0
117.90	302.0
118.80	429.0
123.10	102.0
127.80	300.0
128.80	128.0
130.00	233.0
134.90	178.0
140.90	955.0
142.00	147.0
142.90	1076.0
145.00	200.0
147.80	169.0
155.00	144.0
156.70	143.0
172.00	856.0
173.00	844.0
174.00	51936.0
175.00	3674.0
176.00	49096.0
177.00	3235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
36.10	458.0
37.00	3427.0
37.90	3399.0
39.00	1307.0
43.90	714.0
45.10	728.0
46.90	583.0
47.80	344.0
48.90	3159.0
49.90	14555.0
51.00	4444.0
52.00	211.0
55.00	213.0
55.90	1206.0
56.90	2151.0
58.00	106.0
59.90	464.0
61.00	3849.0
62.00	3827.0
62.90	2986.0
63.90	360.0
64.90	309.0
66.80	289.0
68.00	8024.0
69.00	8503.0
70.00	793.0
71.90	318.0
73.00	3215.0
74.00	13694.0
75.00	37120.0
76.10	3147.0
76.90	492.0
77.80	290.0
78.90	3183.0
79.90	1004.0
80.90	3663.0
81.90	734.0
86.90	2605.0
87.90	2816.0
91.00	286.0
92.00	1883.0
93.00	3511.0
94.00	9211.0
95.00	67168.0
96.00	4165.0
96.80	139.0
103.90	493.0
104.70	115.0
105.90	468.0
110.90	149.0
111.80	118.0
115.80	311.0
116.90	624.0
117.90	268.0
118.80	415.0
127.80	277.0
130.00	255.0
134.90	183.0
137.00	118.0
140.90	1006.0
142.00	178.0
143.00	1094.0
144.90	161.0
147.80	189.0
155.00	194.0
156.80	126.0
172.00	746.0
173.00	972.0
174.00	54080.0
175.00	3862.0
176.00	51384.0
177.00	3429.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
36.10	436.0
37.00	3038.0
37.90	2961.0
39.00	1164.0
43.90	627.0
45.00	657.0
47.00	576.0
47.80	295.0
49.00	2737.0
50.00	13231.0
51.00	3964.0
52.10	148.0
55.00	182.0
55.90	1169.0
56.90	1977.0
59.80	493.0
61.00	3337.0
62.00	3620.0
62.90	2726.0
63.90	313.0
65.10	310.0
66.20	119.0
66.90	256.0
68.00	7477.0
69.00	7656.0
70.00	719.0
71.90	381.0
73.00	3024.0
74.00	12693.0
75.00	33984.0
76.10	2740.0
76.90	380.0
77.90	274.0
78.90	2942.0
79.80	947.0
80.90	3194.0
81.90	649.0
87.00	2478.0
87.90	2691.0
91.00	262.0
92.00	1694.0
93.00	3150.0
94.00	8817.0
95.00	61784.0
96.10	3739.0
103.90	458.0
105.90	473.0
110.90	138.0
111.80	122.0
115.80	255.0
116.90	589.0
117.80	247.0
118.80	403.0
127.80	262.0
130.00	268.0
134.80	138.0
137.00	142.0
140.90	956.0
142.00	176.0
143.00	950.0
144.90	113.0
147.80	180.0
155.00	205.0
156.80	127.0
171.90	541.0
173.00	950.0
174.00	51264.0
175.00	3814.0
176.00	49320.0
177.00	3288.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11