

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
 Data File : VU050191.D
 Acq On : 09 Aug 2022 18:15
 Operator : SY/MD
 Sample : N4115-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 10 04:50:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 09 03:59:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	79195	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	80469	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	30375	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	21224	3.220	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	64.400%	
7) Chloroethane-d5	1.909	69	21161	3.980	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	79.600%	
11) 1,1-Dichloroethene-d2	2.565	65	8195	3.182	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	63.600%	
20) 2-Butanone-d5	4.626	46	102313	63.659	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	127.320%	
24) Chloroform-d	5.067	84	58981	4.811	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.200%	
26) 1,2-Dichloroethane-d4	5.703	65	33123	5.262	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.200%	
32) Benzene-d6	5.729	84	103349	4.116	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	82.400%	
36) 1,2-Dichloropropane-d6	6.694	67	38734	4.684	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.600%	
41) Toluene-d8	7.899	98	76821	3.464	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	69.200%#	
43) trans-1,3-Dichloroprop...	8.182	79	11559	3.901	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	78.000%	
46) 2-Hexanone-d5	8.636	63	65099	61.950	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	123.900%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	38228	5.264	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	105.200%	
66) 1,2-Dichlorobenzene-d4	12.195	152	28858	4.849	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.000%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.520	50	1657	0.174	ug/L #	75
5) Vinyl chloride	1.604	62	97319	11.438	ug/L	99
12) 1,1-Dichloroethene	2.575	96	796	0.145	ug/L #	1
18) trans-1,2-Dichloroethene	3.356	96	2509	0.409	ug/L	99
22) cis-1,2-Dichloroethene	4.668	96	189289	27.824	ug/L	99
25) Chloroform	5.092	83	44	0.004	ug/L #	74
34) Trichloroethene	6.546	95	6582	0.965	ug/L	94
35) Methylcyclohexane	6.694	83	8785	0.998	ug/L #	22
37) 1,2-Dichloropropane	6.694	63	3895	0.519	ug/L #	89
61) 1,2,3-Trichloropropane	11.812	75	3561	0.861	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050191.D
Acq On : 09 Aug 2022 18:15
Operator : SY/MD
Sample : N4115-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Aug 10 04:50:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 09 03:59:45 2022
Response via : Initial Calibration

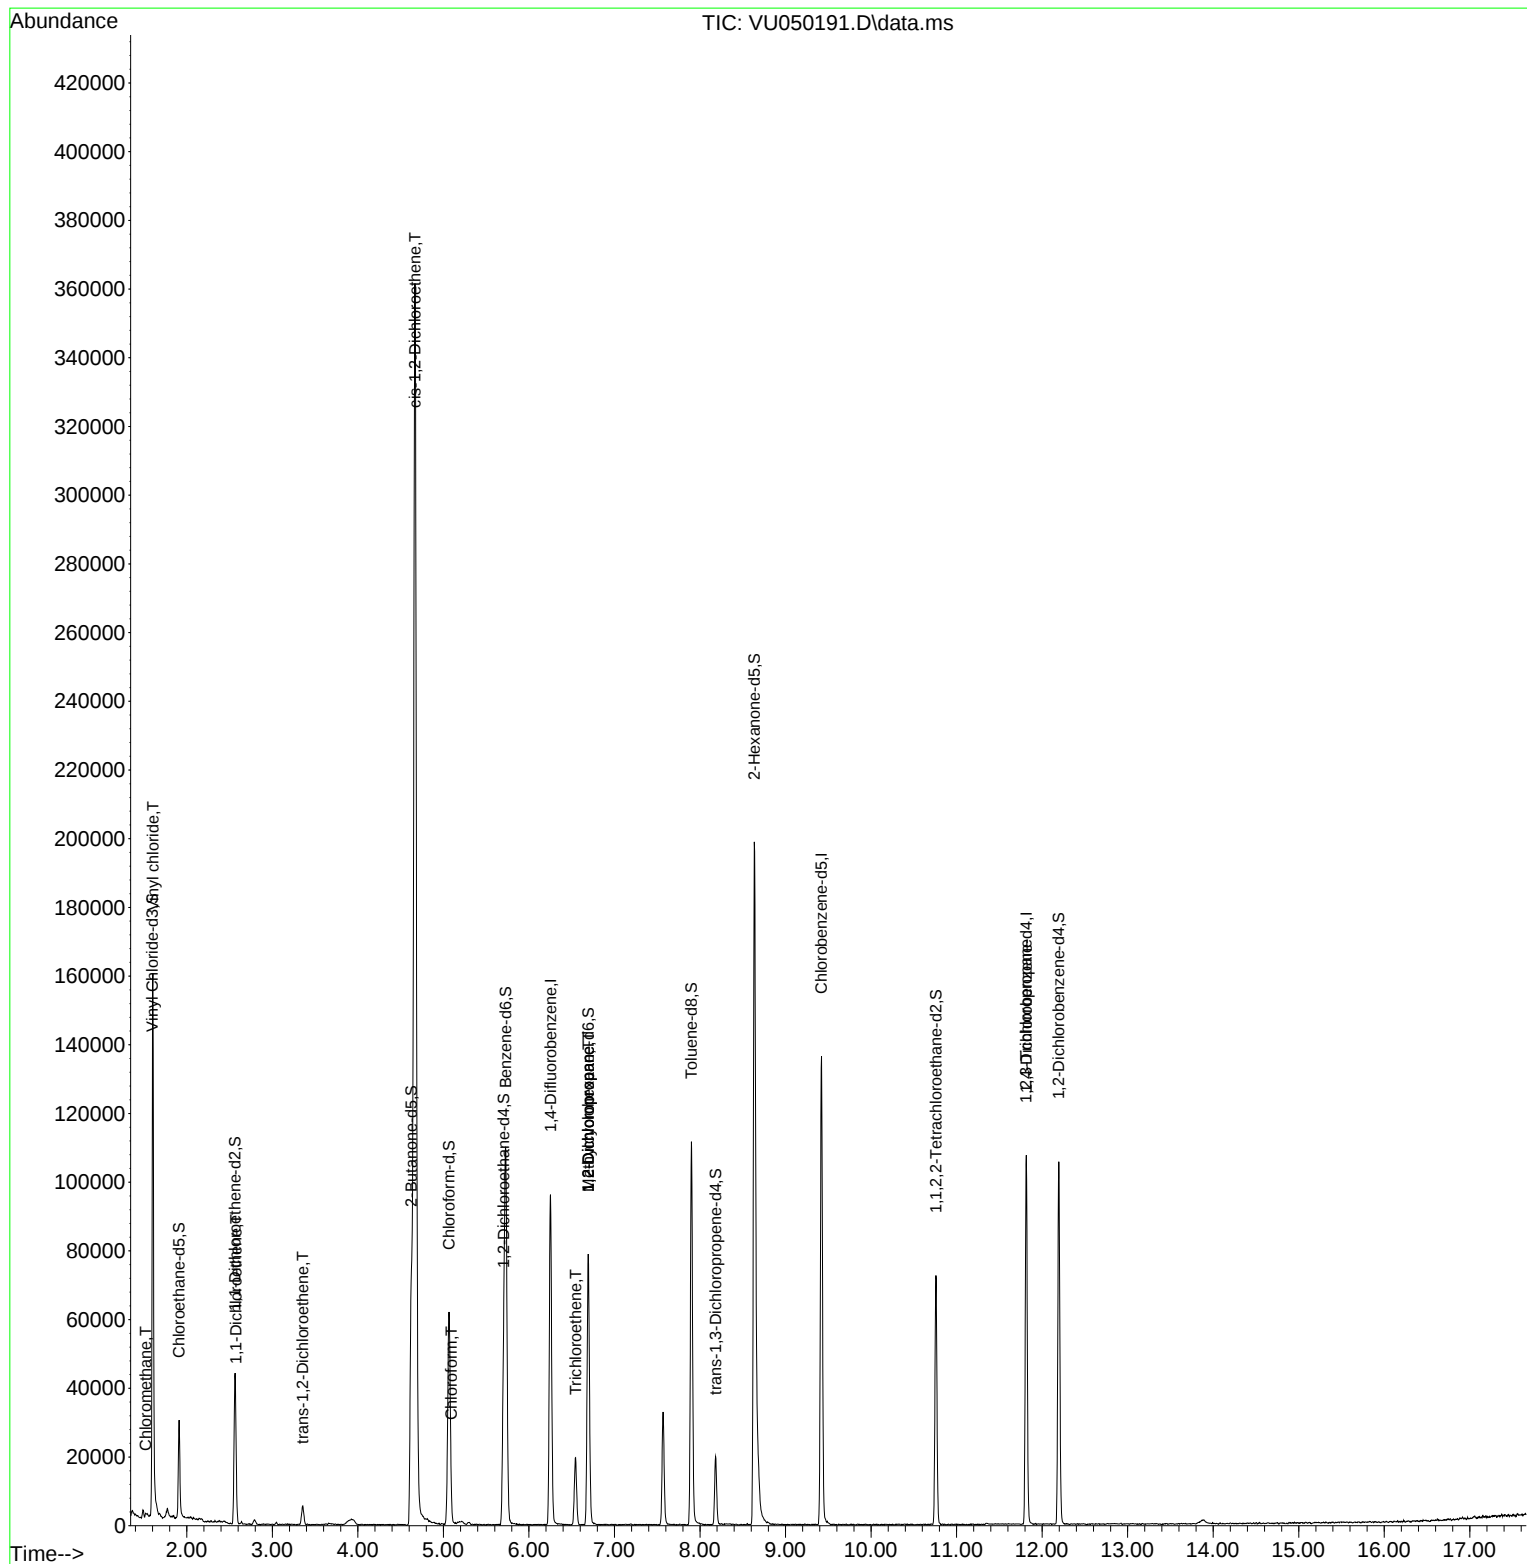



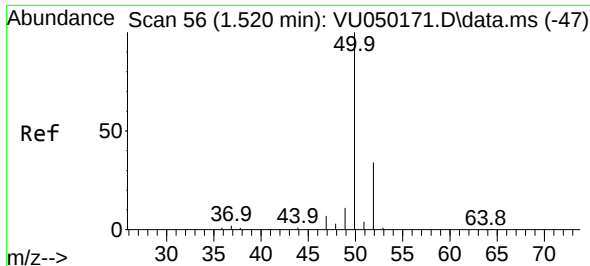


#3
Chloromethane
Concen: 0.174 ug/L
RT: 1.520 min Scan# 50
Delta R.T. -0.000 min
Lab File: VU050191.D
Acq: 09 Aug 2022 18:15

Instrument :
MSVOA_U
ClientSampleId :



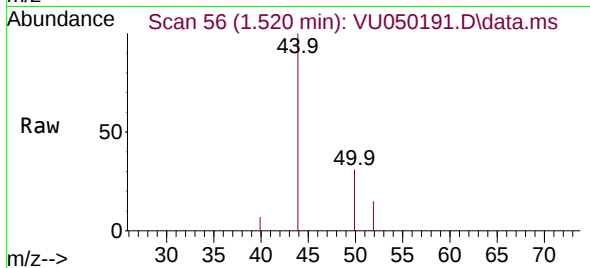



Tgt Ion: 50 Resp: 1657
Ion Ratio Lower Upper
50 100
52 47.1 23.2 43.2#

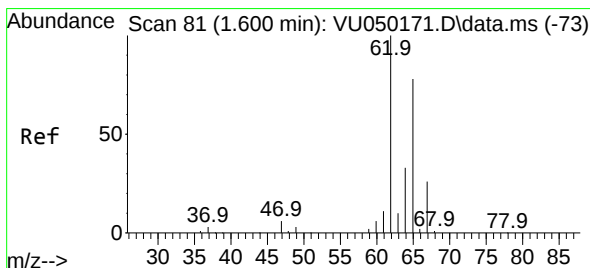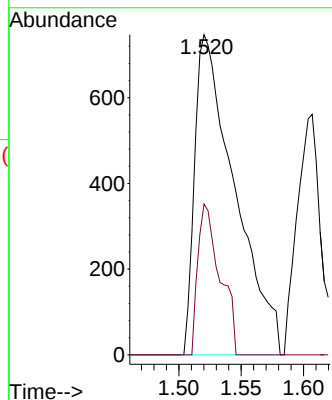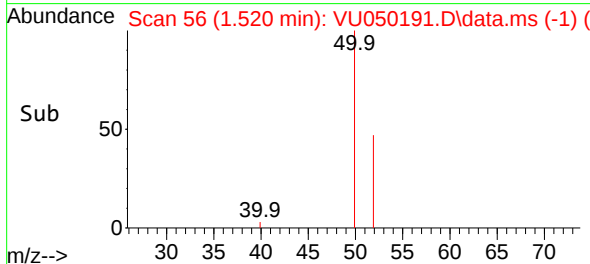

#5
Vinyl chloride
Concen: 11.438 ug/L
RT: 1.604 min Scan# 82
Delta R.T. 0.003 min
Lab File: VU050191.D
Acq: 09 Aug 2022 18:15

Tgt Ion: 62 Resp: 97319
Ion Ratio Lower Upper
62 100
64 32.3 22.8 42.4

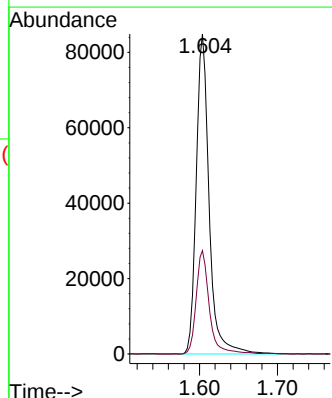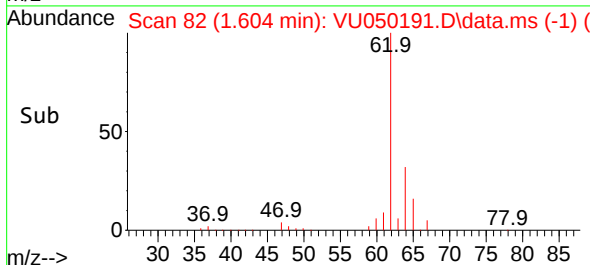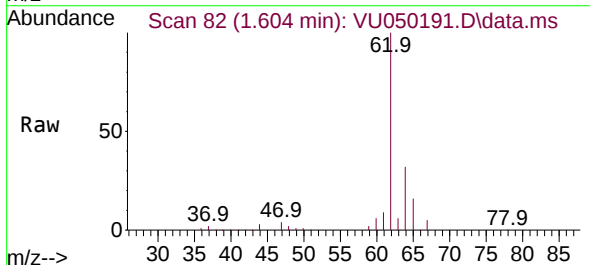

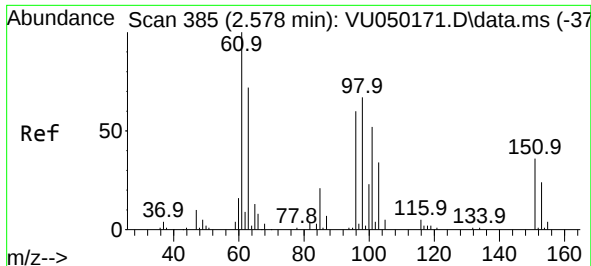

#12

1,1-Dichloroethene

Concen: 0.145 ug/L

RT: 2.575 min Scan# 385

Delta R.T. -0.000 min

Lab File: VU050191.D

Acq: 09 Aug 2022 18:15

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion: 96 Resp: 796

Ion Ratio Lower Upper

96 100

61 315.5 122.7 227.9#

63 1722.0 85.1 158.1#

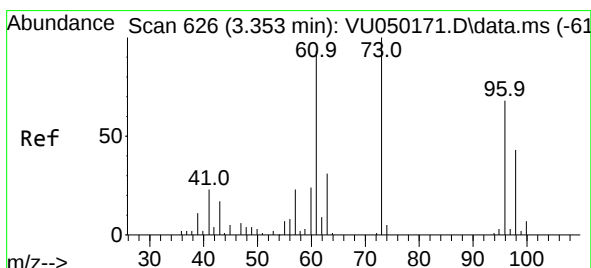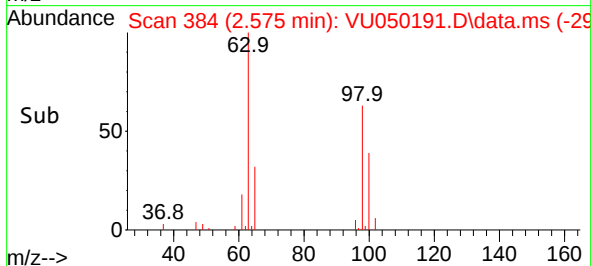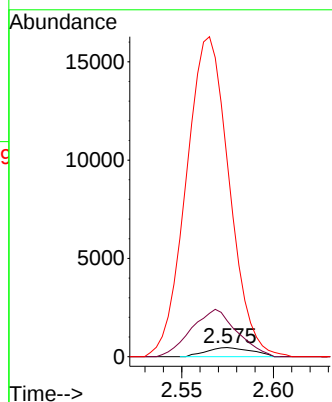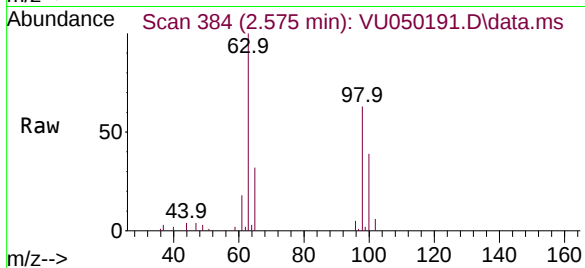

#18

trans-1,2-Dichloroethene

Concen: 0.409 ug/L

RT: 3.356 min Scan# 627

Delta R.T. 0.006 min

Lab File: VU050191.D

Acq: 09 Aug 2022 18:15




Tgt Ion: 96 Resp: 2509


Ion Ratio Lower Upper

96 100

61 131.2 92.3 171.5

98 63.4 43.2 80.2

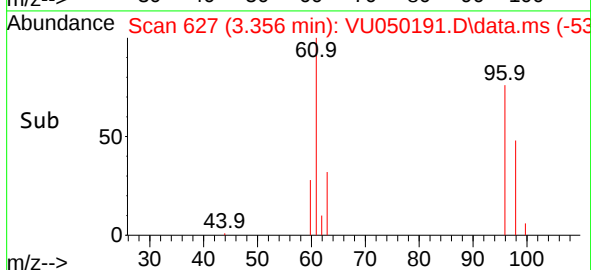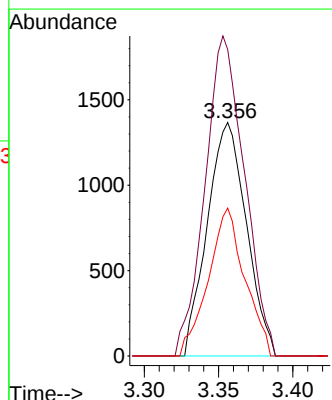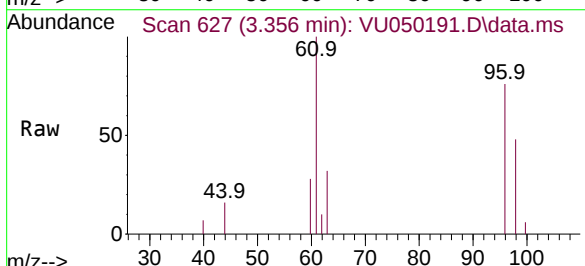

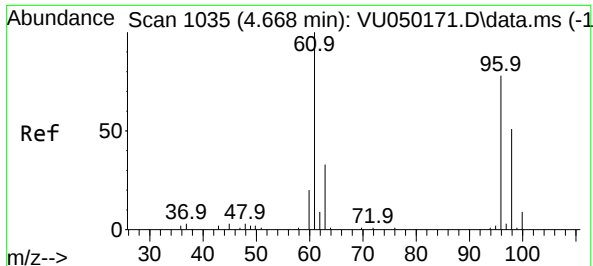

#22

cis-1,2-Dichloroethene

Concen: 27.824 ug/L

RT: 4.668 min Scan# 110

Delta R.T. -0.000 min

Lab File: VU050191.D

Acq: 09 Aug 2022 18:15

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion: 96 Resp: 189289

Ion Ratio Lower Upper

96 100

61 125.8 89.0 165.4

98 64.7 45.2 84.0

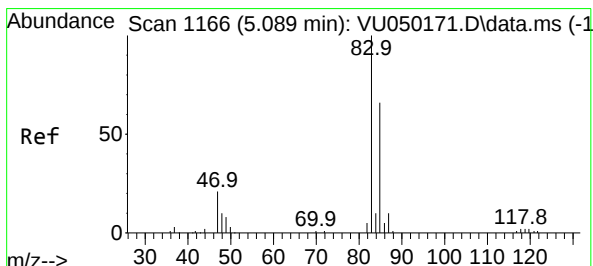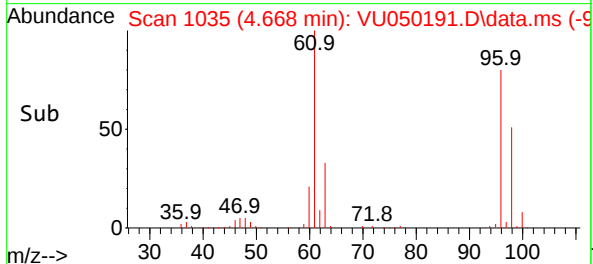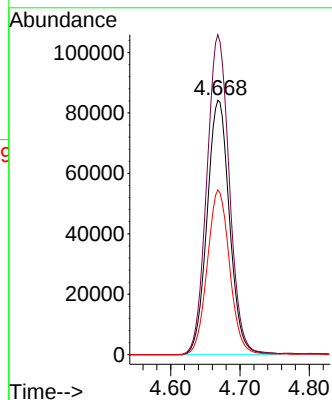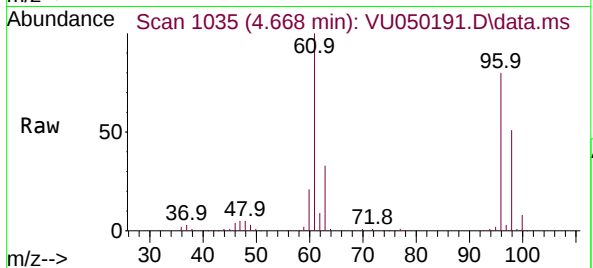

#25

Chloroform

Concen: 0.004 ug/L

RT: 5.092 min Scan# 1167

Delta R.T. 0.003 min

Lab File: VU050191.D




Acq: 09 Aug 2022 18:15


Tgt Ion: 83 Resp: 44

Ion Ratio Lower Upper

83 100

85 86.3 46.1 85.5#


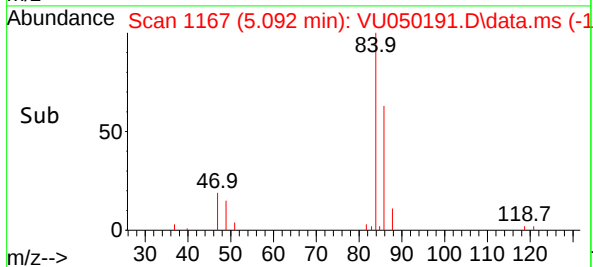
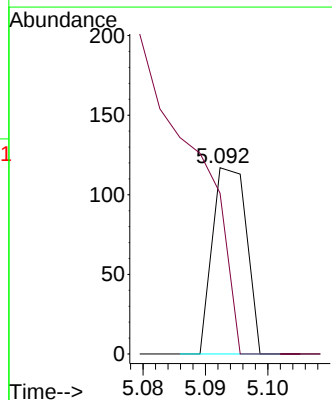
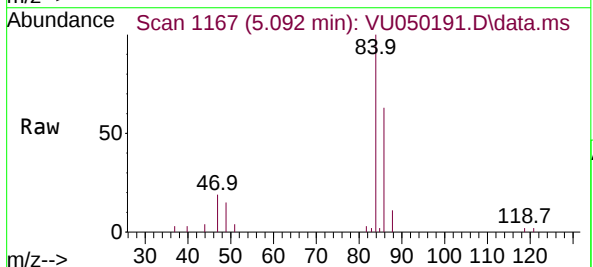


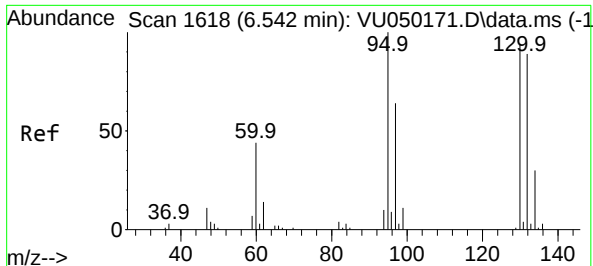

#34
Trichloroethene
Concen: 0.965 ug/L
RT: 6.546 min Scan# 1618
Delta R.T. 0.003 min
Lab File: VU050191.D
Acq: 09 Aug 2022 18:15




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 95 Resp: 6582
Ion Ratio Lower Upper
95 100
97 58.2 45.6 84.8
132 89.1 65.0 120.6
130 93.1 69.3 128.7

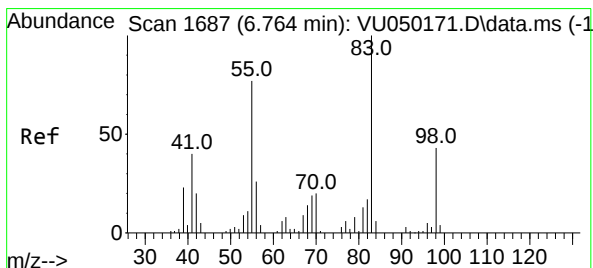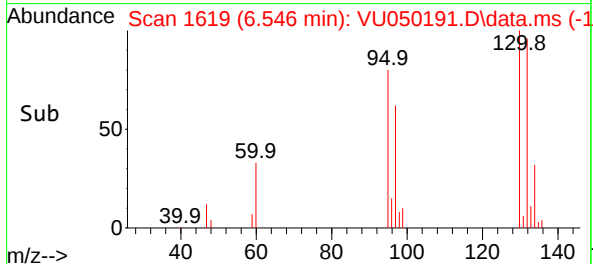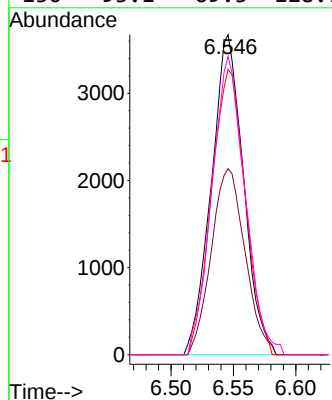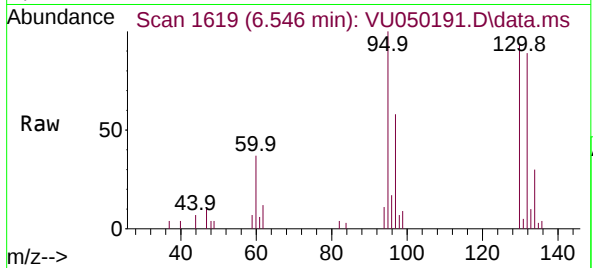

#35
Methylcyclohexane
Concen: 0.998 ug/L
RT: 6.694 min Scan# 1665
Delta R.T. -0.071 min
Lab File: VU050191.D
Acq: 09 Aug 2022 18:15

Tgt Ion: 83 Resp: 8785
Ion Ratio Lower Upper
83 100
55 0.0 62.7 94.1#
98 7.7 36.2 54.2#

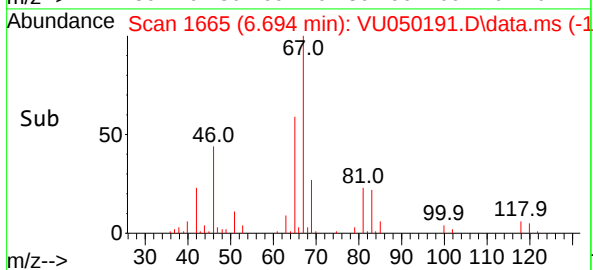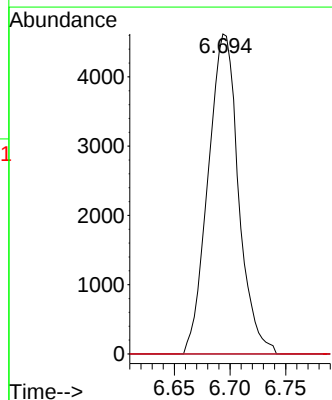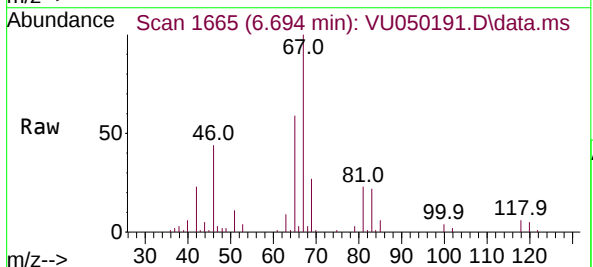

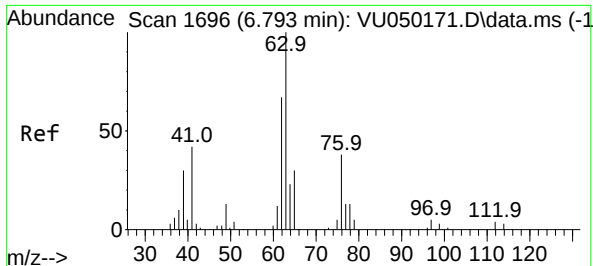

#37

1,2-Dichloropropane

Concen: 0.519 ug/L

RT: 6.694 min Scan# 1

Delta R.T. -0.100 min

Lab File: VU050191.D

Acq: 09 Aug 2022 18:15

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 63 Resp: 3895

Ion Ratio Lower Upper

63 100

112 0.0 3.0 4.4#

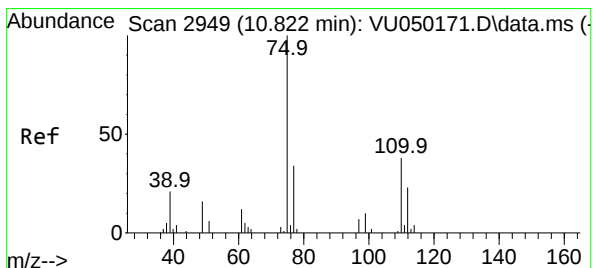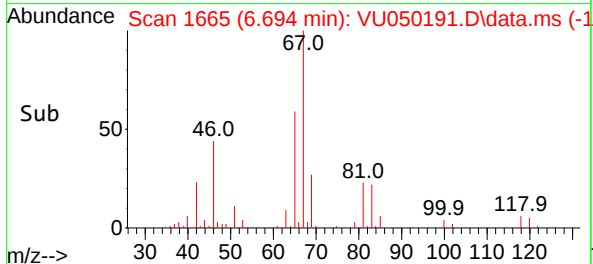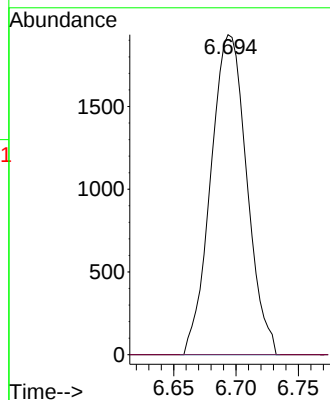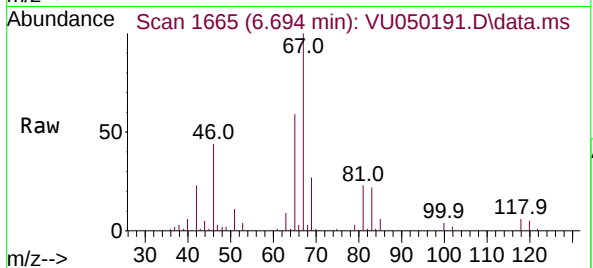

#61

1,2,3-Trichloropropane

Concen: 0.861 ug/L

RT: 11.812 min Scan# 3257

Delta R.T. 0.987 min

Lab File: VU050191.D

Acq: 09 Aug 2022 18:15

Tgt Ion: 75 Resp: 3561

Ion Ratio Lower Upper

75 100

110 0.0 28.5 42.7#

77 29.9 25.8 38.6

