

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
 Data File : VU050150.D
 Acq On : 08 Aug 2022 21:48
 Operator : SY/MD
 Sample : VU0808WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK103

Quant Time: Aug 09 04:06:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 09 03:59:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	91303	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	89076	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	34284	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	42610	5.608	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	112.200%
7) Chloroethane-d5	1.909	69	35096	5.725	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	114.600%
11) 1,1-Dichloroethene-d2	2.565	65	16260	5.475	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	109.600%
20) 2-Butanone-d5	4.633	46	107099	57.800	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.600%
24) Chloroform-d	5.067	84	76106	5.385	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.600%
26) 1,2-Dichloroethane-d4	5.703	65	38926	5.364	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.200%
32) Benzene-d6	5.729	84	154097	5.544	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.800%
36) 1,2-Dichloropropane-d6	6.694	67	50783	5.548	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	111.000%
41) Toluene-d8	7.899	98	123242	5.020	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
43) trans-1,3-Dichloroprop...	8.182	79	15794	4.815	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.200%
46) 2-Hexanone-d5	8.636	63	66814	57.438	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	114.880%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	40651	5.057	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.200%
66) 1,2-Dichlorobenzene-d4	12.195	152	38461	5.726	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.600%
Target Compounds						Qvalue
16) Methylene chloride	3.044	84	6272	0.650	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050150.D
Acq On : 08 Aug 2022 21:48
Operator : SY/MD
Sample : VU0808WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK103

Quant Time: Aug 09 04:06:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 09 03:59:45 2022
Response via : Initial Calibration

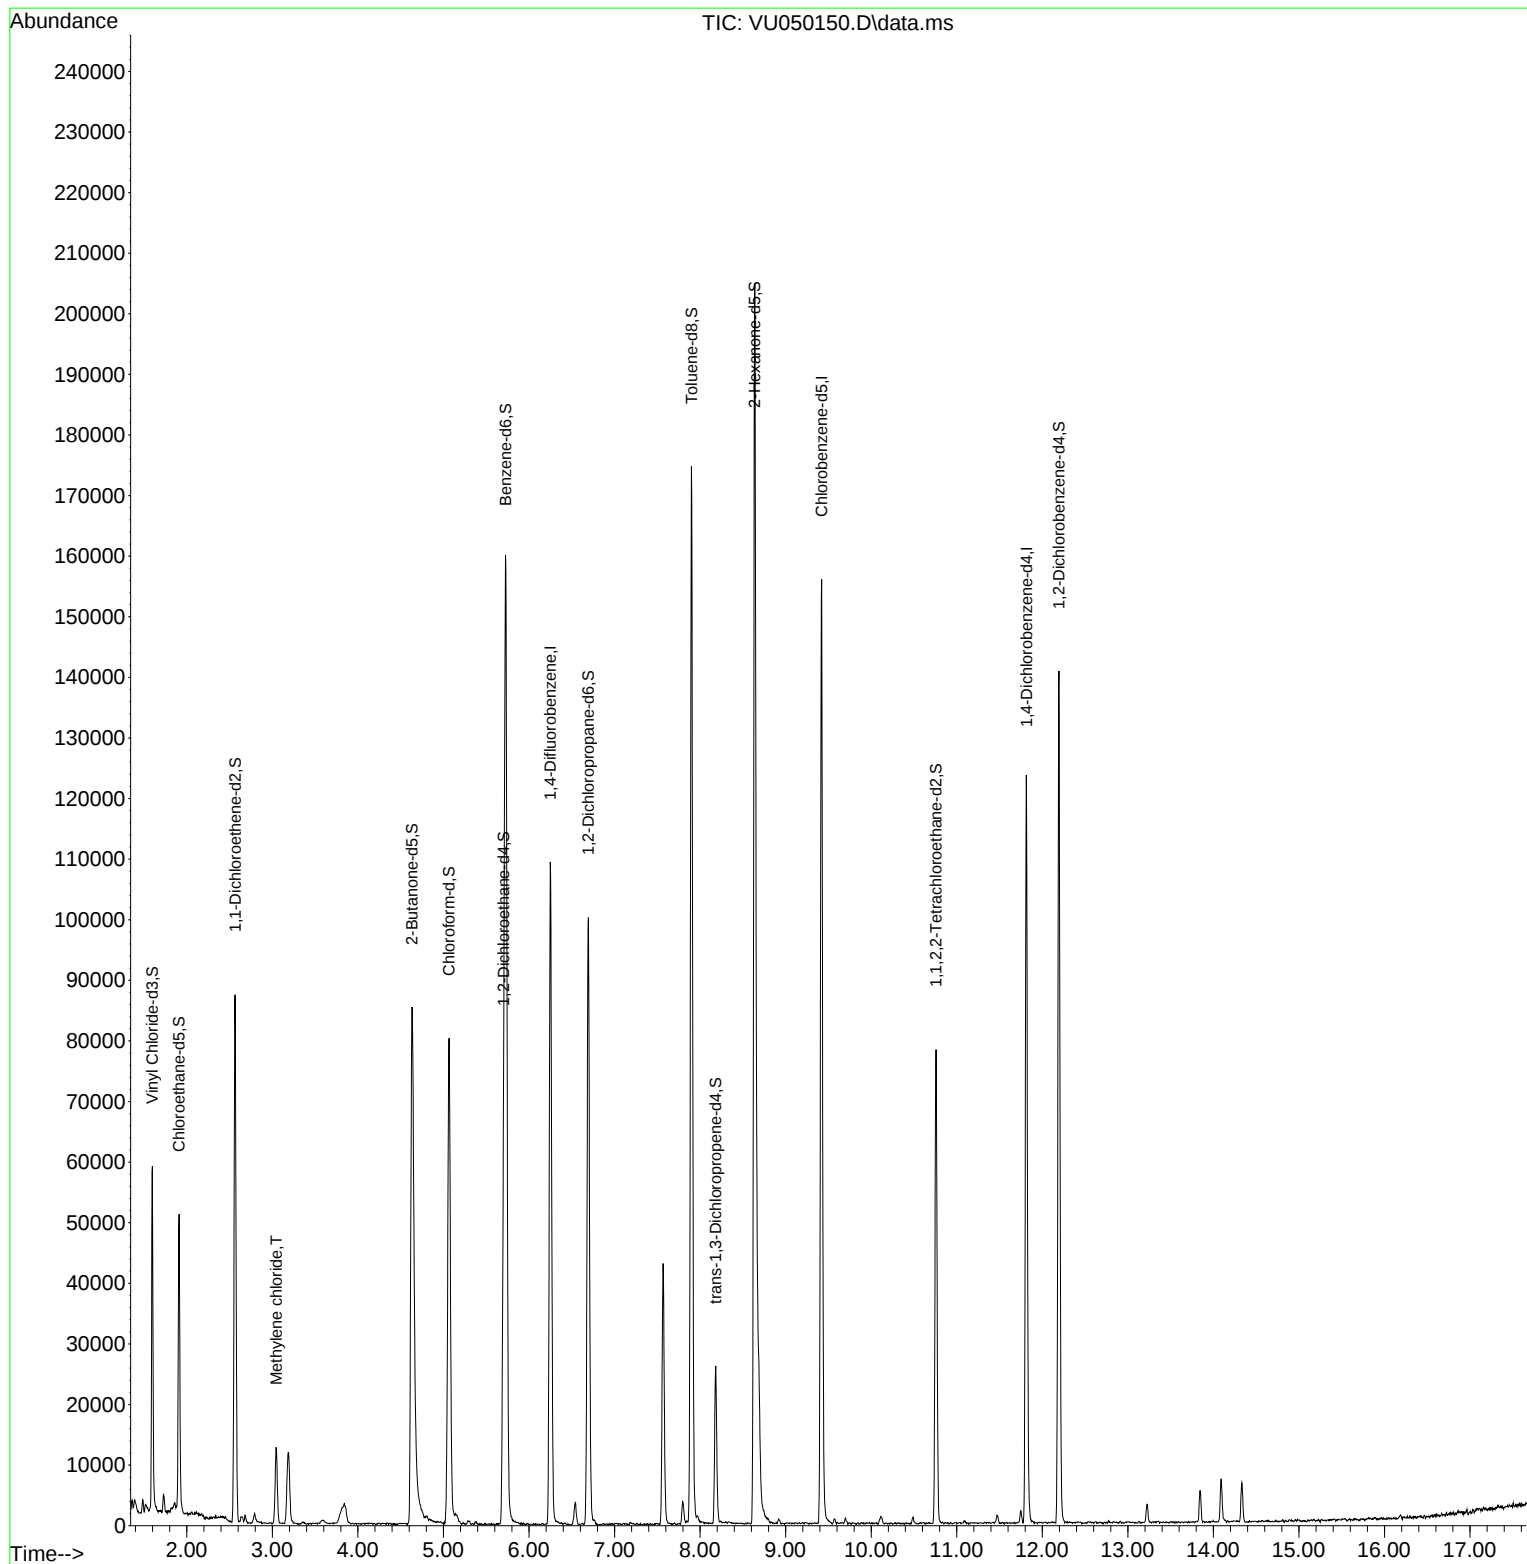

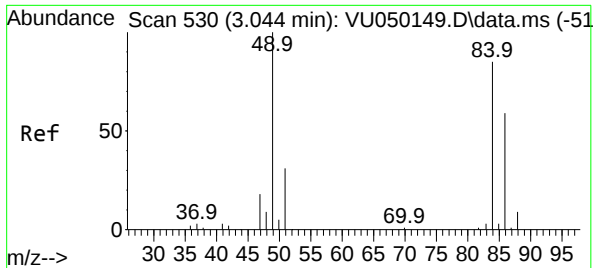

#16
Methylene chloride
Concen: 0.650 ug/L
RT: 3.044 min Scan# 51
Delta R.T. -0.000 min
Lab File: VU050150.D
Acq: 08 Aug 2022 21:48

Instrument :
MSVOA_U
ClientSampleId :
VBLK103

Tgt Ion: 84 Resp: 6272
Ion Ratio Lower Upper
84 100
86 65.9 45.9 85.3
49 107.7 77.6 144.0

