

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
 Data File : VU050163.D
 Acq On : 09 Aug 2022 03:33
 Operator : SY/MD
 Sample : N4075-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUV6

Quant Time: Aug 09 05:19:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 09 03:59:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	78540	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	78613	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	30115	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	23043	3.526	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	70.600%	
7) Chloroethane-d5	1.909	69	22508	4.268	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	85.400%	
11) 1,1-Dichloroethene-d2	2.562	65	9207	3.604	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.000%	
20) 2-Butanone-d5	4.626	46	98045	61.513	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	123.020%	
24) Chloroform-d	5.063	84	59799	4.919	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.400%	
26) 1,2-Dichloroethane-d4	5.703	65	32631	5.228	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.600%	
32) Benzene-d6	5.729	84	108882	4.438	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.800%	
36) 1,2-Dichloropropane-d6	6.690	67	40010	4.953	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.000%	
41) Toluene-d8	7.899	98	83680	3.862	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	77.200%	
43) trans-1,3-Dichloroprop...	8.182	79	12050	4.162	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.200%	
46) 2-Hexanone-d5	8.636	63	61604	60.008	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	120.020%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	37289	5.256	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	105.200%	
66) 1,2-Dichlorobenzene-d4	12.195	152	30080	5.098	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	102.000%	
Target Compounds						
					Qvalue	
16) Methylene chloride	3.044	84	4707	0.567	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050163.D
Acq On : 09 Aug 2022 03:33
Operator : SY/MD
Sample : N4075-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUV6

Quant Time: Aug 09 05:19:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 09 03:59:45 2022
Response via : Initial Calibration

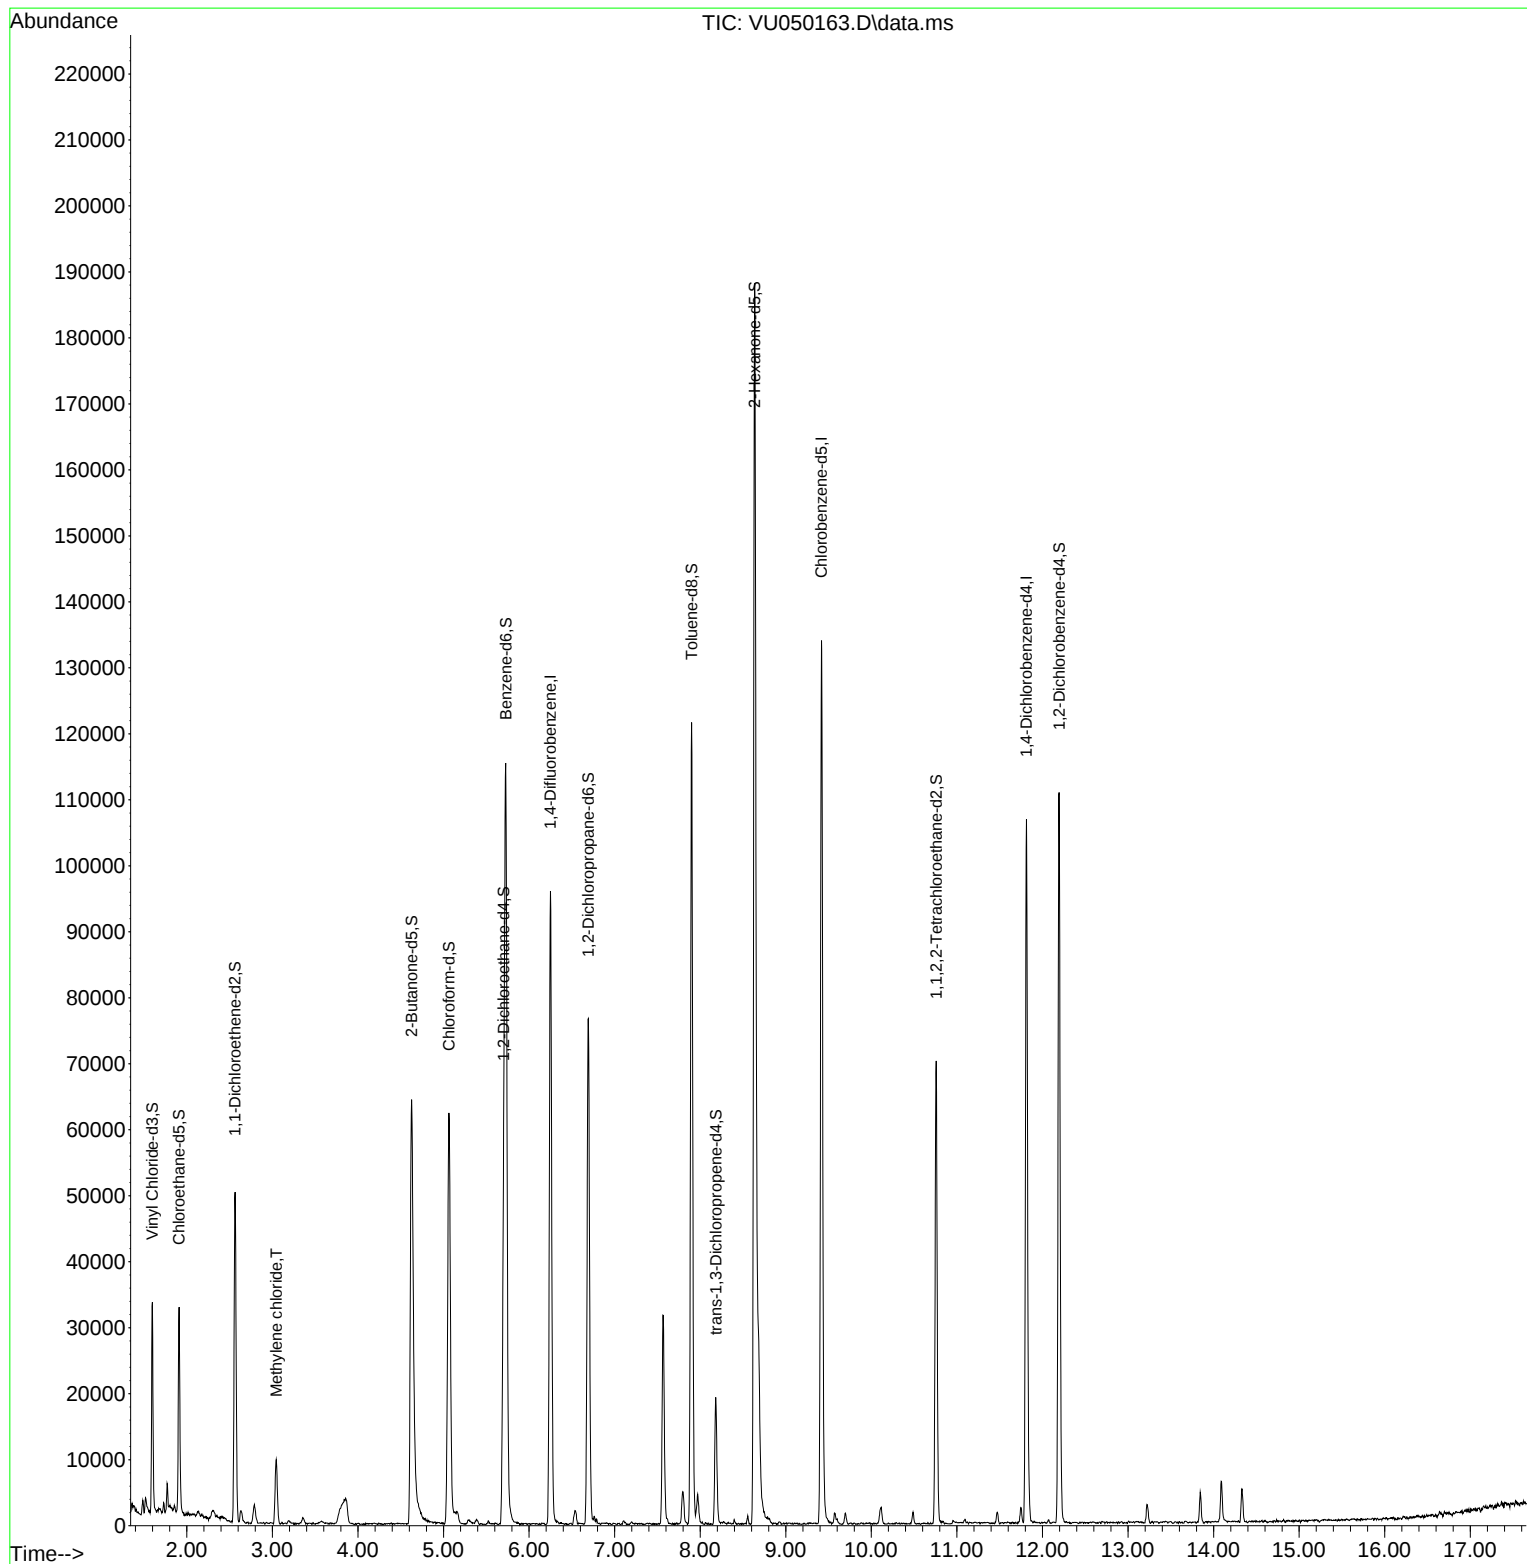

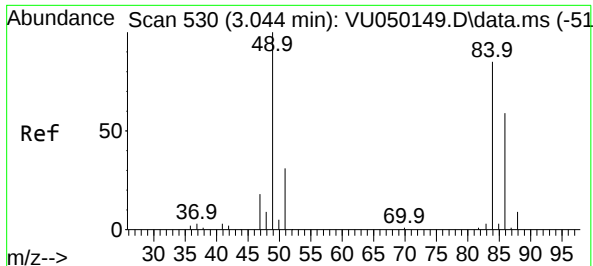

#16
Methylene chloride
Concen: 0.567 ug/L
RT: 3.044 min Scan# 51
Delta R.T. -0.000 min
Lab File: VU050163.D
Acq: 09 Aug 2022 03:33

Instrument :
MSVOA_U
ClientSampleId :
DBUV6

Tgt Ion: 84 Resp: 4707
Ion Ratio Lower Upper
84 100
86 71.8 45.9 85.3
49 134.2 77.6 144.0

