

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
 Data File : VU050172.D
 Acq On : 09 Aug 2022 08:04
 Operator : SY/MD
 Sample : VU0808WBL03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK104

Quant Time: Aug 09 08:19:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 09 03:59:45 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	91105	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	90679	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	36202	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	40344	5.321	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 106.400%		
7) Chloroethane-d5	1.912	69	34182	5.588	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 111.800%		
11) 1,1-Dichloroethene-d2	2.565	65	15077	5.088	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 101.800%		
20) 2-Butanone-d5	4.639	46	117766	63.695	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	= 127.400%		
24) Chloroform-d	5.063	84	74679	5.295	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 106.000%		
26) 1,2-Dichloroethane-d4	5.703	65	39563	5.464	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 109.200%		
32) Benzene-d6	5.729	84	150833	5.330	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 106.600%		
36) 1,2-Dichloropropane-d6	6.694	67	51038	5.477	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 109.600%		
41) Toluene-d8	7.899	98	121371	4.856	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 97.200%		
43) trans-1,3-Dichloroprop...	8.182	79	14641	4.385	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 87.600%		
46) 2-Hexanone-d5	8.636	63	75925	64.117	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 128.240%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	43449	5.310	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 106.200%		
66) 1,2-Dichlorobenzene-d4	12.195	152	39099	5.512	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 110.200%		
Target Compounds						Qvalue
16) Methylene chloride	3.044	84	6015	0.625	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050172.D
Acq On : 09 Aug 2022 08:04
Operator : SY/MD
Sample : VU0808WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK104

Quant Time: Aug 09 08:19:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 09 03:59:45 2022
Response via : Initial Calibration

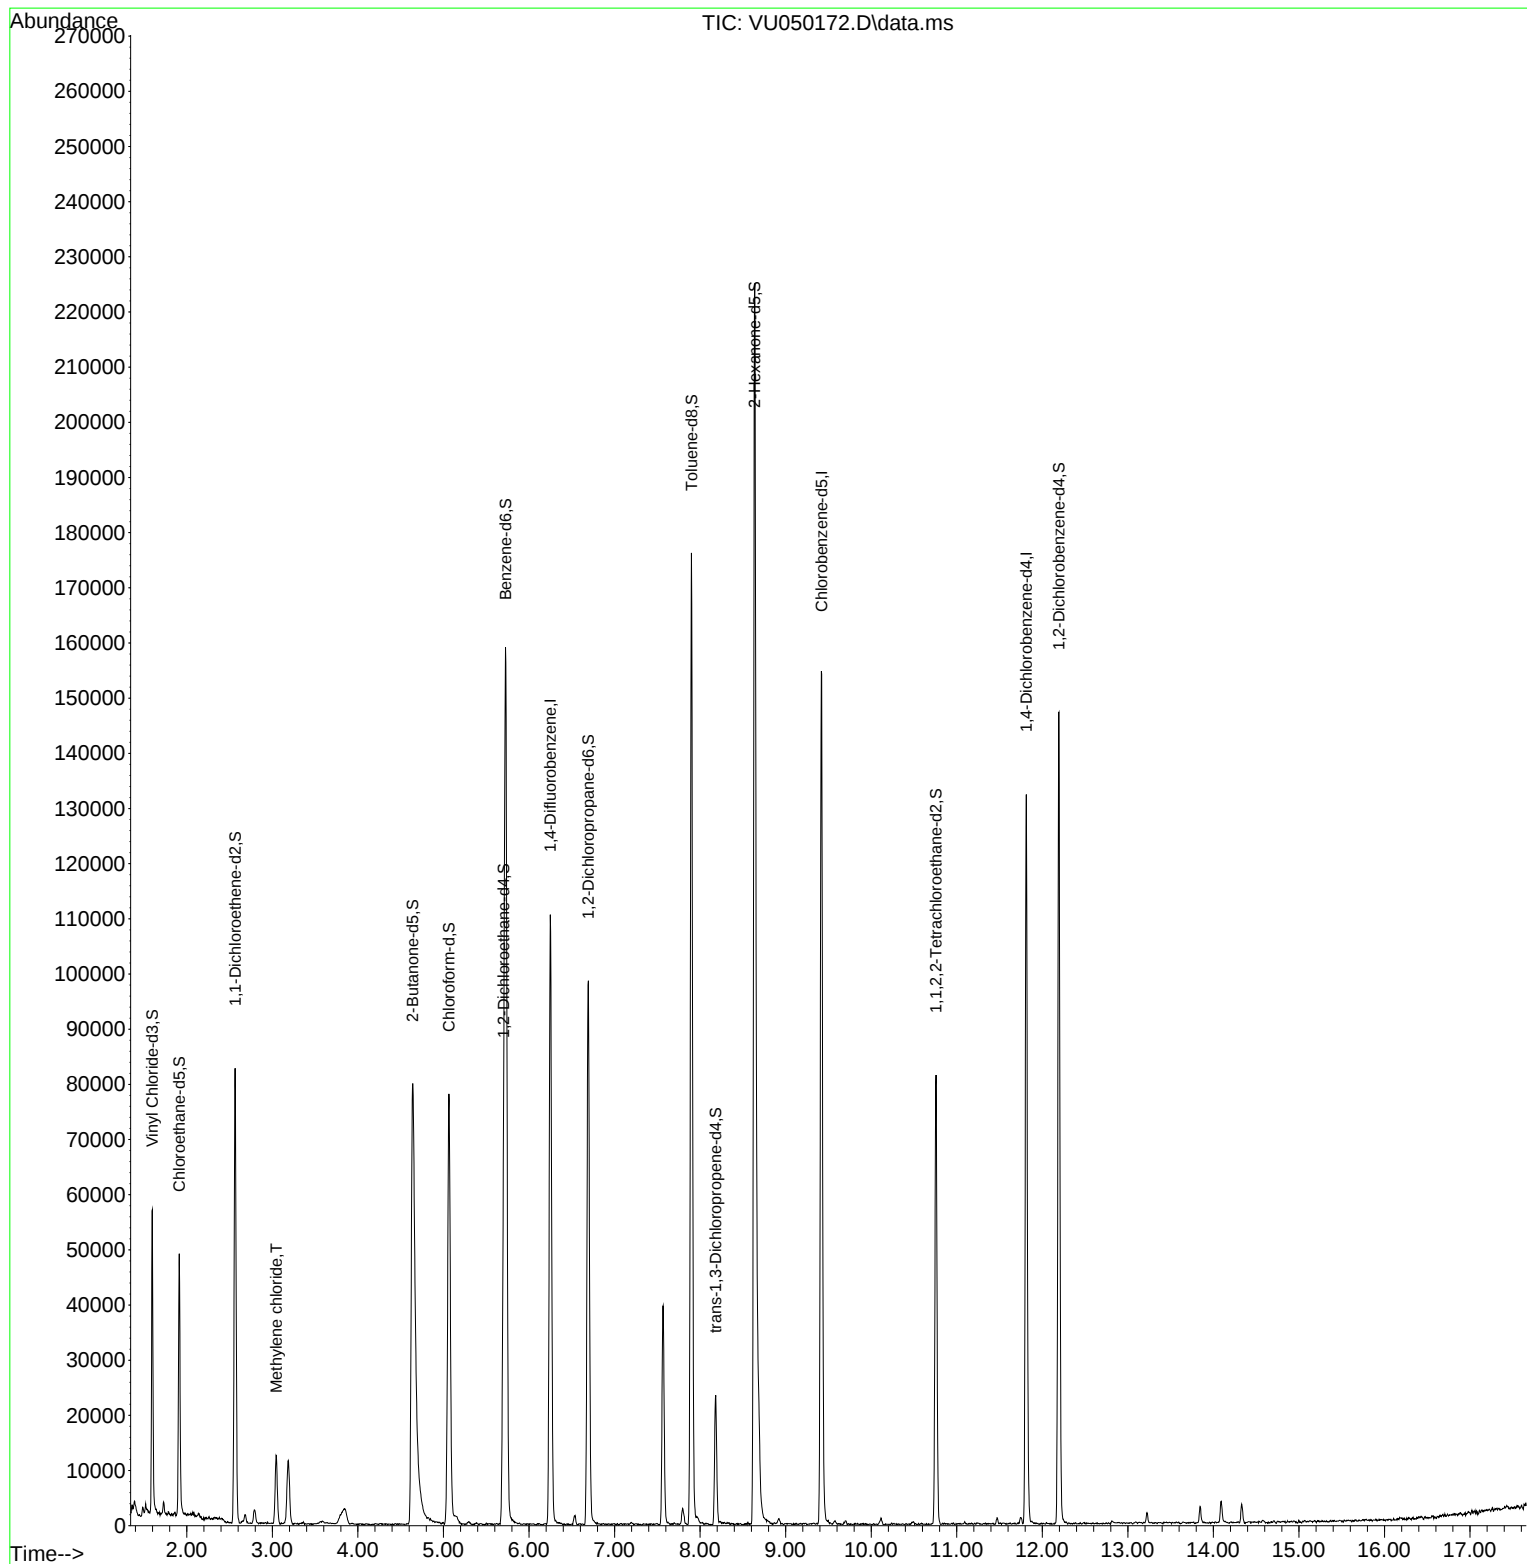

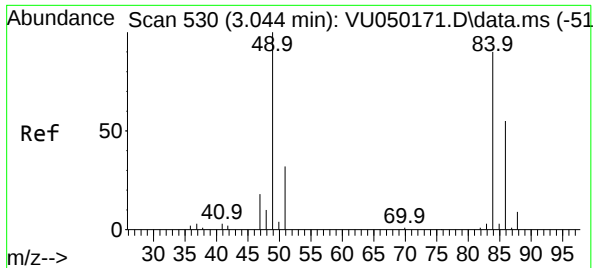

#16
Methylene chloride
Concen: 0.625 ug/L
RT: 3.044 min Scan# 51
Delta R.T. -0.000 min
Lab File: VU050172.D
Acq: 09 Aug 2022 08:04

Instrument :
MSVOA_U
ClientSampleId :
VBLK104

Tgt Ion:	84	Resp:	6015
Ion	Ratio	Lower	Upper
84	100		
86	66.5	45.9	85.3
49	118.4	77.6	144.0

