

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
 Data File : VU050188.D
 Acq On : 09 Aug 2022 17:00
 Operator : SY/MD
 Sample : N4075-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUV6

Quant Time: Aug 10 04:49:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 09 03:59:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	80007	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	82436	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	31846	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	21322	3.202	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	64.000%
7) Chloroethane-d5	1.909	69	22036	4.102	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.000%
11) 1,1-Dichloroethene-d2	2.562	65	8775	3.372	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.400%
20) 2-Butanone-d5	4.626	46	100983	62.194	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.380%
24) Chloroform-d	5.063	84	59264	4.785	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%
26) 1,2-Dichloroethane-d4	5.703	65	32168	5.059	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.200%
32) Benzene-d6	5.729	84	104587	4.066	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.400%
36) 1,2-Dichloropropane-d6	6.694	67	40042	4.727	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.600%
41) Toluene-d8	7.899	98	79586	3.503	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.000%
43) trans-1,3-Dichloroprop...	8.182	79	12600	4.151	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.000%
46) 2-Hexanone-d5	8.636	63	65365	60.719	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	121.440%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	38095	5.121	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.400%
66) 1,2-Dichlorobenzene-d4	12.195	152	29586	4.742	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.800%
Target Compounds						
16) Methylene chloride	3.044	84	4008	0.474	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050188.D
Acq On : 09 Aug 2022 17:00
Operator : SY/MD
Sample : N4075-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUV6

Quant Time: Aug 10 04:49:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 09 03:59:45 2022
Response via : Initial Calibration

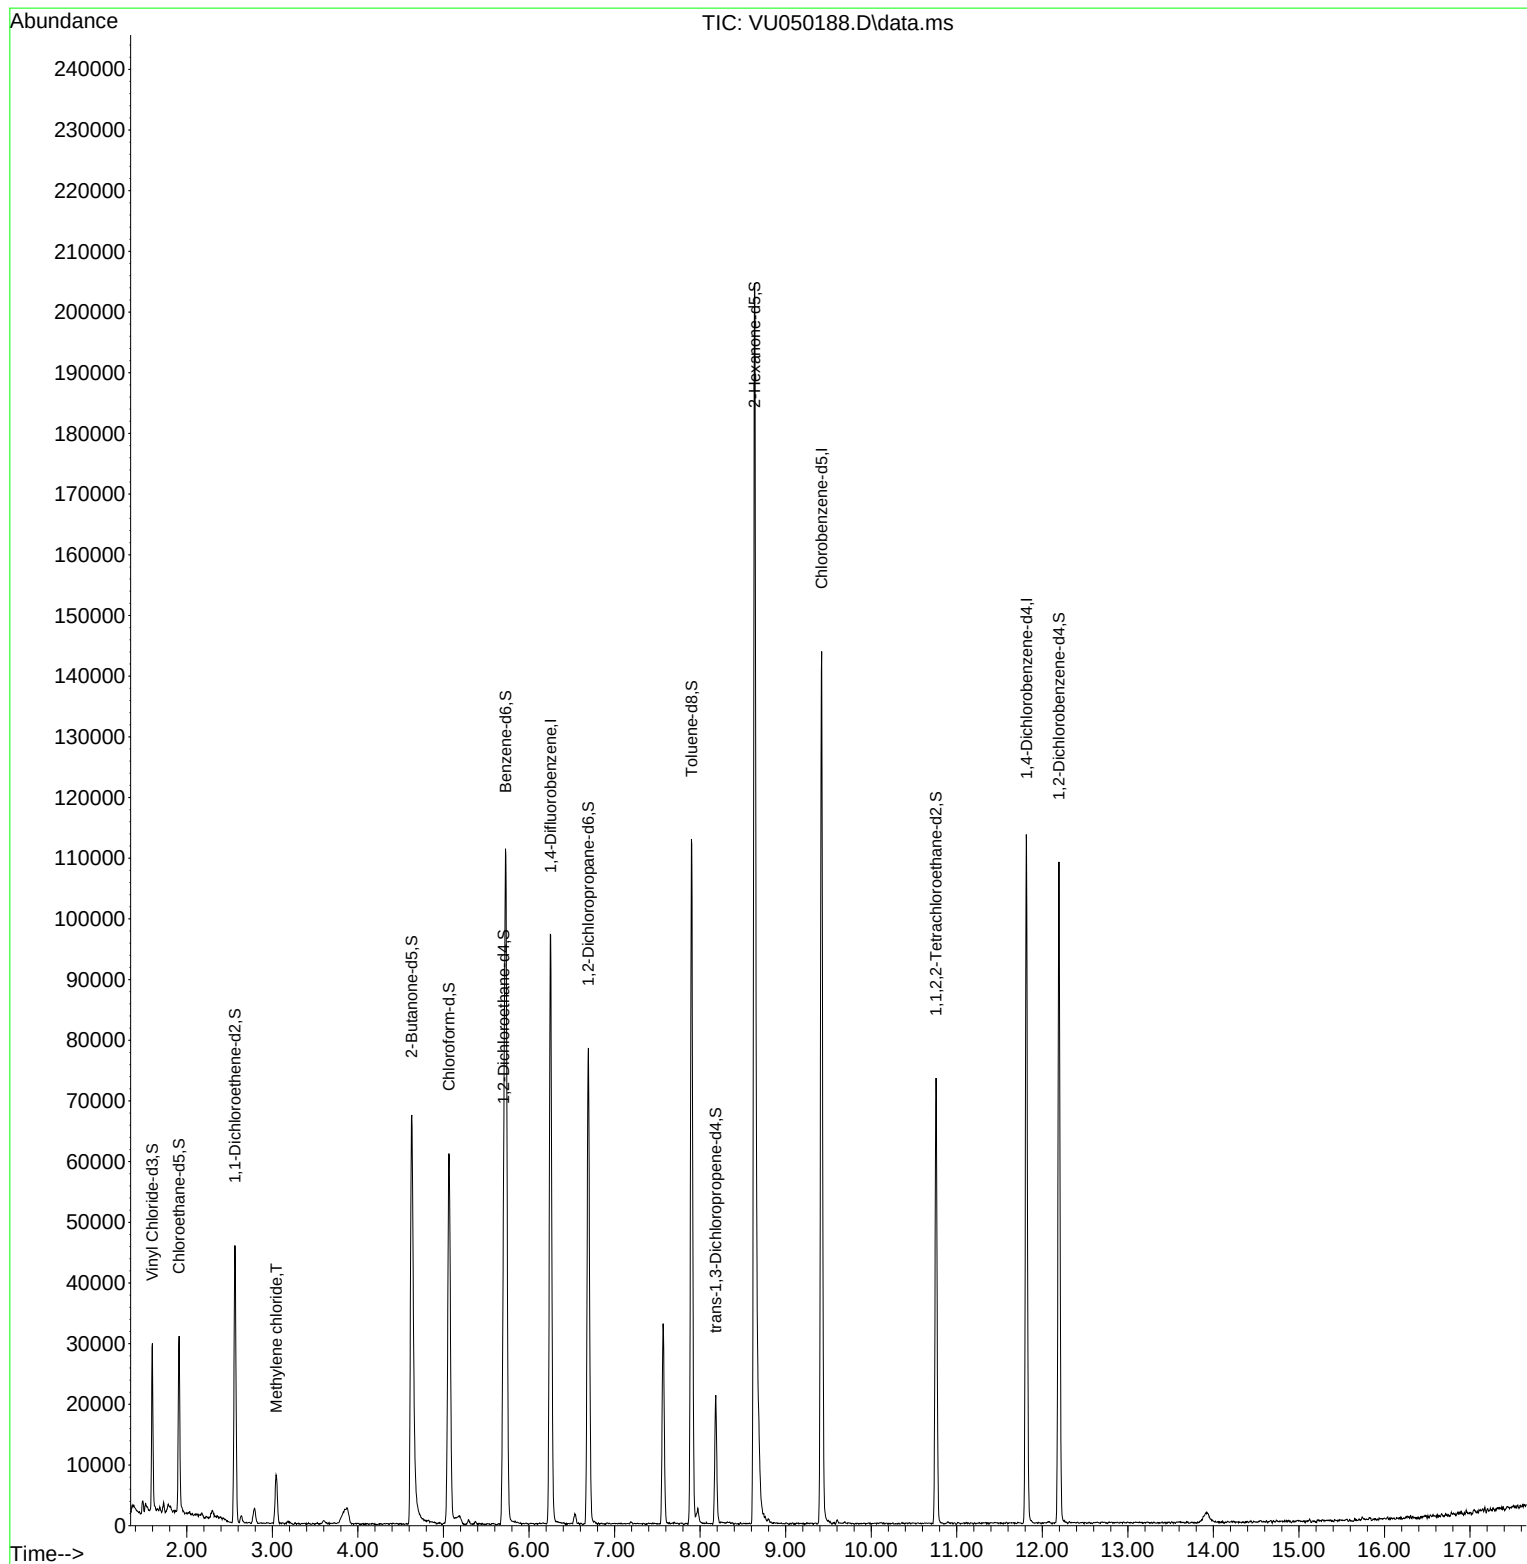

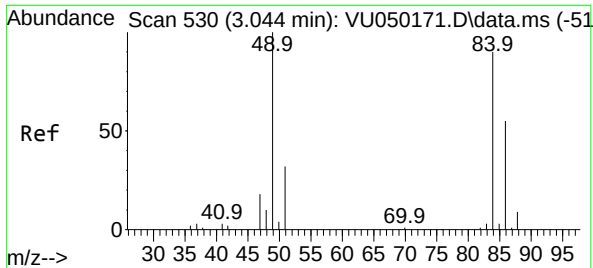

#16
Methylene chloride
Concen: 0.474 ug/L
RT: 3.044 min Scan# 51
Delta R.T. -0.000 min
Lab File: VU050188.D
Acq: 09 Aug 2022 17:00

Instrument :
MSVOA_U
ClientSampleId :
DBUV6

Tgt Ion: 84	Resp: 4008
Ion Ratio	Lower Upper
84	100
86	66.7 45.9 85.3
49	120.4 77.6 144.0

