

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
 Data File : VU050133.D
 Acq On : 08 Aug 2022 13:59
 Operator : SY/MD
 Sample : VU0808WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK102

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU050133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	96	rVB	34785	38982	8.86%	1.397%
2	1.912	169	178	193	rVB	33326	43541	9.89%	1.561%
3	2.562	369	380	393	rVB	55472	89084	20.24%	3.193%
4	3.044	521	530	540	rVB2	5387	9293	2.11%	0.333%
5	3.189	559	575	588	rVB	4606	9676	2.20%	0.347%
6	3.832	749	775	777	rBV	1884	5501	1.25%	0.197%
7	4.639	1012	1026	1066	rBV2	63211	212946	48.38%	7.633%
8	5.063	1143	1158	1180	rBV	64094	143971	32.71%	5.161%
9	5.186	1188	1196	1218	rVB	1768	5731	1.30%	0.205%
10	5.726	1341	1364	1387	rBV2	125141	327492	74.40%	11.739%
11	6.250	1514	1527	1542	rBV	105949	198658	45.13%	7.121%
12	6.694	1651	1665	1683	rBV	83584	161160	36.61%	5.777%
13	7.568	1919	1937	1957	rBV	37468	66987	15.22%	2.401%
14	7.899	2027	2040	2060	rBV	133065	232142	52.74%	8.321%
15	8.182	2117	2128	2141	rBV	22892	38549	8.76%	1.382%
16	8.639	2258	2270	2302	rBV3	191188	440154	100.00%	15.778%
17	9.420	2498	2513	2530	rBV	147482	251189	57.07%	9.004%
18	10.758	2914	2929	2947	rVB	74764	119435	27.13%	4.281%
19	11.812	3245	3257	3277	rBV	124464	197005	44.76%	7.062%
20	12.195	3363	3376	3395	rBV	119210	198202	45.03%	7.105%


Sum of corrected areas: 2789698

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050133.D
Acq On : 08 Aug 2022 13:59
Operator : SY/MD
Sample : VU0808WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

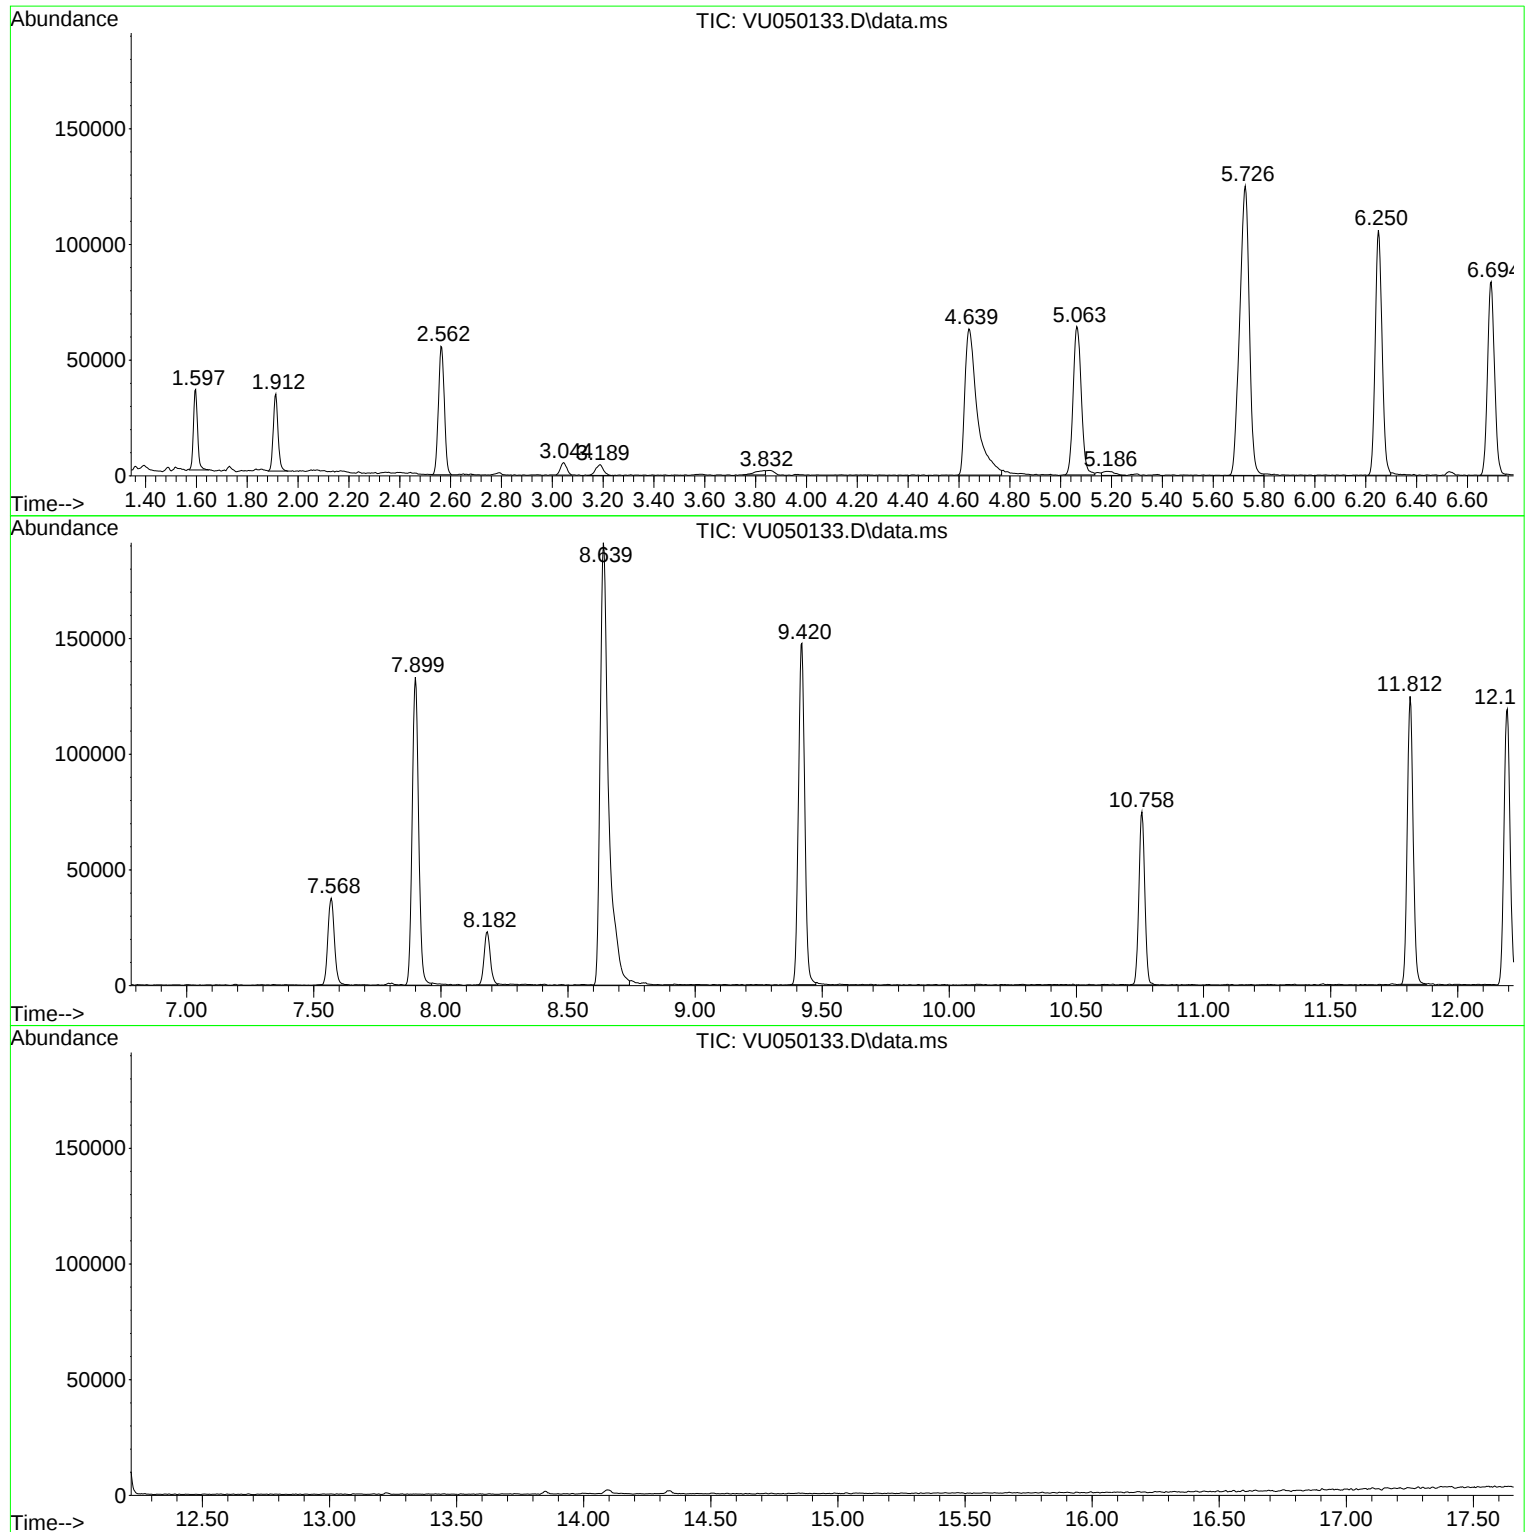

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050133.D
Acq On : 08 Aug 2022 13:59
Operator : SY/MD
Sample : VU0808WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050133.D
Acq On : 08 Aug 2022 13:59
Operator : SY/MD
Sample : VU0808WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
