

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
 Data File : VU050139.D
 Acq On : 08 Aug 2022 16:50
 Operator : SY/MD
 Sample : N4027-14DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBJH7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	91	rBV	32288	36889	8.78%	1.264%
2	1.729	115	121	130	rVB	8791	10435	2.48%	0.357%
3	1.909	169	177	196	rVB	32126	42407	10.09%	1.453%
4	2.565	367	381	394	rBV	53046	84386	20.09%	2.890%
5	3.044	517	530	545	rVB2	10842	20138	4.79%	0.690%
6	3.186	562	574	591	rVB	6184	14287	3.40%	0.489%
7	3.870	778	787	797	rVB3	2564	6186	1.47%	0.212%
8	4.629	1010	1023	1054	rBV2	75552	222494	52.96%	7.621%
9	5.063	1141	1158	1177	rBV	64444	142484	33.92%	4.880%
10	5.726	1345	1364	1382	rBV2	119284	312402	74.36%	10.700%
11	6.250	1514	1527	1544	rBV	101853	192333	45.78%	6.588%
12	6.546	1606	1619	1635	rBV	103210	199562	47.50%	6.835%
13	6.694	1648	1665	1683	rBV	82135	158486	37.73%	5.428%
14	7.568	1926	1937	1953	rBV	36582	62891	14.97%	2.154%
15	7.899	2028	2040	2068	rBV	125641	221162	52.65%	7.575%
16	8.182	2117	2128	2140	rBV	21779	36647	8.72%	1.255%
17	8.639	2257	2270	2305	rBV2	190472	420096	100.00%	14.389%
18	9.420	2500	2513	2530	rBV	143310	242226	57.66%	8.297%
19	10.758	2917	2929	2945	rBV	72496	115591	27.52%	3.959%
20	11.812	3244	3257	3272	rBV	118850	189267	45.05%	6.483%
21	12.195	3361	3376	3396	rBV	114269	189206	45.04%	6.481%




Sum of corrected areas: 2919575

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050139.D
Acq On : 08 Aug 2022 16:50
Operator : SY/MD
Sample : N4027-14DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJH7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

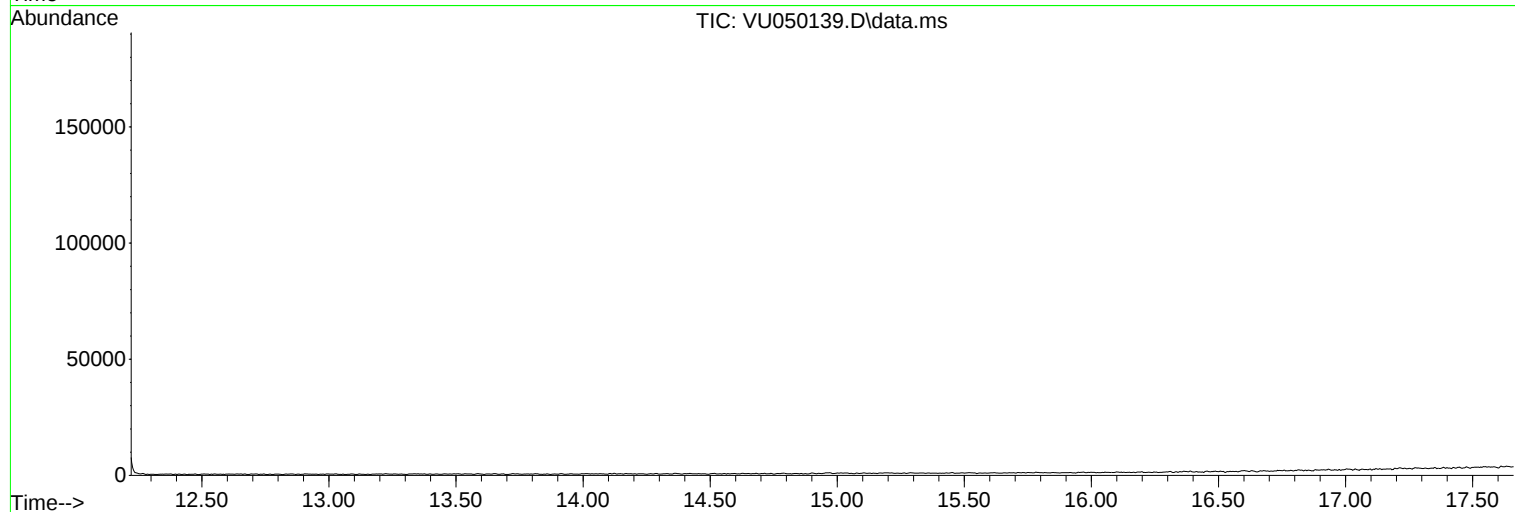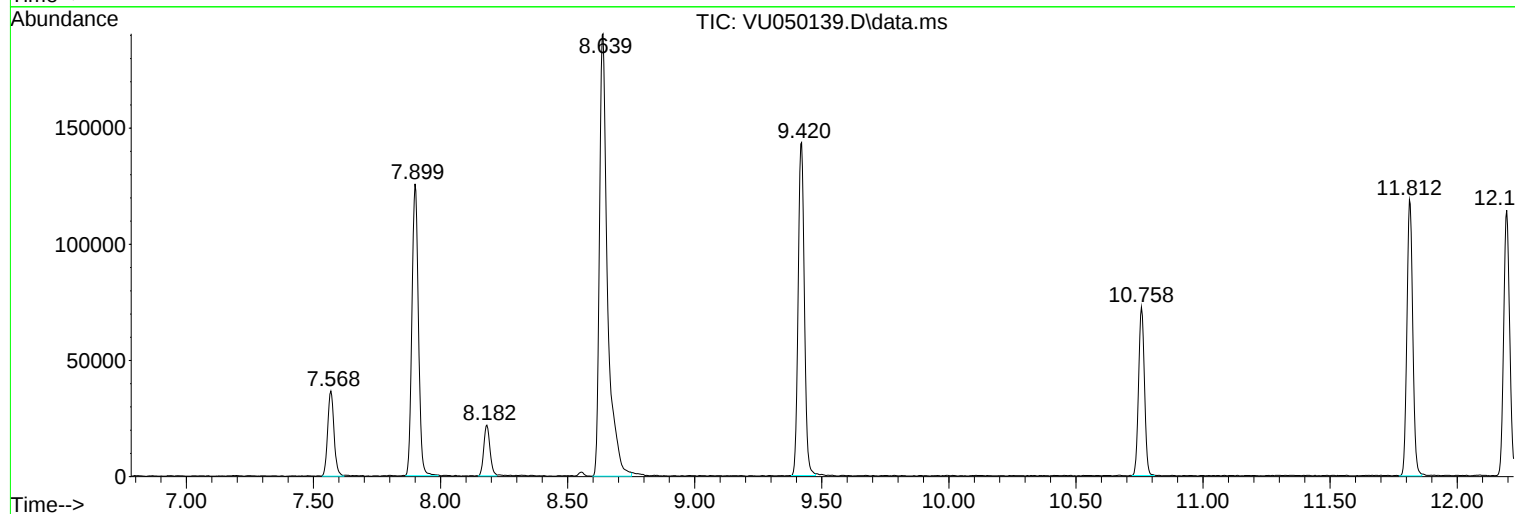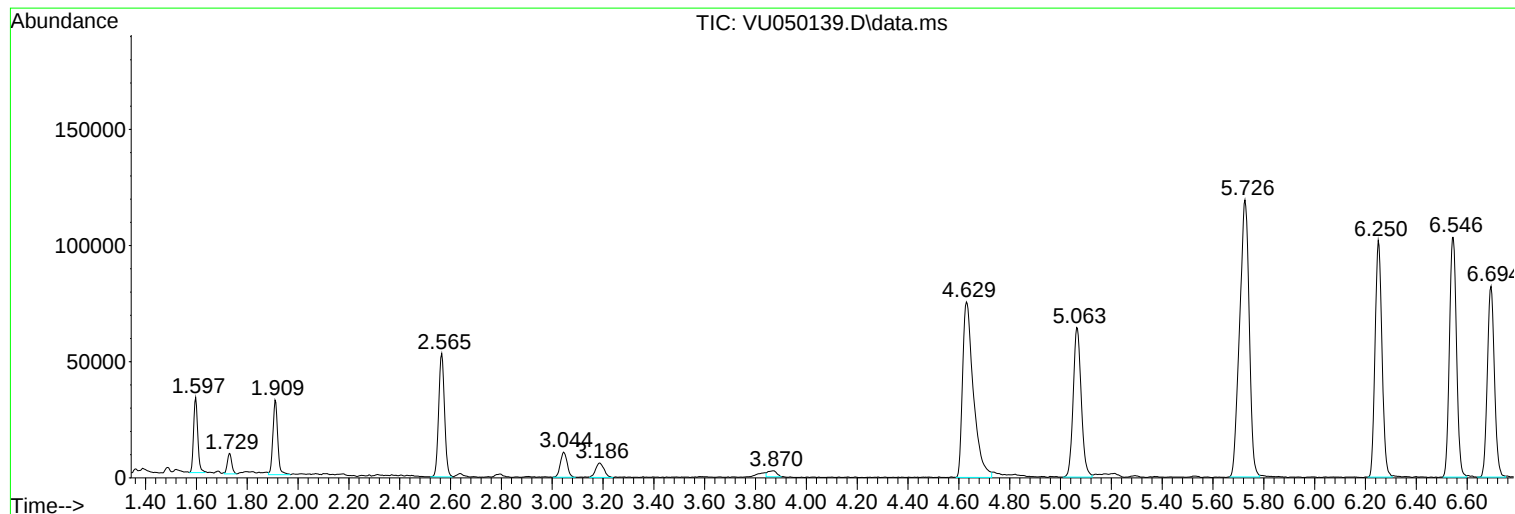

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050139.D
Acq On : 08 Aug 2022 16:50
Operator : SY/MD
Sample : N4027-14DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJH7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050139.D
Acq On : 08 Aug 2022 16:50
Operator : SY/MD
Sample : N4027-14DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJH7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
