

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
 Data File : VU050164.D
 Acq On : 09 Aug 2022 03:58
 Operator : SY/MD
 Sample : N4075-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUV7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU050164.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	91	rBV2	42880	51043	12.24%	1.933%
2	1.909	168	177	193	rVB	30824	40987	9.83%	1.552%
3	2.565	368	381	395	rVB	49474	80277	19.26%	3.040%
4	2.642	395	405	420	rVB	3623	7208	1.73%	0.273%
5	2.790	439	451	461	rBV2	3277	6358	1.53%	0.241%
6	3.359	612	628	648	rBV3	62283	148360	35.59%	5.618%
7	3.877	768	789	791	rBV	2577	4580	1.10%	0.173%
8	4.632	1011	1024	1061	rBV	62513	189008	45.34%	7.157%
9	5.063	1143	1158	1176	rBV2	58645	129066	30.96%	4.887%
10	5.726	1343	1364	1382	rBV2	110935	293837	70.48%	11.126%
11	5.944	1421	1432	1448	rVB4	2692	5888	1.41%	0.223%
12	6.250	1514	1527	1544	rBV	86123	164422	39.44%	6.226%
13	6.690	1651	1664	1685	rBV	76121	149011	35.74%	5.642%
14	7.568	1924	1937	1952	rBV2	30448	53295	12.78%	2.018%
15	7.899	2026	2040	2055	rBV	115015	202522	48.58%	7.669%
16	8.182	2115	2128	2146	rBV2	18985	32448	7.78%	1.229%
17	8.639	2257	2270	2301	rBV3	193885	416899	100.00%	15.786%
18	9.417	2500	2512	2532	rBV	123576	208920	50.11%	7.911%
19	10.758	2917	2929	2943	rBV	70271	112682	27.03%	4.267%
20	11.812	3243	3257	3277	rBV	101297	162820	39.06%	6.165%
21	12.195	3363	3376	3396	rBV	108615	181286	43.48%	6.865%




Sum of corrected areas: 2640917

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050164.D
Acq On : 09 Aug 2022 03:58
Operator : SY/MD
Sample : N4075-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUV7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

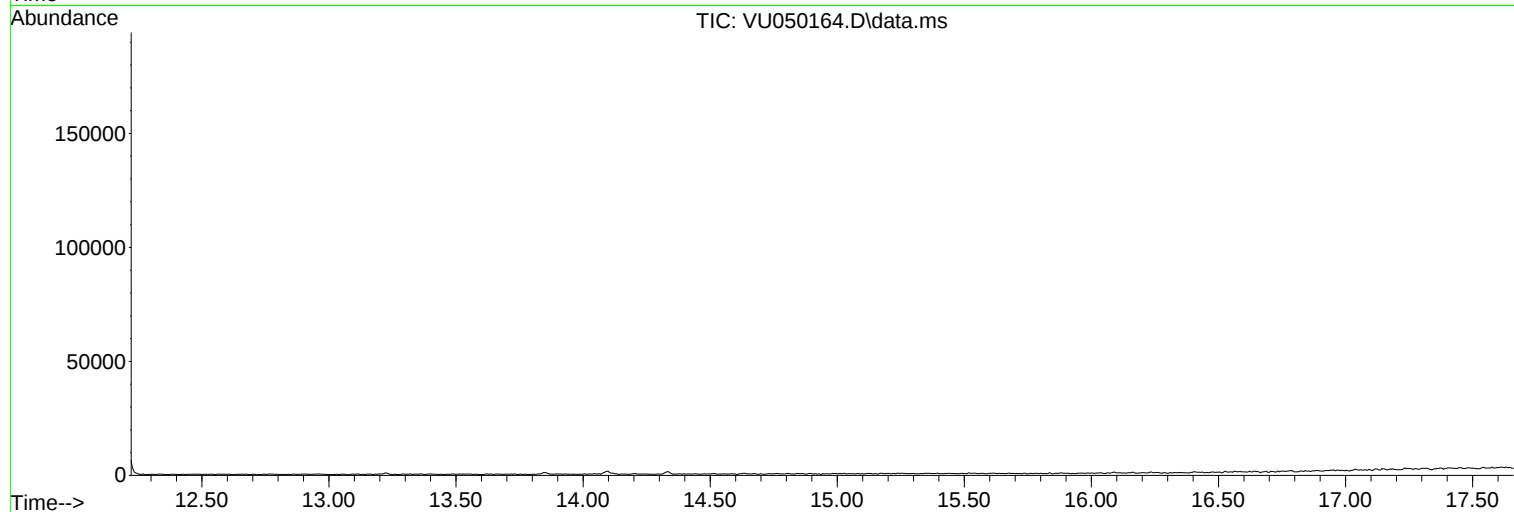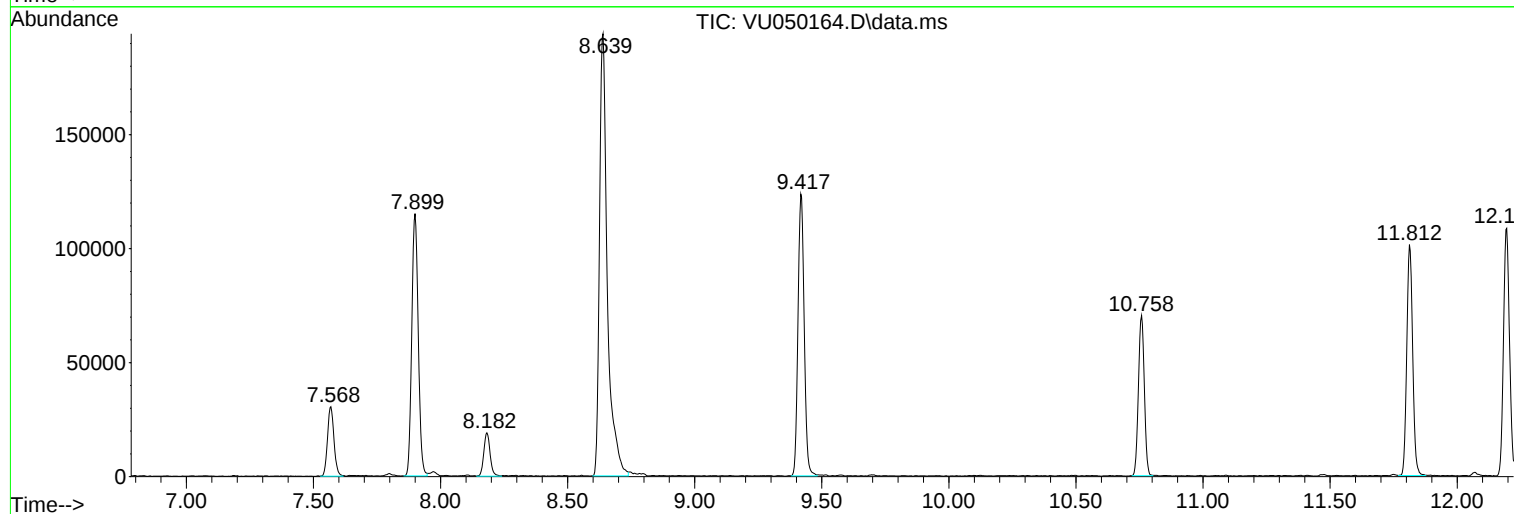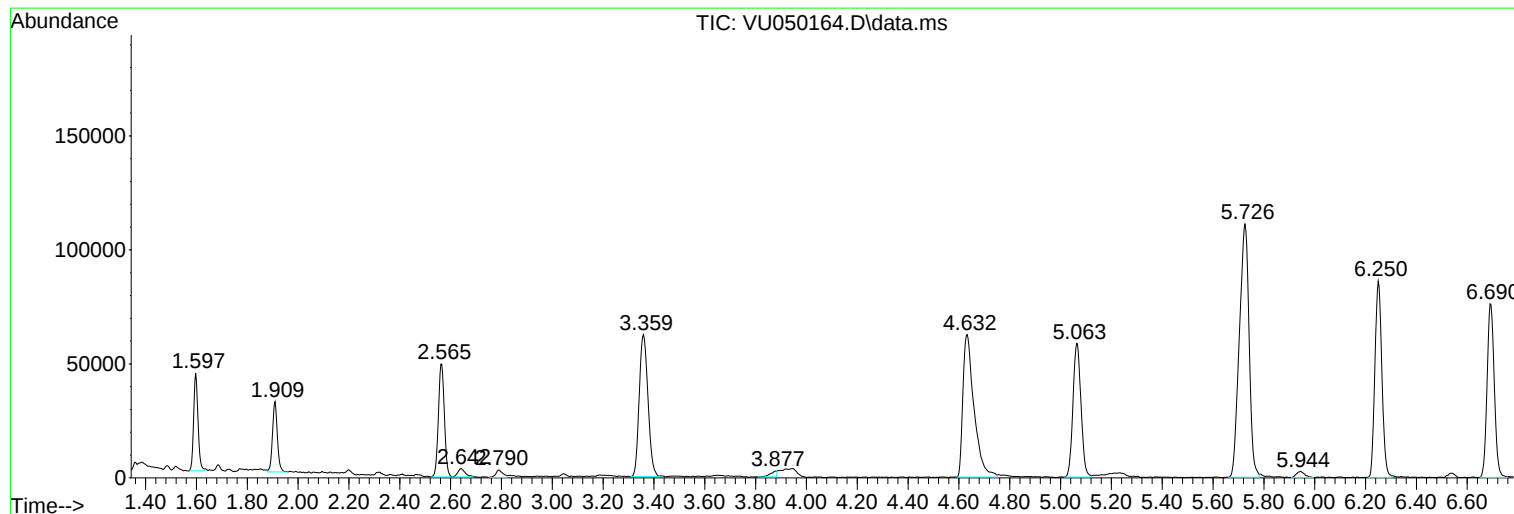

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050164.D
Acq On : 09 Aug 2022 03:58
Operator : SY/MD
Sample : N4075-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUV7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050164.D
Acq On : 09 Aug 2022 03:58
Operator : SY/MD
Sample : N4075-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUV7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc