

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
 Data File : VU050172.D
 Acq On : 09 Aug 2022 08:04
 Operator : SY/MD
 Sample : VU0808WBL03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK104

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	71	80	94	rBV	55038	63228	13.06%	1.901%
2	1.912	169	178	193	rBV	47058	60013	12.40%	1.805%
3	2.565	368	381	397	rBV	82477	133264	27.53%	4.008%
4	3.044	520	530	544	rVB	12480	22366	4.62%	0.673%
5	3.186	561	574	590	rVB	11548	25363	5.24%	0.763%
6	4.639	1011	1026	1079	rBV2	79794	277104	57.25%	8.333%
7	5.063	1142	1158	1177	rBV	78053	173401	35.82%	5.215%
8	5.726	1344	1364	1387	rBV2	158933	405349	83.74%	12.190%
9	6.250	1513	1527	1544	rBV	110563	209789	43.34%	6.309%
10	6.694	1651	1665	1691	rBV	98542	192467	39.76%	5.788%
11	7.568	1925	1937	1952	rBV	39668	69562	14.37%	2.092%
12	7.796	1994	2008	2018	rBV3	2920	5453	1.13%	0.164%
13	7.899	2026	2040	2056	rBV	176137	303731	62.75%	9.134%
14	8.182	2117	2128	2140	rBV	23458	40087	8.28%	1.206%
15	8.639	2257	2270	2303	rBV2	224859	484059	100.00%	14.557%
16	9.417	2499	2512	2535	rBV	154589	265243	54.80%	7.977%
17	10.758	2916	2929	2947	rVB	81466	131881	27.24%	3.966%
18	11.812	3244	3257	3274	rBV	132196	212449	43.89%	6.389%
19	12.195	3361	3376	3391	rBV	147077	239192	49.41%	7.193%
20	14.092	3957	3966	3977	rBV	3844	6021	1.24%	0.181%
21	14.330	4032	4040	4051	rVB3	3454	5182	1.07%	0.156%




Sum of corrected areas: 3325204

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050172.D
Acq On : 09 Aug 2022 08:04
Operator : SY/MD
Sample : VU0808WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK104

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

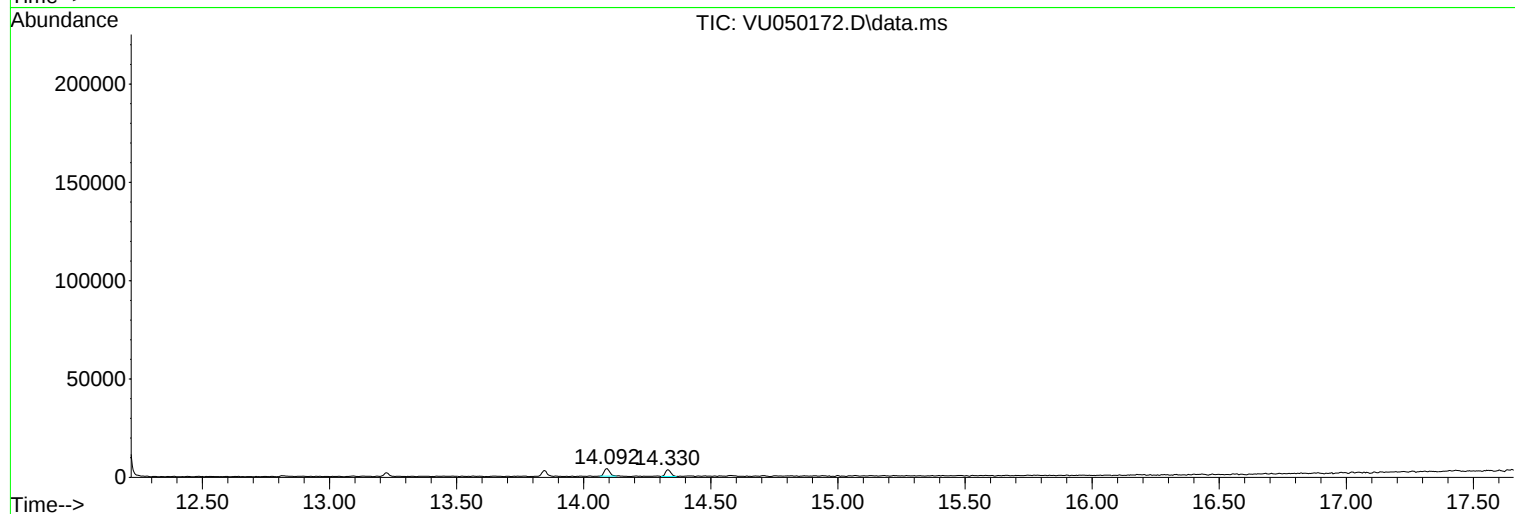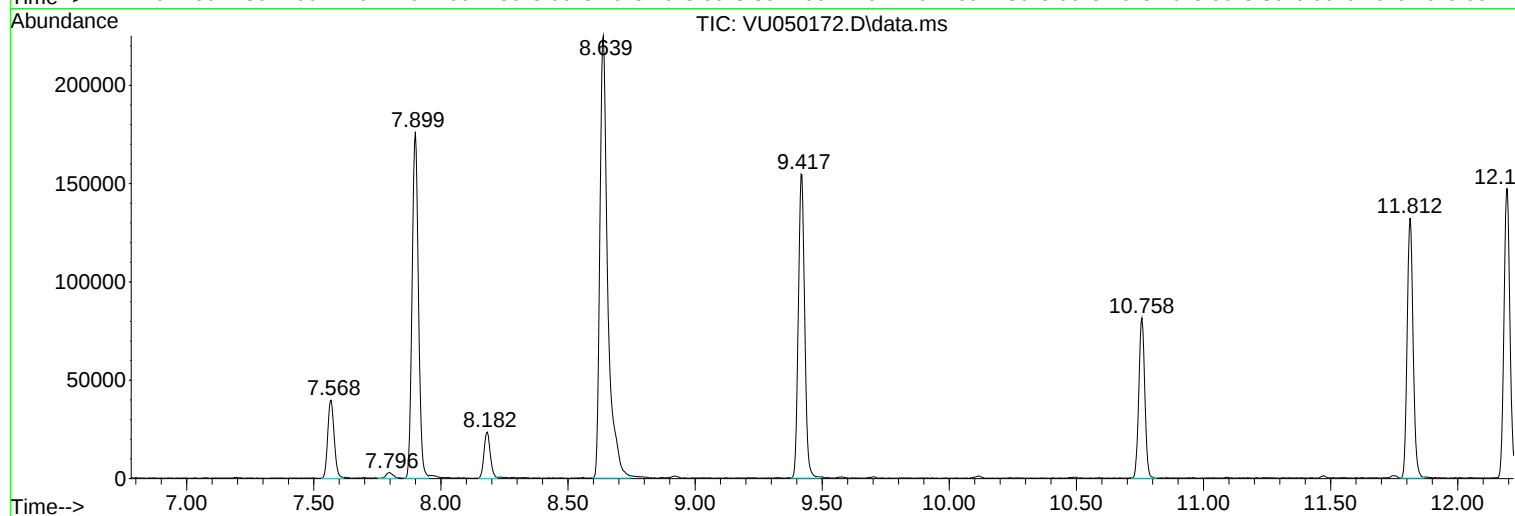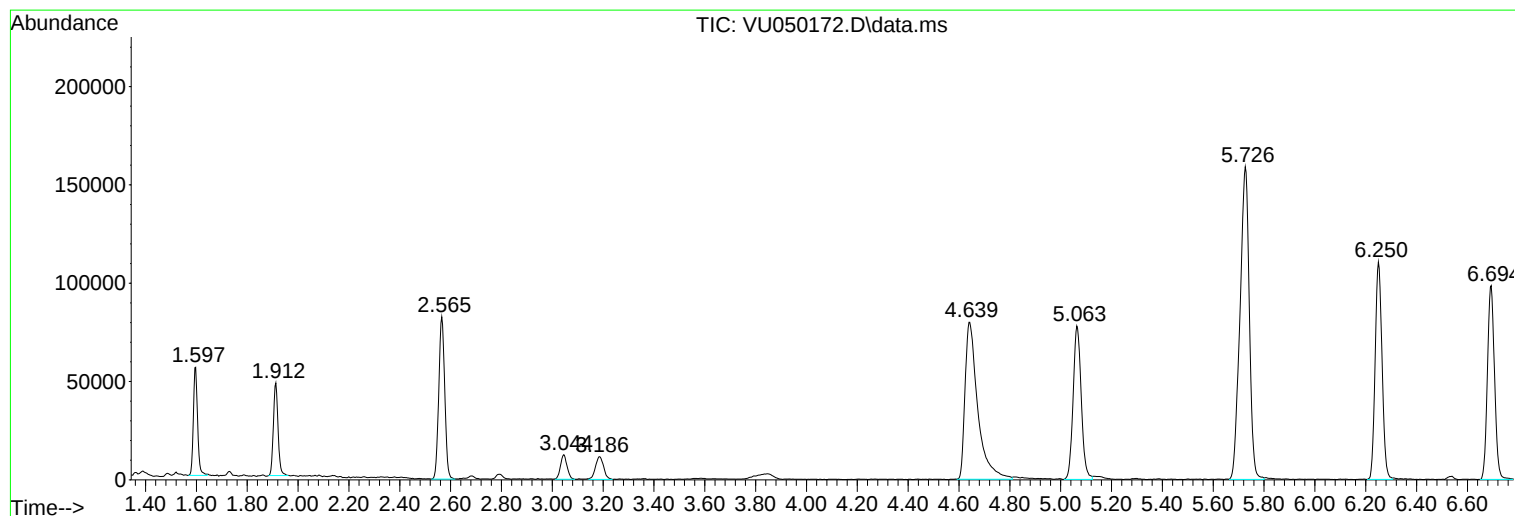

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050172.D
Acq On : 09 Aug 2022 08:04
Operator : SY/MD
Sample : VU0808WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK104

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050172.D
Acq On : 09 Aug 2022 08:04
Operator : SY/MD
Sample : VU0808WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK104

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc