

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
 Data File : VU050182.D
 Acq On : 09 Aug 2022 14:31
 Operator : SY/MD
 Sample : N4075-11DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUX8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU050182.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	71	80	89	rBV	30436	34183	8.16%	1.228%
2	1.909	169	177	191	rBV	29228	37869	9.03%	1.361%
3	2.565	369	381	393	rVB	48270	76474	18.24%	2.748%
4	3.044	516	530	543	rBV	13327	23977	5.72%	0.862%
5	3.189	562	575	589	rBV2	4974	10734	2.56%	0.386%
6	3.366	614	630	657	rVB2	72628	167085	39.86%	6.004%
7	4.626	1009	1022	1051	rBV	72906	188541	44.98%	6.775%
8	5.066	1143	1159	1175	rBV	63693	138813	33.12%	4.988%
9	5.726	1344	1364	1385	rBV3	113133	302374	72.14%	10.865%
10	5.944	1422	1432	1446	rVB2	2462	4905	1.17%	0.176%
11	6.250	1513	1527	1547	rBV	100830	189907	45.31%	6.824%
12	6.542	1605	1618	1629	rVB5	6379	12166	2.90%	0.437%
13	6.693	1652	1665	1687	rBV2	78523	154066	36.76%	5.536%
14	7.568	1925	1937	1954	rBV	34637	58676	14.00%	2.108%
15	7.899	2025	2040	2060	rBV	117133	205683	49.07%	7.391%
16	8.182	2117	2128	2142	rBV	20456	33302	7.94%	1.197%
17	8.635	2256	2269	2306	rBV2	191605	419162	100.00%	15.062%
18	9.420	2500	2513	2539	rBV	142690	240556	57.39%	8.644%
19	10.758	2915	2929	2948	rVB	72072	116529	27.80%	4.187%
20	11.812	3246	3257	3274	rBV	114816	184417	44.00%	6.627%
21	12.195	3364	3376	3392	rBV	113939	183566	43.79%	6.596%




Sum of corrected areas: 2782985

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050182.D
Acq On : 09 Aug 2022 14:31
Operator : SY/MD
Sample : N4075-11DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUX8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

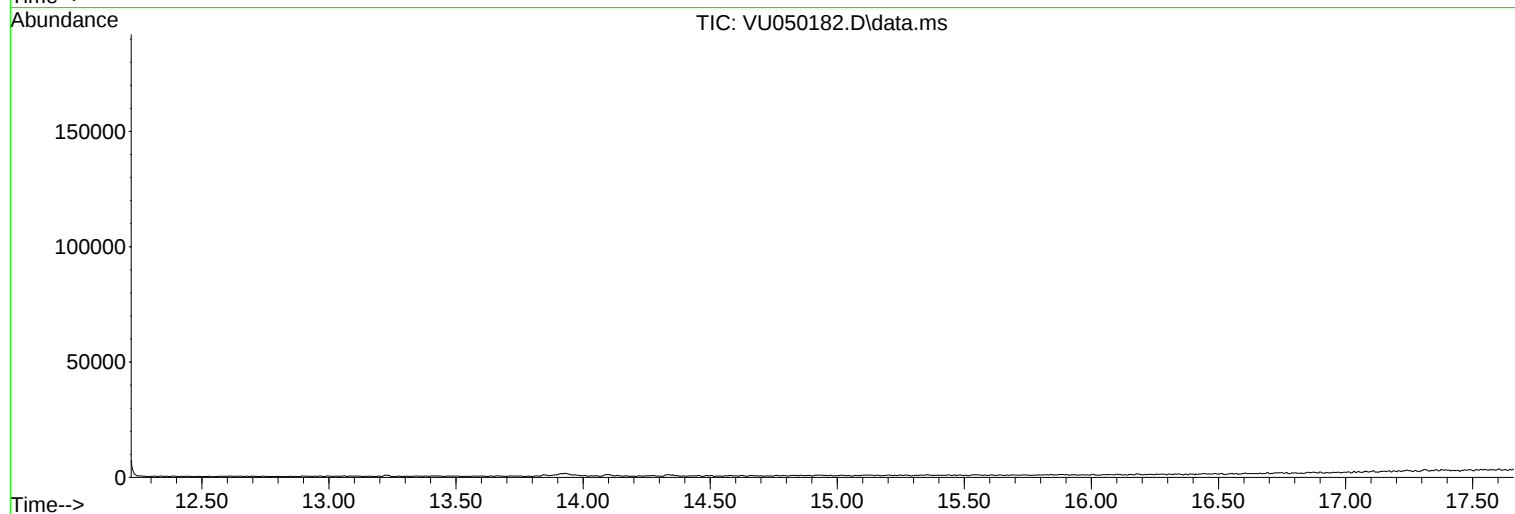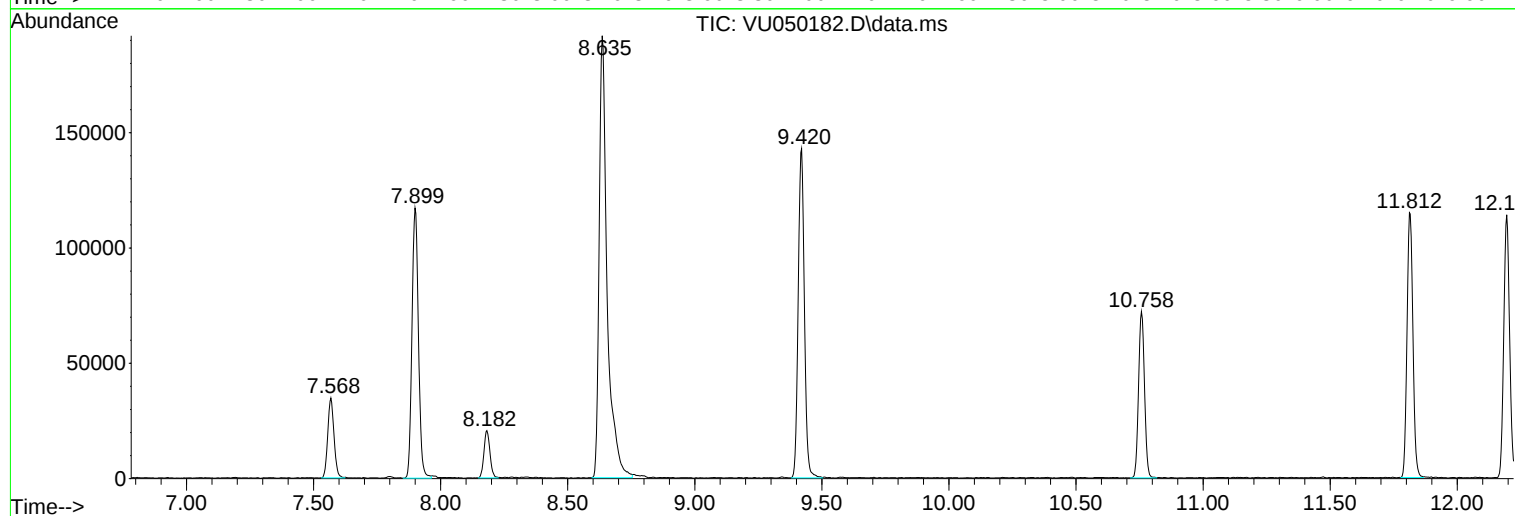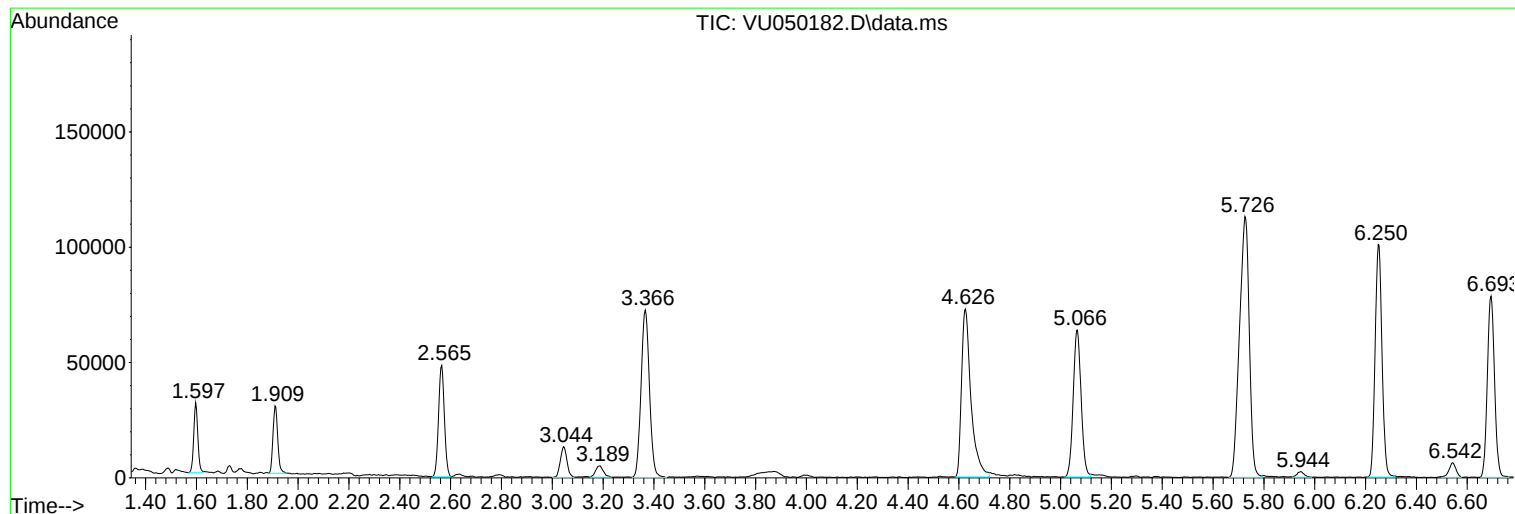

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050182.D
Acq On : 09 Aug 2022 14:31
Operator : SY/MD
Sample : N4075-11DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUX8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050182.D
Acq On : 09 Aug 2022 14:31
Operator : SY/MD
Sample : N4075-11DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUX8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc