

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
 Data File : VU050184.D
 Acq On : 09 Aug 2022 15:21
 Operator : SY/MD
 Sample : N4075-13DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUY0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	71	80	92	rBV	28933	33070	8.04%	1.219%
2	1.909	169	177	194	rVB	29098	38309	9.31%	1.412%
3	2.565	370	381	393	rBV2	45695	73035	17.75%	2.692%
4	3.044	520	530	542	rVB	11717	21090	5.13%	0.777%
5	3.189	563	575	584	rBV2	3735	7451	1.81%	0.275%
6	3.366	613	630	648	rBV	61666	139025	33.79%	5.124%
7	4.626	1009	1022	1048	rBV	69681	174661	42.45%	6.437%
8	5.067	1143	1159	1181	rBV2	60697	134287	32.64%	4.949%
9	5.726	1342	1364	1382	rBV3	112066	295135	71.73%	10.877%
10	5.945	1420	1432	1443	rBV3	4778	9166	2.23%	0.338%
11	6.250	1514	1527	1546	rBV	101544	195191	47.44%	7.194%
12	6.543	1606	1618	1626	rBV6	3153	5967	1.45%	0.220%
13	6.694	1652	1665	1680	rBV	76425	149753	36.39%	5.519%
14	7.568	1926	1937	1949	rBV	32257	56203	13.66%	2.071%
15	7.899	2026	2040	2071	rBV	115527	201338	48.93%	7.420%
16	8.182	2118	2128	2142	rBV	19995	32300	7.85%	1.190%
17	8.636	2257	2269	2313	rBV2	185684	411479	100.00%	15.165%
18	9.420	2500	2513	2536	rBV	145409	250975	60.99%	9.249%
19	10.758	2915	2929	2944	rBV	72263	115175	27.99%	4.245%
20	11.812	3245	3257	3276	rBV	120061	191213	46.47%	7.047%
21	12.195	3364	3376	3395	rBV	107792	178597	43.40%	6.582%




Sum of corrected areas: 2713420

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050184.D
Acq On : 09 Aug 2022 15:21
Operator : SY/MD
Sample : N4075-13DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUY0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

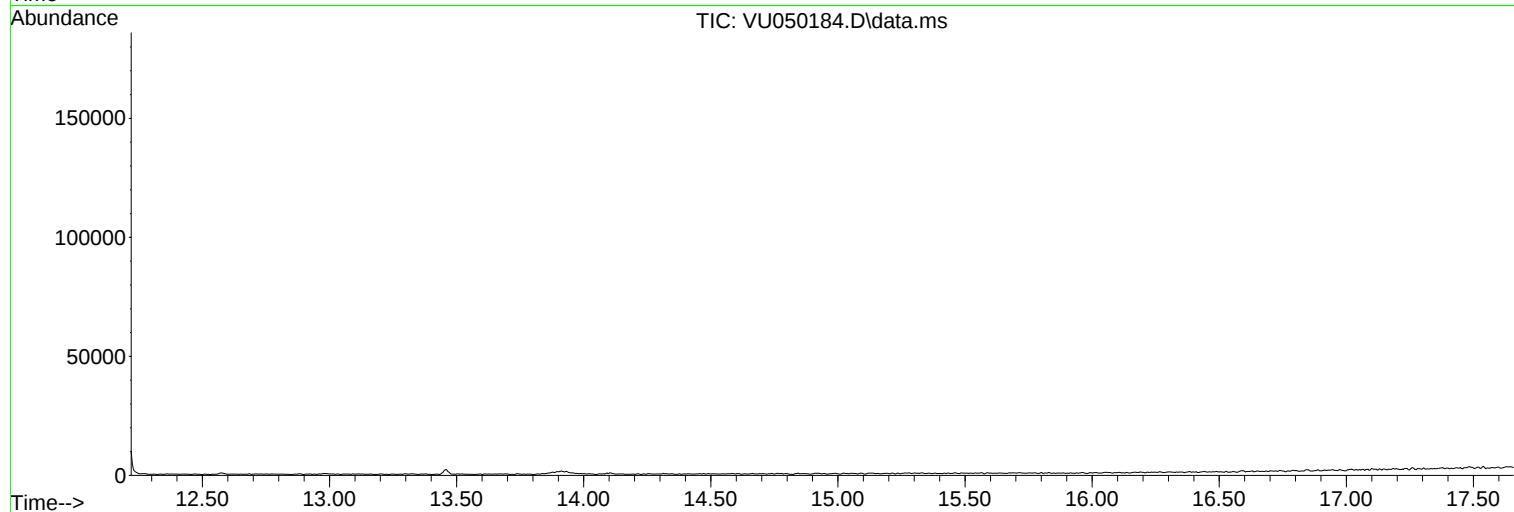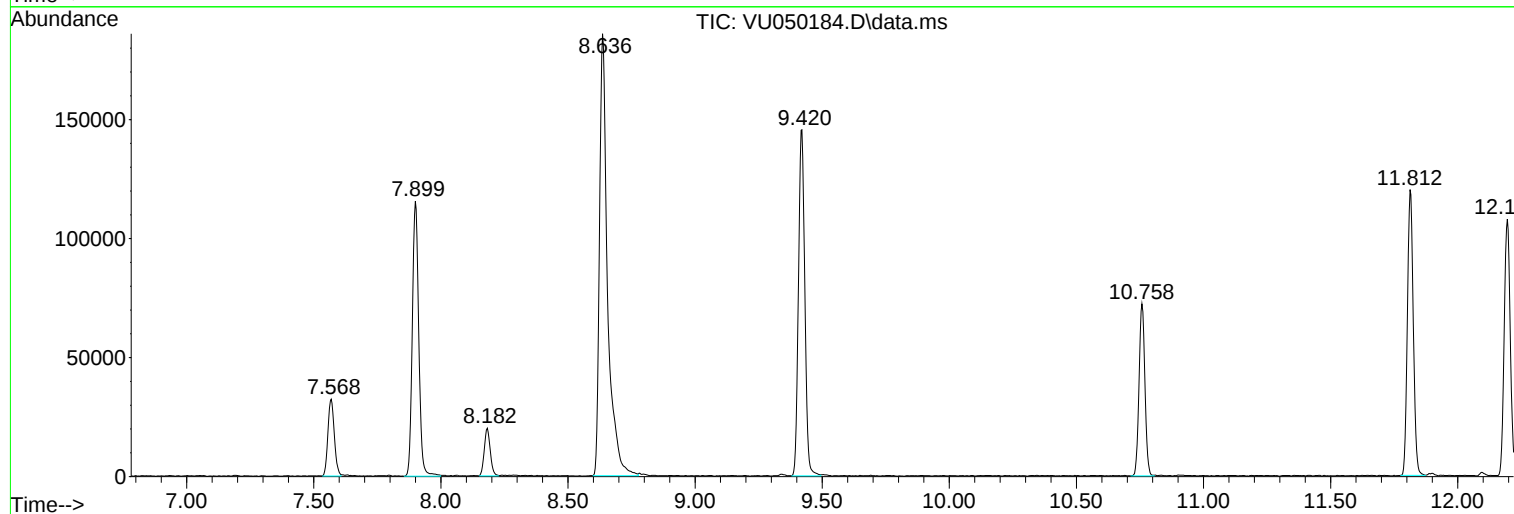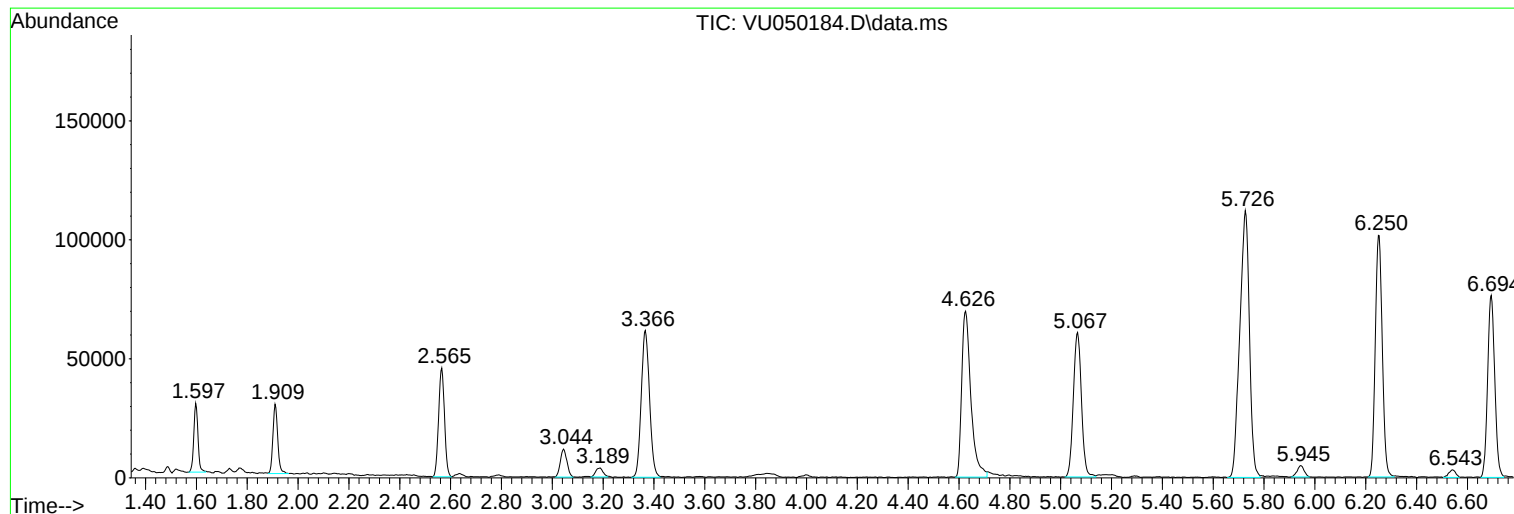

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050184.D
Acq On : 09 Aug 2022 15:21
Operator : SY/MD
Sample : N4075-13DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUY0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050184.D
Acq On : 09 Aug 2022 15:21
Operator : SY/MD
Sample : N4075-13DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUY0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc