

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
 Data File : VU050187.D
 Acq On : 09 Aug 2022 16:35
 Operator : SY/MD
 Sample : N4075-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUV5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.356	3	5	27	rVB3	7864	14134	3.40%	0.574%
2	1.597	72	80	90	rBV	34310	39218	9.44%	1.592%
3	1.909	170	177	198	rVB	29667	41112	9.90%	1.669%
4	2.562	369	380	392	rBV	46028	74709	17.99%	3.032%
5	2.626	392	400	411	rVB	3577	5853	1.41%	0.238%
6	2.765	424	443	464	rBV3	6297	17127	4.12%	0.695%
7	3.842	754	778	781	rBV	2309	6641	1.60%	0.270%
8	4.626	1009	1022	1045	rBV2	68140	168147	40.49%	6.825%
9	5.067	1143	1159	1179	rBV	59474	129994	31.30%	5.277%
10	5.726	1345	1364	1382	rBV2	107033	286877	69.07%	11.645%
11	6.250	1514	1527	1547	rBV	91988	174385	41.99%	7.078%
12	6.533	1607	1615	1629	rVB8	2203	4509	1.09%	0.183%
13	6.694	1650	1665	1686	rVB	75405	146552	35.29%	5.949%
14	7.568	1925	1937	1954	rBV	31591	54439	13.11%	2.210%
15	7.899	2028	2040	2055	rBV	109388	188546	45.40%	7.653%
16	8.182	2115	2128	2142	rBV2	19540	32339	7.79%	1.313%
17	8.636	2256	2269	2304	rBV2	199569	415321	100.00%	16.858%
18	9.420	2501	2513	2533	rBV	131105	219928	52.95%	8.927%
19	10.758	2918	2929	2949	rVB	70094	114402	27.55%	4.644%
20	11.816	3247	3258	3279	rBV	100502	162954	39.24%	6.614%
21	12.195	3365	3376	3395	rBV	102938	166439	40.07%	6.756%




Sum of corrected areas: 2463626

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050187.D
Acq On : 09 Aug 2022 16:35
Operator : SY/MD
Sample : N4075-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUV5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

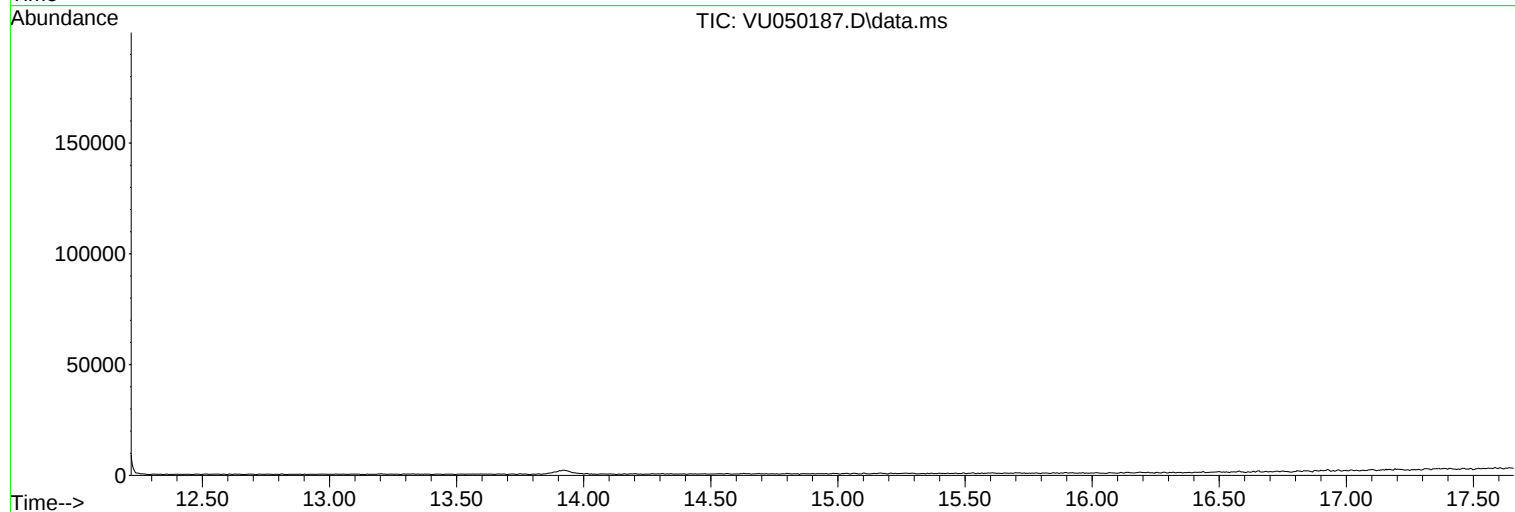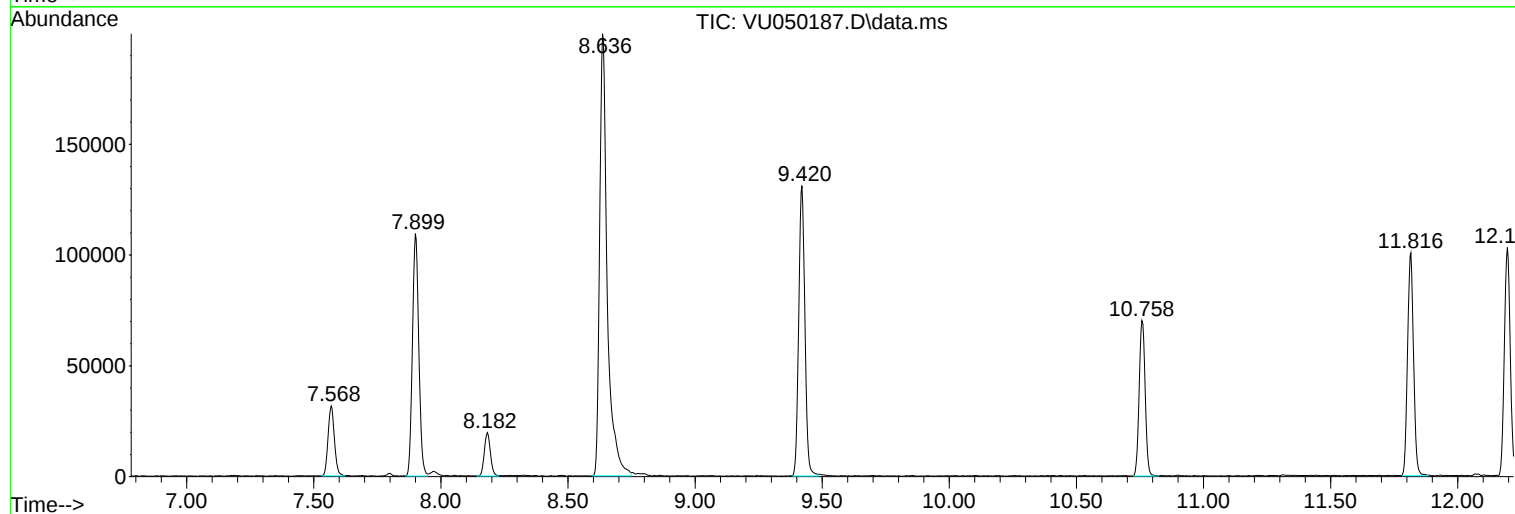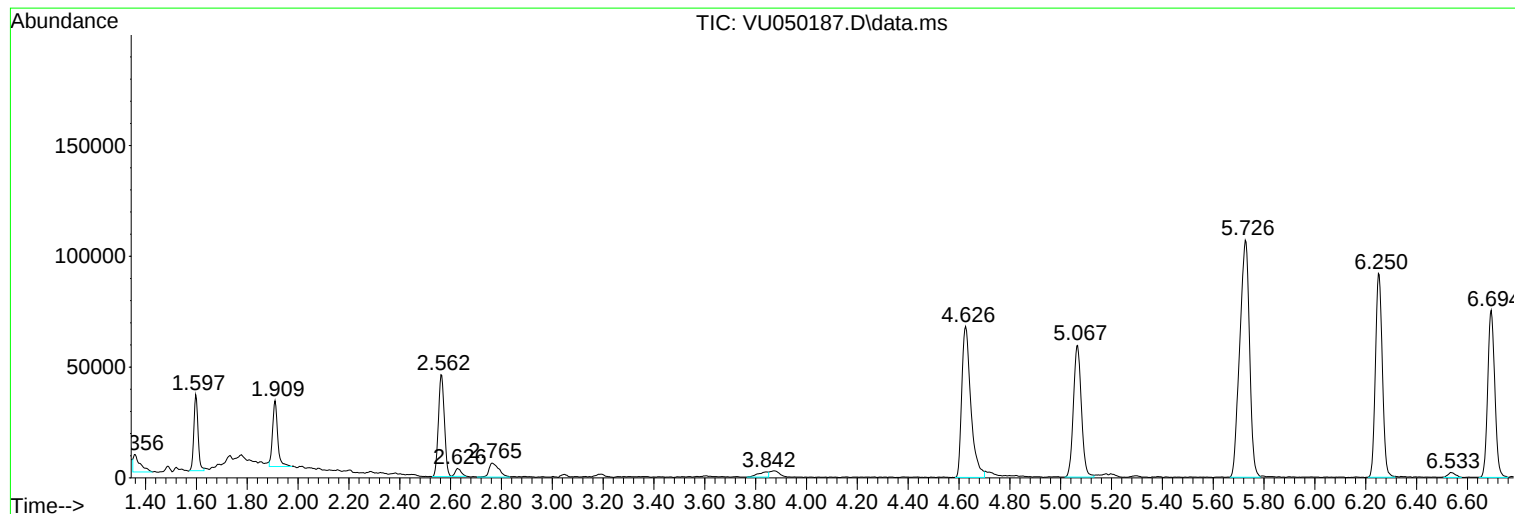

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050187.D
Acq On : 09 Aug 2022 16:35
Operator : SY/MD
Sample : N4075-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUV5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
Data File : VU050187.D
Acq On : 09 Aug 2022 16:35
Operator : SY/MD
Sample : N4075-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUV5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc