
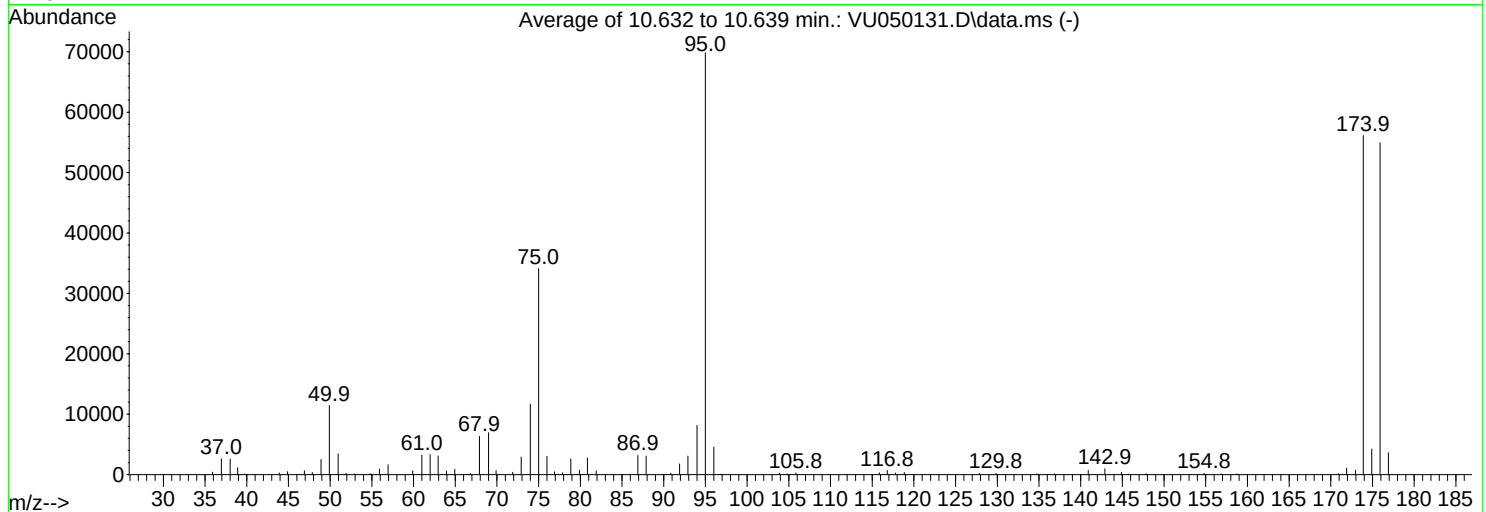


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080822\
 Data File : VU050131.D
 Acq On : 08 Aug 2022 09:36
 Operator : SY/MD
 Sample : BFB102
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB102

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Aug 09 00:39:33 2022

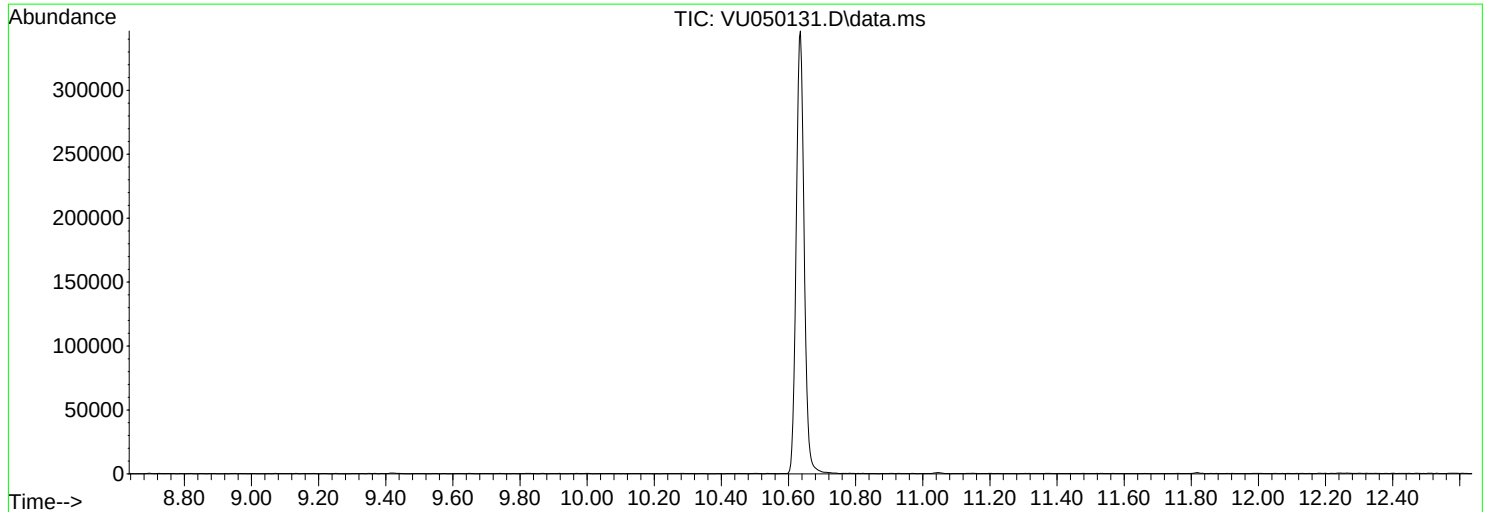

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	11454	PASS
75	95	30	80	48.9	34117	PASS
95	95	100	100	100.0	69819	PASS
96	95	5	9	6.5	4554	PASS
173	174	0.00	2	1.3	714	PASS
174	95	50	120	80.4	56131	PASS
175	174	5	9	7.5	4230	PASS
176	174	95	101	97.8	54923	PASS
177	176	5	9	6.6	3642	PASS

m/z	Abundance
43.90	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

m/z	Abundance
35.90	461.0
36.90	2743.0
38.00	2564.0
38.90	1159.0
39.80	111.0
43.90	528.0
44.90	481.0
46.90	625.0
47.90	334.0
48.90	2723.0
49.90	11766.0
50.90	3680.0
51.90	181.0
52.90	159.0
54.80	197.0
55.90	973.0
57.00	1744.0
59.90	704.0
61.00	3290.0
62.00	3419.0
63.00	3059.0
63.90	602.0
64.90	830.0
65.90	120.0
66.80	178.0
67.90	6475.0
69.00	7243.0
69.90	666.0
71.90	444.0
72.90	2971.0
74.00	11901.0
75.00	35016.0
76.00	3124.0
76.90	559.0
77.90	338.0
78.90	2722.0
79.90	712.0
80.90	2906.0
81.90	579.0
85.90	105.0
86.90	3259.0
87.90	3049.0
90.90	276.0
91.90	1910.0
92.90	3045.0
94.00	8202.0
95.00	70848.0
96.00	4802.0
96.90	155.0
103.90	255.0
104.80	126.0
105.80	301.0
115.80	333.0
116.80	691.0
117.80	297.0
118.80	355.0
127.90	201.0
129.80	254.0
134.80	140.0
136.80	142.0
140.90	700.0
142.90	1012.0
144.90	429.0
147.90	144.0
154.80	223.0
156.90	140.0
158.70	141.0
170.90	184.0
171.90	1094.0
172.90	747.0
173.90	56184.0
174.90	4392.0
175.90	55008.0
176.90	3800.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

m/z	Abundance
35.90	427.0
36.90	2710.0
38.00	2716.0
38.90	1163.0
39.70	108.0
43.90	543.0
44.90	509.0
46.90	664.0
47.80	385.0
48.90	2592.0
49.90	11791.0
51.00	3505.0
51.90	209.0
52.90	162.0
54.80	179.0
55.90	956.0
56.90	1690.0
59.90	657.0
61.00	3360.0
62.00	3452.0
62.90	3230.0
64.00	588.0
64.90	871.0
66.80	186.0
67.90	6521.0
69.00	7125.0
69.90	679.0
71.90	413.0
72.90	2994.0
74.00	12066.0
75.00	35232.0
76.00	3164.0
76.90	496.0
77.80	306.0
78.80	2672.0
79.90	743.0
80.80	2824.0
81.90	611.0
86.00	119.0
86.90	3314.0
87.90	3202.0
90.90	259.0
91.90	1805.0
92.90	3161.0
94.00	8435.0
95.00	71848.0
96.00	4696.0
96.90	116.0
103.90	269.0
104.80	142.0
105.90	317.0
106.70	101.0
115.80	339.0
116.80	717.0
117.80	292.0
118.80	371.0
127.80	193.0
129.90	226.0
130.80	102.0
134.80	132.0
136.80	124.0
140.90	698.0
142.90	987.0
144.90	430.0
145.70	117.0
147.80	159.0
154.80	248.0
156.90	131.0
158.80	148.0
170.90	187.0
171.90	1105.0
173.00	726.0
173.90	57800.0
174.90	4385.0
175.90	56680.0
176.90	3797.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

m/z	Abundance
35.90	423.0
37.00	2403.0
38.00	2447.0
38.90	1079.0
39.80	108.0
43.90	527.0
44.90	503.0
46.90	638.0
47.80	410.0
48.90	2258.0
49.90	10806.0
51.00	3147.0
51.90	214.0
52.90	113.0
54.80	136.0
55.90	838.0
56.90	1468.0
59.90	541.0
61.00	3025.0
62.00	3059.0
62.90	3004.0
64.00	556.0
65.00	904.0
66.80	169.0
67.90	6032.0
69.00	6472.0
69.90	632.0
71.90	355.0
72.90	2794.0
74.00	11066.0
75.00	32104.0
76.00	2843.0
76.90	419.0
77.80	282.0
78.80	2367.0
79.90	695.0
80.80	2525.0
81.90	633.0
86.00	126.0
86.90	3012.0
87.90	3001.0
90.80	213.0
91.90	1627.0
92.90	2975.0
94.00	7860.0
95.00	66760.0
96.00	4163.0
103.90	262.0
104.80	118.0
105.90	300.0
115.90	319.0
116.80	633.0
117.80	242.0
118.90	377.0
127.80	198.0
129.90	202.0
134.70	117.0
136.90	118.0
140.90	644.0
142.90	921.0
144.90	372.0
145.70	120.0
147.80	166.0
154.80	224.0
156.80	108.0
158.80	126.0
170.90	174.0
171.90	1089.0
173.00	669.0
173.90	54408.0
174.90	3912.0
175.90	53080.0
176.90	3328.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102