




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
Data File : VU060359.D
Acq On : 08 Aug 2024 16:29
Operator : MD/SY
Sample : P3401-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GG3

Manual IntegrationsAPPROVED

Quant Time: Aug 09 00:03:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Aug 08 23:46:27 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/12/2024
Supervised By :Semsettin Yesilyurt 08/12/2024

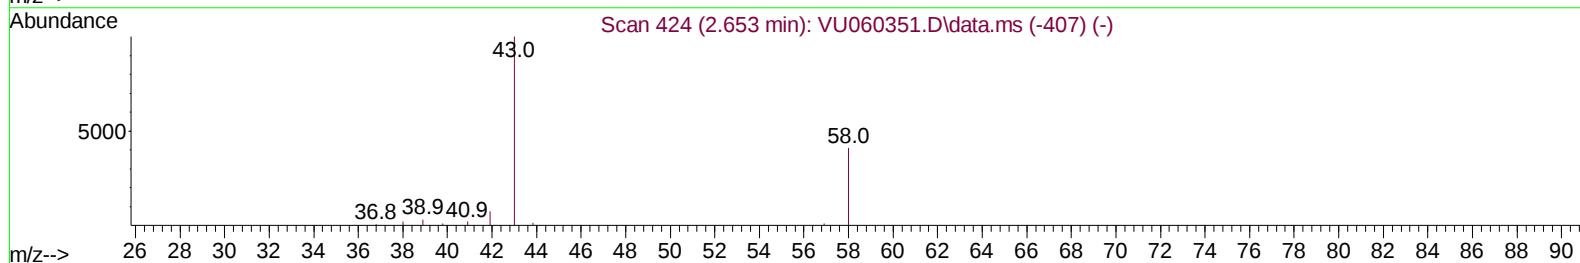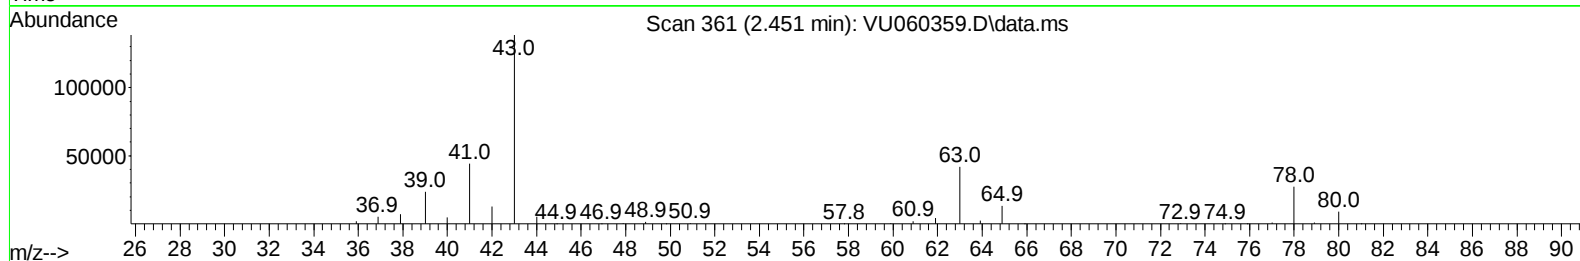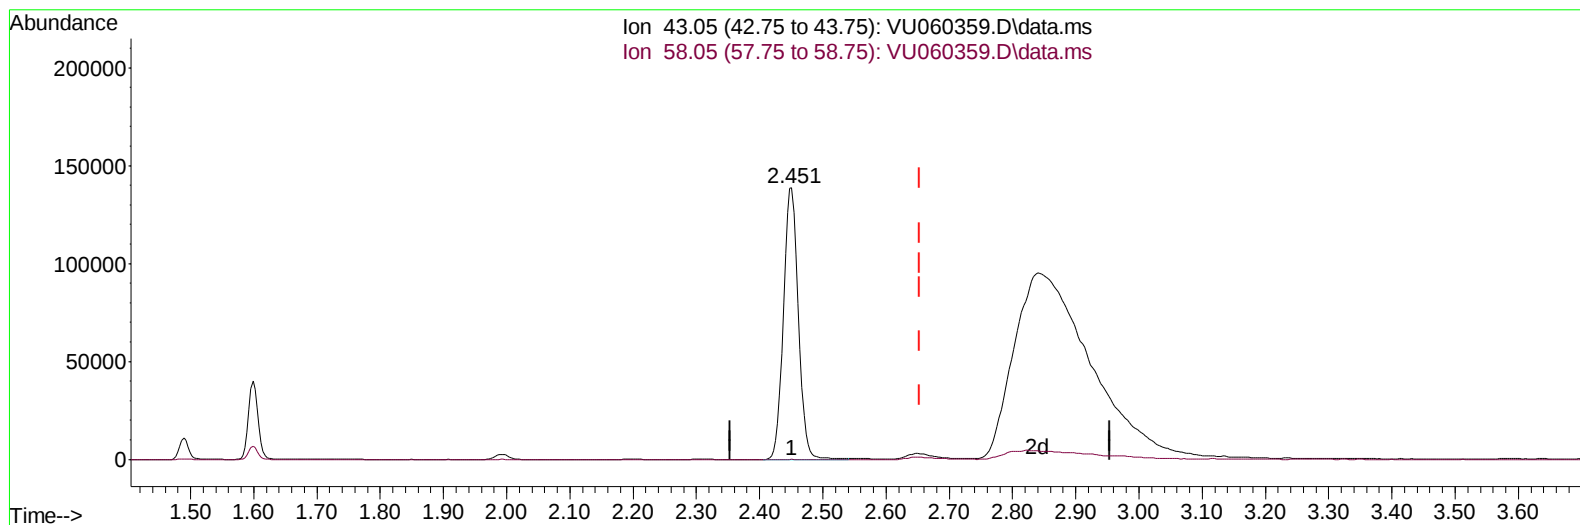

TIC: VU060359.D\data.ms

(13) Acetone (T)

2.451min (-0.203) 173.94 ug/L

response 227272

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	39.40	1.61
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
Data File : VU060359.D
Acq On : 08 Aug 2024 16:29
Operator : MD/SY
Sample : P3401-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GG3

Manual IntegrationsAPPROVED

Quant Time: Aug 09 00:03:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Aug 08 23:46:27 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/12/2024
Supervised By :Semsettin Yesilyurt 08/12/2024

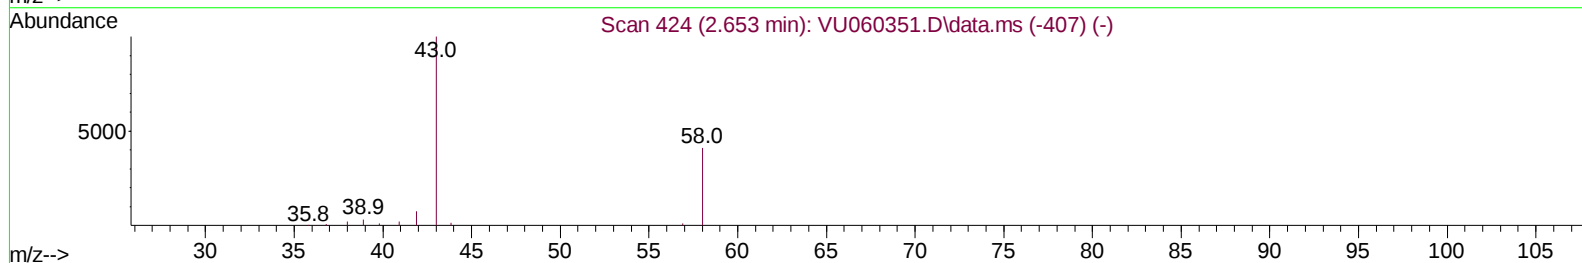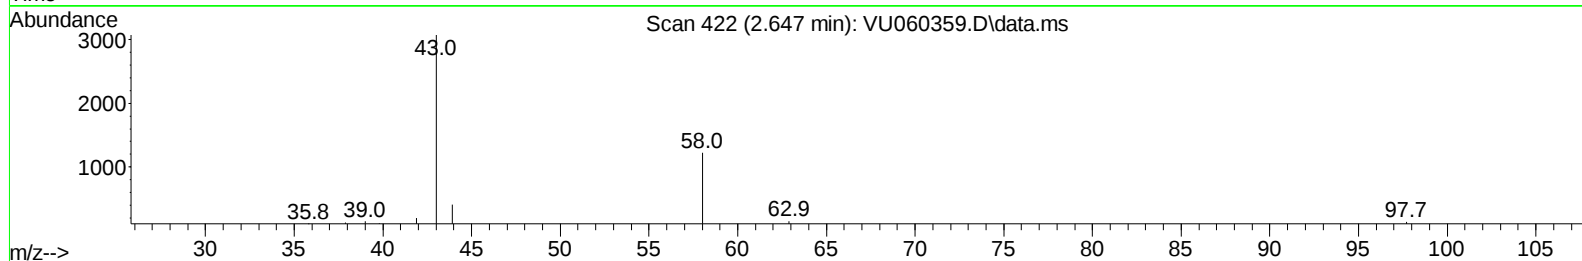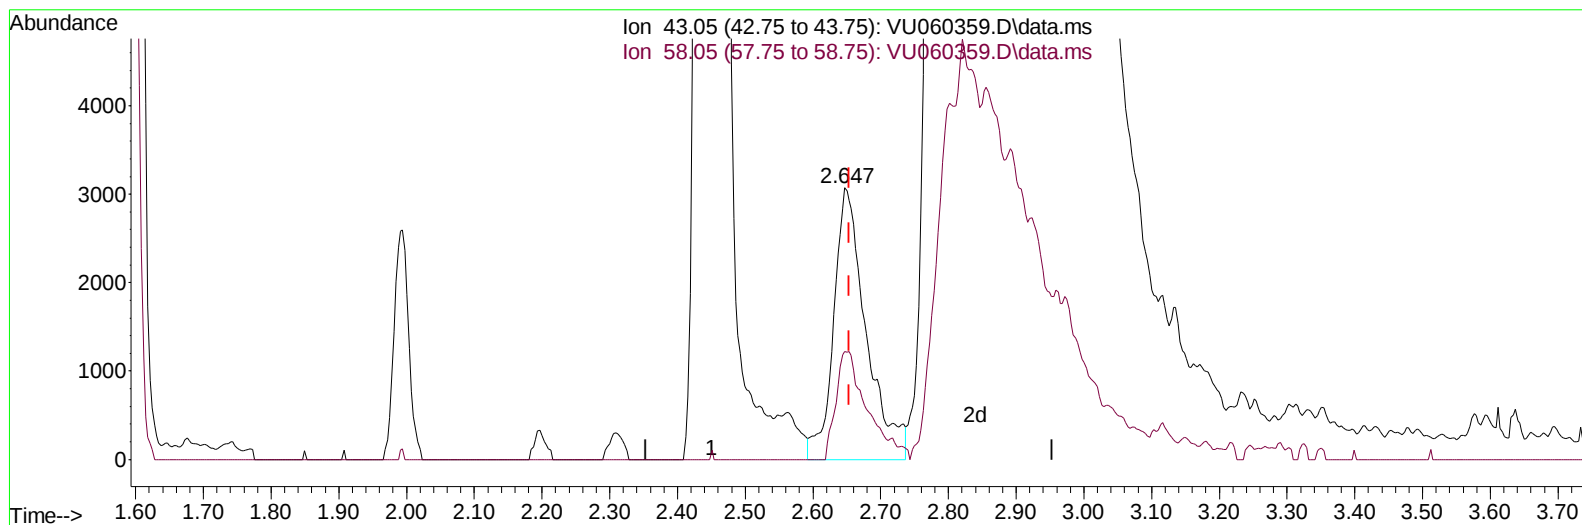

TIC: VU060359.D\data.ms

(13) Acetone (T)

2.647min (-0.006) 7.84 ug/L m

response 10242

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	39.40	35.80
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
 Data File : VU060359.D
 Acq On : 08 Aug 2024 16:29
 Operator : MD/SY
 Sample : P3401-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GG3

Manual IntegrationsAPPROVED

Quant Time: Aug 09 00:03:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Aug 08 23:46:27 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/12/2024
 Supervised By :Semsettin Yesilyurt 08/12/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		114859	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		120410	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		52271	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		43622	4.838	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	96.800%	
7) Chloroethane-d5	1.911	69		39090	4.808	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	96.200%	
11) 1,1-Dichloroethene-d2	2.563	65		17721	4.618	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	92.400%	
20) 2-Butanone-d5	4.628	46		98755	51.613	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	103.220%	
24) Chloroform-d	5.055	84		85200	4.773	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	95.400%	
26) 1,2-Dichloroethane-d4	5.695	65		40403	4.880	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	97.600%	
32) Benzene-d6	5.721	84		174305	4.800	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	96.000%	
36) 1,2-Dichloropropane-d6	6.682	67		56811	5.044	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	100.800%	
41) Toluene-d8	7.891	98		145481	4.487	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	89.800%	
43) trans-1,3-Dichloroprop...	8.174	79		17383	4.774	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	95.400%	
46) 2-Hexanone-d5	8.627	63		75830	46.924	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	93.840%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		43010	4.654	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	93.000%	
66) 1,2-Dichlorobenzene-d4	12.187	152		53222	5.527	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	110.600%	
Target Compounds							
						Qvalue	
5) Vinyl chloride	1.602	62		97925	10.852	ug/L	98
12) 1,1-Dichloroethene	2.573	96		8375	1.106	ug/L #	1
13) Acetone	2.647	43		10242m	7.839	ug/L	
16) Methylene chloride	3.039	84		1671	0.155	ug/L	94
18) trans-1,2-Dichloroethene	3.348	96		22463	3.024	ug/L	97
22) cis-1,2-Dichloroethene	4.656	96		1626586	181.358	ug/L	97
27) 1,2-Dichloroethane	5.791	62		4651	0.524	ug/L	100
33) Benzene	5.769	78		13500	0.389	ug/L	100
34) Trichloroethene	6.534	95		577502	63.639	ug/L	98
42) Toluene	7.968	91		7247	0.198	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
Data File : VU060359.D
Acq On : 08 Aug 2024 16:29
Operator : MD/SY
Sample : P3401-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 3

Instrument :
MSVOA_U
ClientSampleId :
E1GG3

Manual IntegrationsAPPROVED

Quant Time: Aug 09 00:03:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Aug 08 23:46:27 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/12/2024
Supervised By :Semsettin Yesilyurt 08/12/2024

