

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
 Data File : VU060361.D
 Acq On : 08 Aug 2024 17:17
 Operator : MD/SY
 Sample : P3401-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GF4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060361.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.451	342	361	380	rBV	545033	887163	12.47%	7.819%
2	2.563	384	396	413	rVV	96154	161971	2.28%	1.428%
3	2.872	449	492	606	rBV	654887	7114938	100.00%	62.711%
4	4.631	1029	1039	1086	rBV2	47159	175398	2.47%	1.546%
5	5.055	1155	1171	1197	rBV2	85603	196816	2.77%	1.735%
6	5.721	1357	1378	1410	rBV2	174295	451624	6.35%	3.981%
7	6.245	1527	1541	1572	rBV	123530	243942	3.43%	2.150%
8	6.685	1664	1678	1699	rBV	106386	211329	2.97%	1.863%
9	7.563	1940	1951	1970	rBV2	42396	77719	1.09%	0.685%
10	7.891	2036	2053	2069	rBV	201438	363521	5.11%	3.204%
11	8.631	2272	2283	2324	rBV	196573	395660	5.56%	3.487%
12	9.412	2514	2526	2564	rBV	187999	324445	4.56%	2.860%
13	10.749	2928	2942	2963	rBV	81050	134407	1.89%	1.185%
14	11.807	3258	3271	3288	rBV	173436	289818	4.07%	2.554%
15	12.187	3377	3389	3410	rBV	191245	316776	4.45%	2.792%




Sum of corrected areas: 11345527

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
Data File : VU060361.D
Acq On : 08 Aug 2024 17:17
Operator : MD/SY
Sample : P3401-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

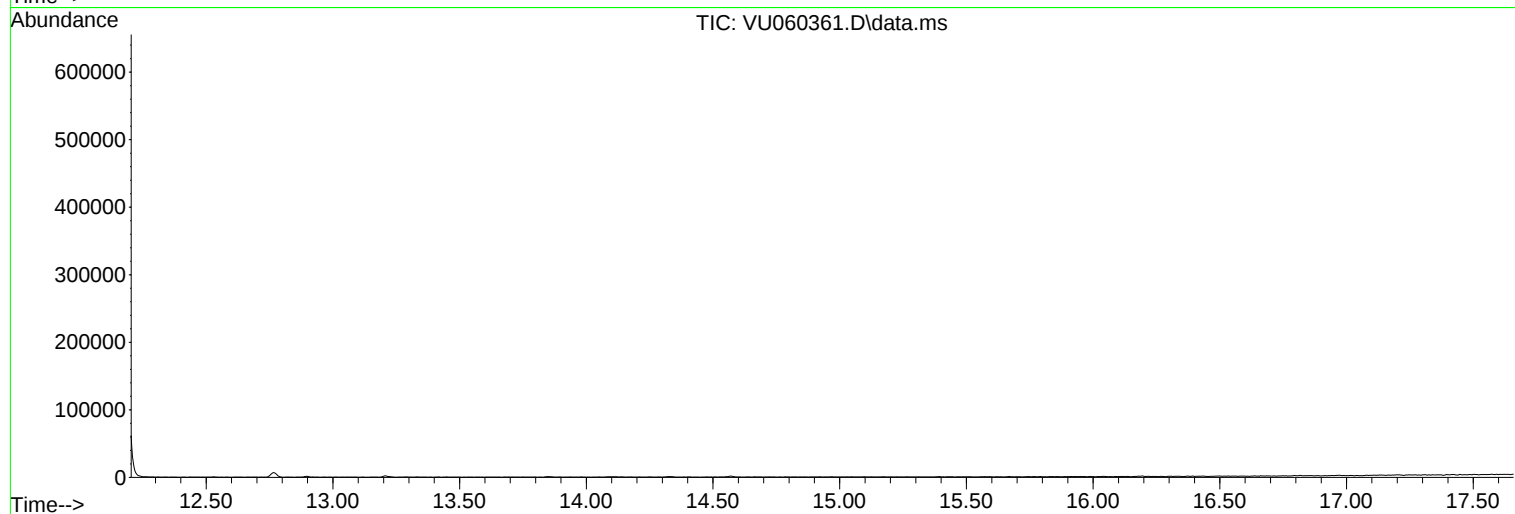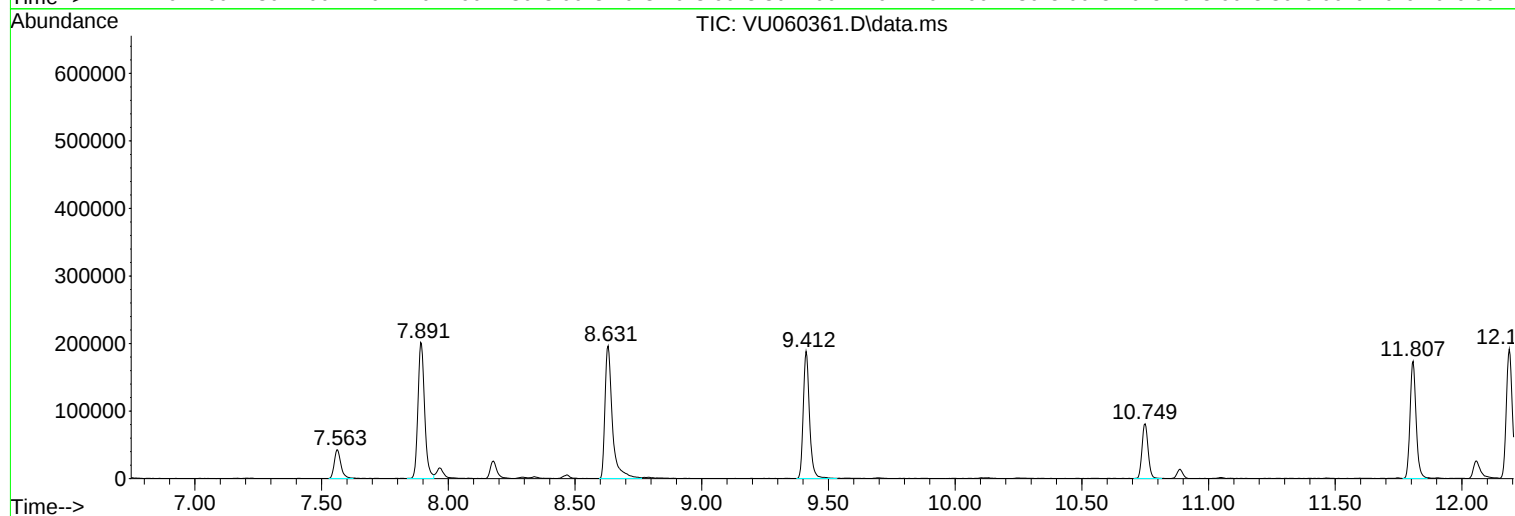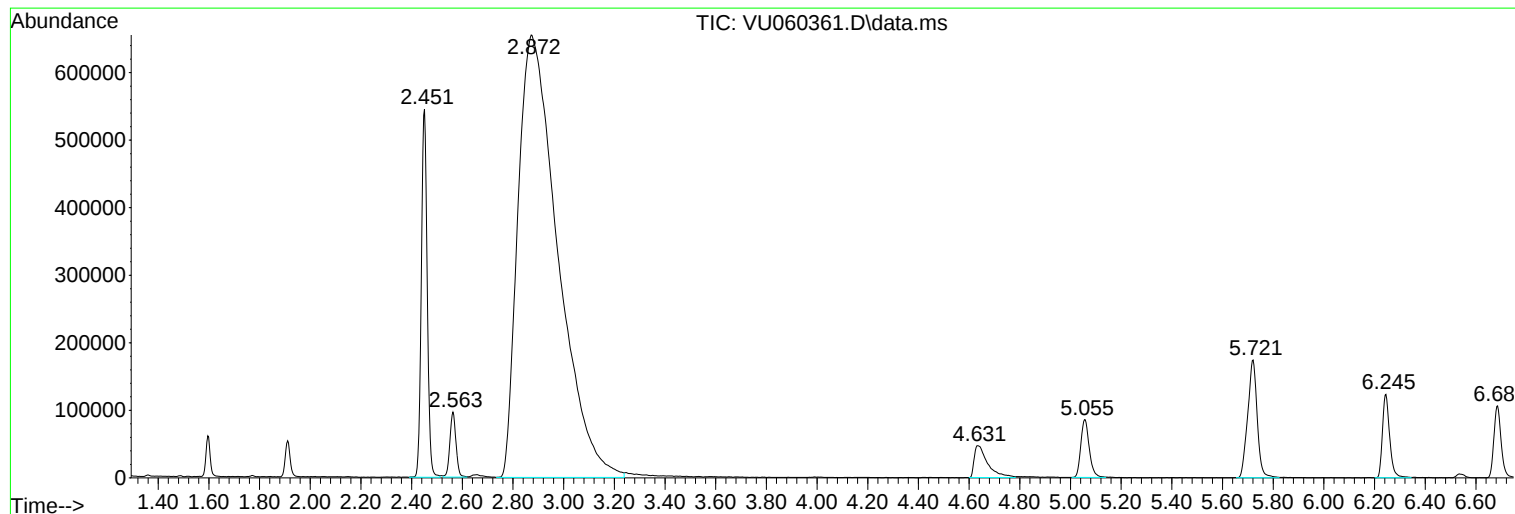

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
Data File : VU060361.D
Acq On : 08 Aug 2024 17:17
Operator : MD/SY
Sample : P3401-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF4







Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.451	18.18 ug/L	887163	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	78
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	42
4	Acetyl chloride			78	C2H3ClO	000075-36-5	9
5	2-Chloroethanol			80	C2H5ClO	000107-07-3	4

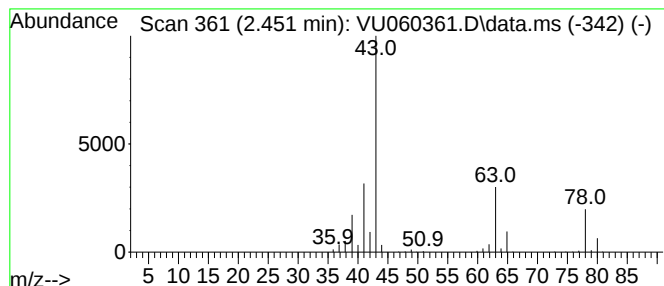

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
Data File : VU060361.D
Acq On : 08 Aug 2024 17:17
Operator : MD/SY
Sample : P3401-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.872	145.83 ug/L	7114940	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	56
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

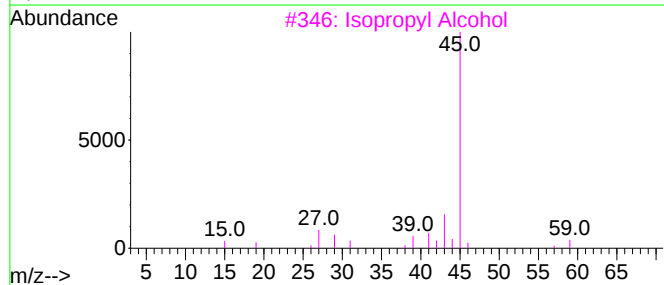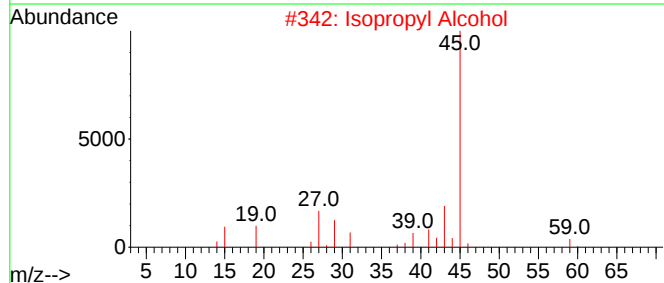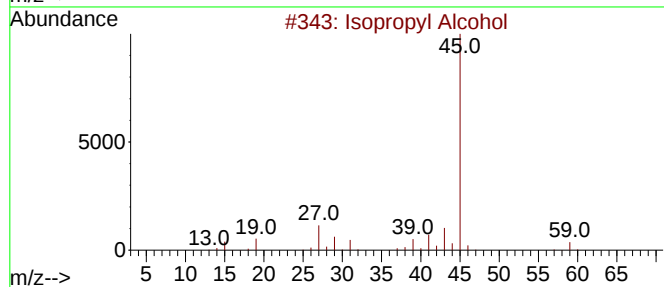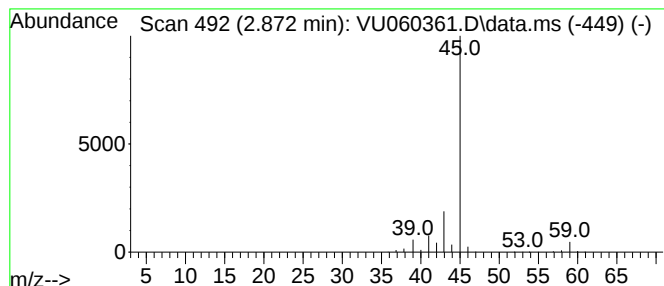

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
Data File : VU060361.D
Acq On : 08 Aug 2024 17:17
Operator : MD/SY
Sample : P3401-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.451	18.2	ug/L	887163	1	6.245	243942	5.0
Isopropyl Alcohol	2.872	145.8	ug/L	7114940	1	6.245	243942	5.0