

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
 Data File : VU060363.D
 Acq On : 08 Aug 2024 18:05
 Operator : MD/SY
 Sample : P3401-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GF7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU060363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.451	348	361	384	rBV	562435	915586	13.50%	8.331%
2	2.563	384	396	410	rVB	92594	151424	2.23%	1.378%
3	2.878	452	494	601	rBV	626864	6781451	100.00%	61.702%
4	4.634	1027	1040	1076	rBV2	46642	162583	2.40%	1.479%
5	5.055	1157	1171	1199	rBV2	85194	194435	2.87%	1.769%
6	5.717	1358	1377	1406	rBV3	167379	441790	6.51%	4.020%
7	6.242	1528	1540	1565	rBV	122919	243213	3.59%	2.213%
8	6.682	1665	1677	1707	rBV	103316	206930	3.05%	1.883%
9	7.563	1939	1951	1970	rBV2	40880	76070	1.12%	0.692%
10	7.891	2036	2053	2069	rBV	196942	356461	5.26%	3.243%
11	8.630	2272	2283	2321	rBV	194368	391988	5.78%	3.567%
12	9.412	2513	2526	2548	rBV	186767	325574	4.80%	2.962%
13	10.749	2931	2942	2963	rVB	82090	132227	1.95%	1.203%
14	11.807	3259	3271	3294	rBV	174813	295477	4.36%	2.688%
15	12.187	3378	3389	3413	rVB	189018	315389	4.65%	2.870%




Sum of corrected areas: 10990598

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
Data File : VU060363.D
Acq On : 08 Aug 2024 18:05
Operator : MD/SY
Sample : P3401-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

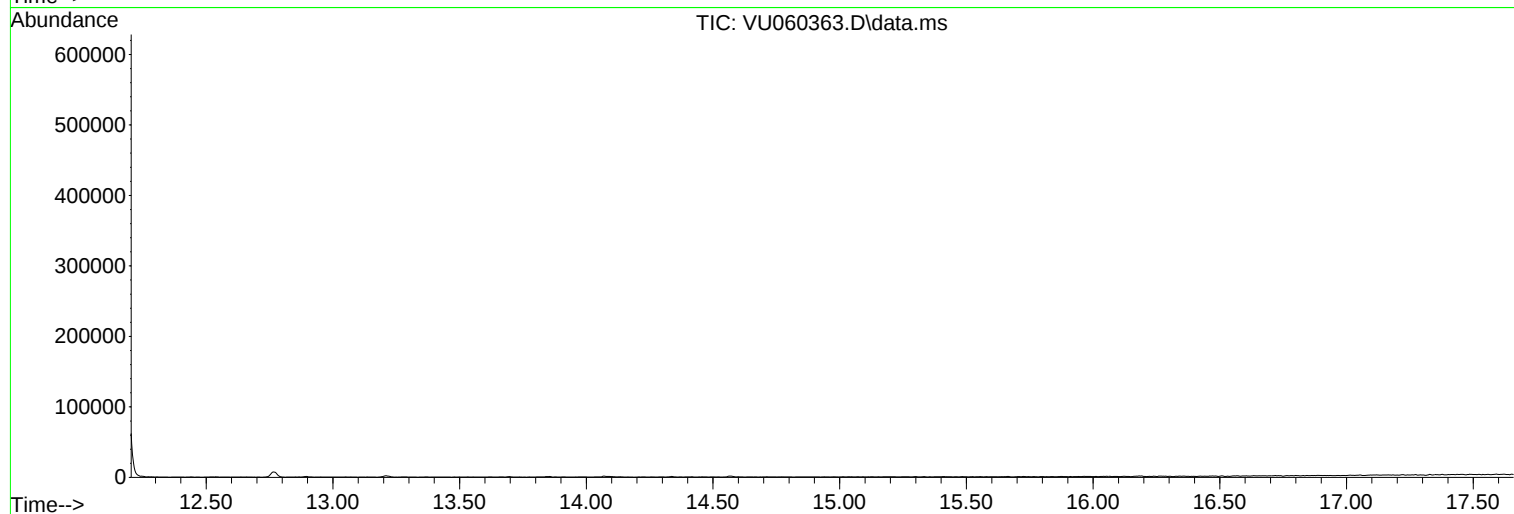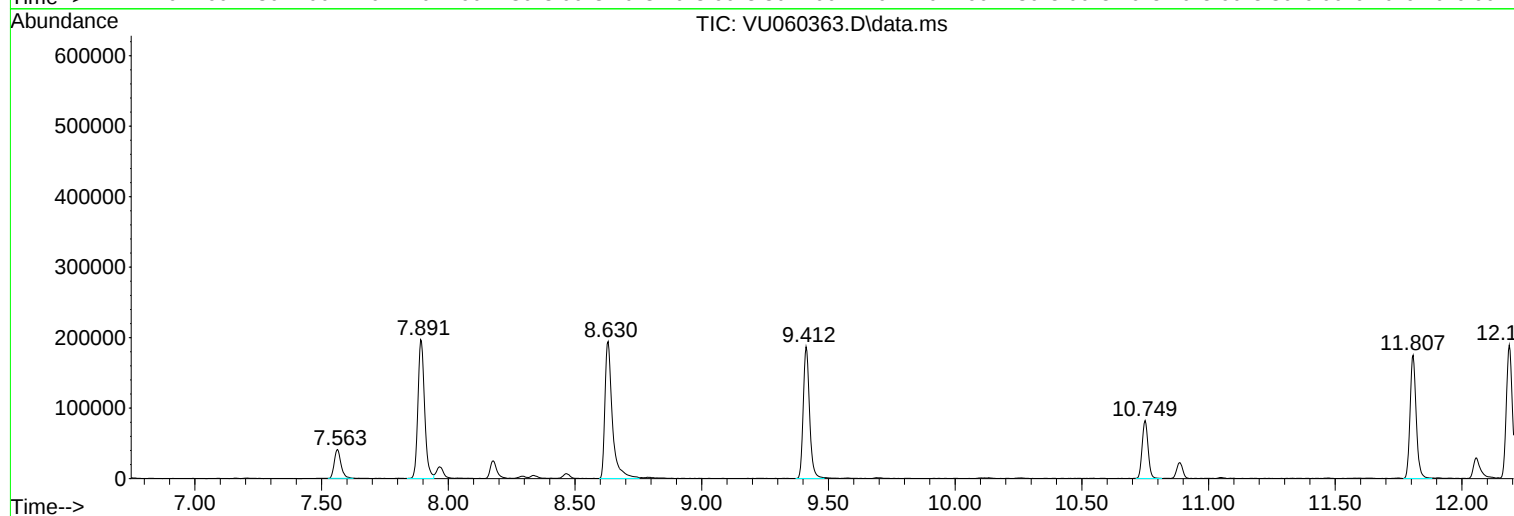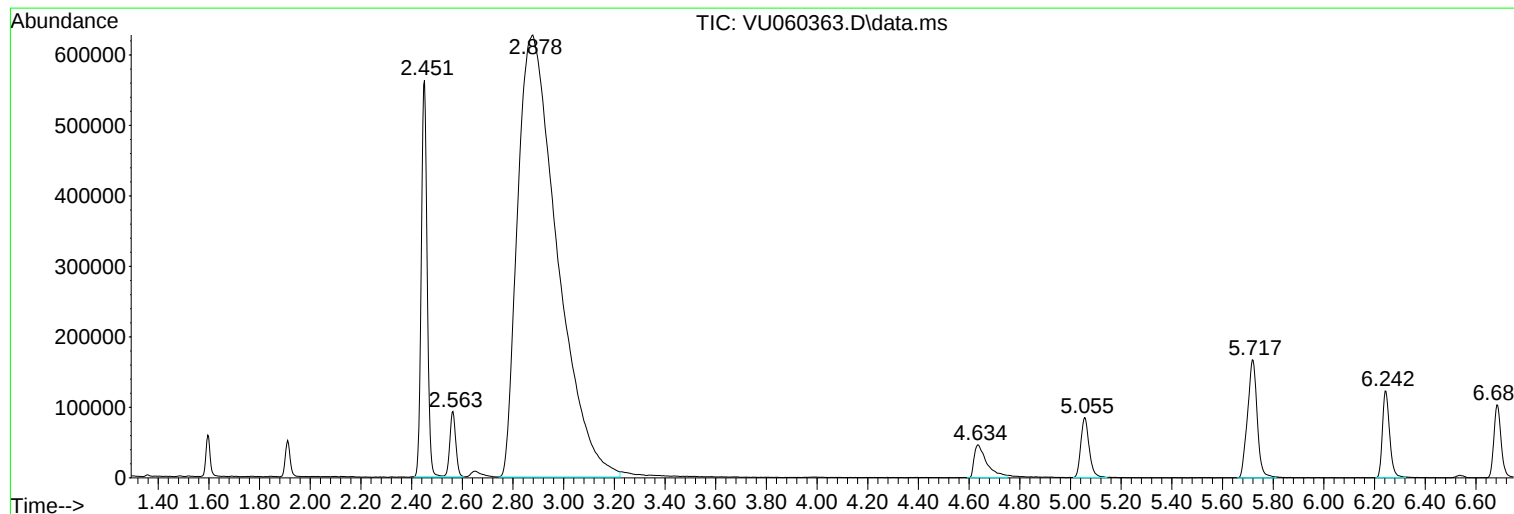

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
Data File : VU060363.D
Acq On : 08 Aug 2024 18:05
Operator : MD/SY
Sample : P3401-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF7







Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.451	18.82 ug/L	915586	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	78
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	33
4	Acetyl chloride			78	C2H3ClO	000075-36-5	9
5	2-Chloroethanol			80	C2H5ClO	000107-07-3	4

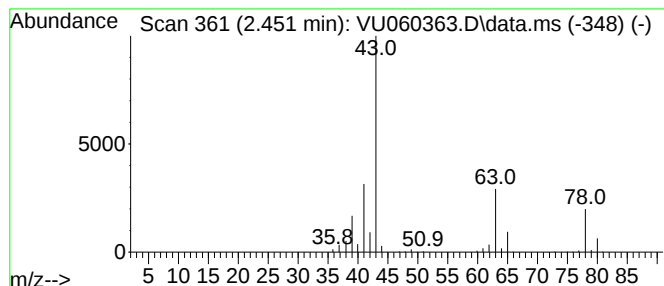

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
Data File : VU060363.D
Acq On : 08 Aug 2024 18:05
Operator : MD/SY
Sample : P3401-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.878	139.41 ug/L	6781450	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	56
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

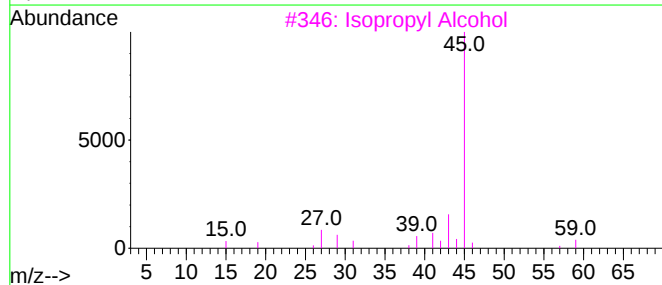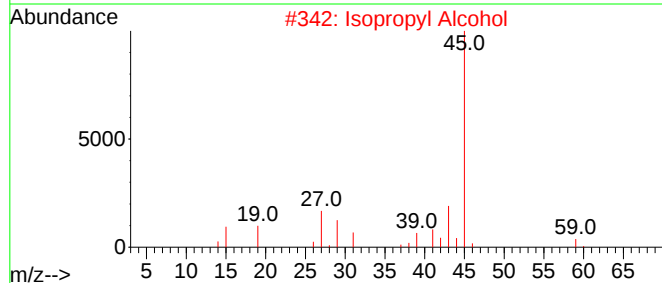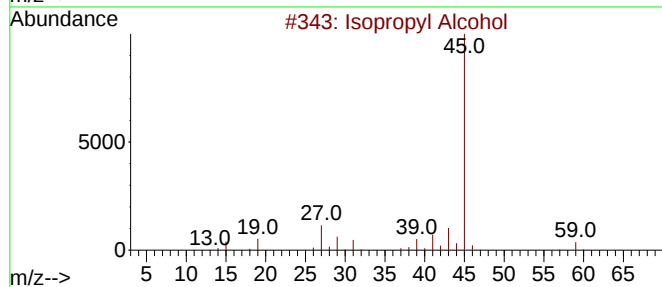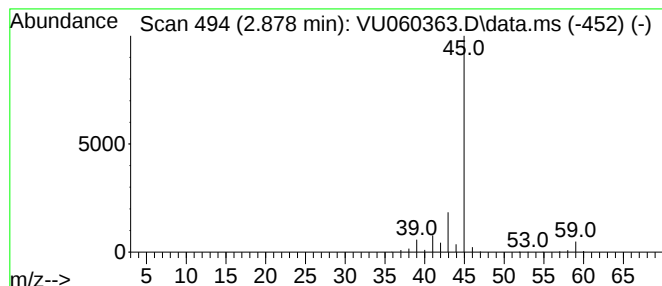

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
Data File : VU060363.D
Acq On : 08 Aug 2024 18:05
Operator : MD/SY
Sample : P3401-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.451	18.8	ug/L	915586	1	6.245	243213	5.0
Isopropyl Alcohol	2.878	139.4	ug/L	6781450	1	6.245	243213	5.0