


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080824\
Data File : VU060348.D
Acq On : 08 Aug 2024 10:16
Operator : MD/SY
Sample : BFB181
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB181

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Aug 10 05:58:50 2024

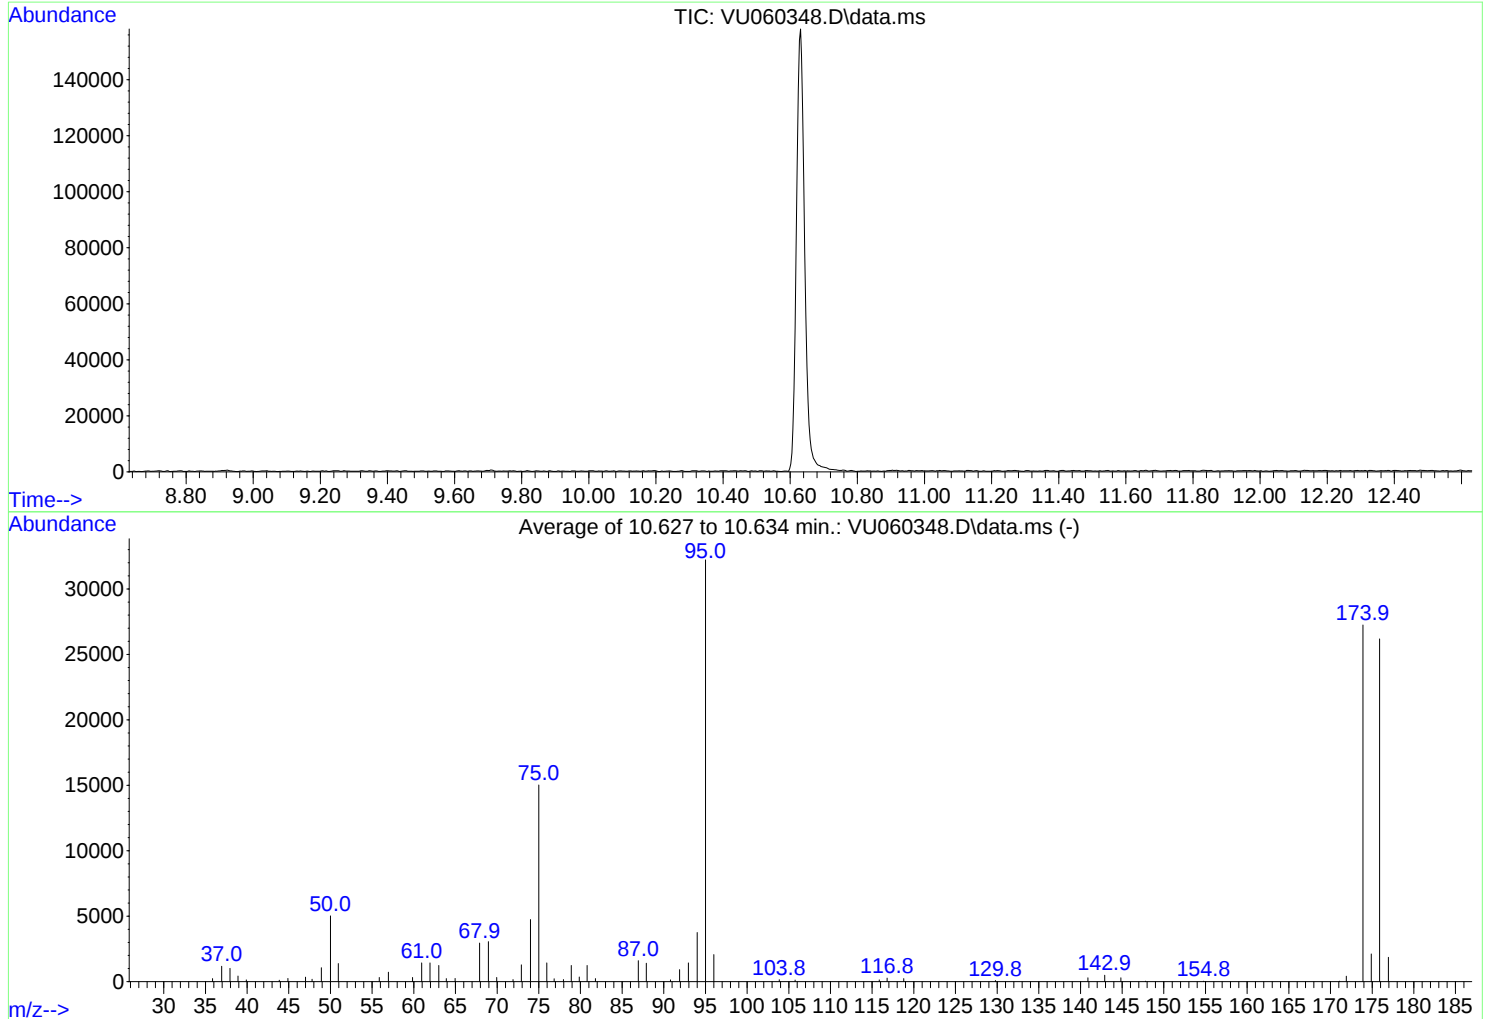

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.6	5024	PASS
75	95	30	80	46.6	15025	PASS
95	95	100	100	100.0	32224	PASS
96	95	5	9	6.4	2067	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.5	27245	PASS
175	174	5	9	7.8	2114	PASS
176	174	95	101	96.1	26181	PASS
177	176	5	9	7.1	1858	PASS

m/z	Abundance
43.90	282.0

Instrument :
MSVOA_U
ClientSampleId :
BFB181

m/z	Abundance
35.90	294.0
37.00	1146.0
38.00	997.0
38.90	438.0
39.90	143.0
43.90	366.0
44.90	248.0
47.00	401.0
47.70	206.0
48.90	1020.0
50.00	5111.0
50.90	1555.0
55.90	356.0
56.90	682.0
59.80	256.0
60.90	1460.0
61.90	1425.0
63.00	1261.0
63.90	245.0
65.00	219.0
67.90	3007.0
69.00	3258.0
69.90	331.0
71.90	183.0
72.90	1300.0
74.00	4803.0
75.00	15252.0
76.00	1369.0
76.90	226.0
78.00	159.0
78.90	1190.0
79.80	376.0
80.80	1210.0
81.80	228.0
87.00	1632.0
87.90	1362.0
90.80	130.0
91.90	933.0
92.90	1399.0
94.00	3691.0
95.00	32448.0
96.00	2119.0
103.80	156.0
105.70	133.0
115.90	118.0
116.80	252.0
118.80	210.0
129.80	140.0
140.90	266.0
142.90	459.0
144.80	284.0
154.80	110.0
171.10	120.0
171.90	374.0
173.90	27144.0
174.90	2139.0
175.90	25840.0
176.90	1839.0

Instrument :
MSVOA_U
ClientSampleId :
BFB181

m/z	Abundance
35.90	236.0
37.00	1194.0
38.00	1046.0
38.90	450.0
39.90	137.0
43.90	394.0
44.90	259.0
47.00	342.0
47.80	198.0
48.90	1109.0
50.00	5188.0
51.00	1381.0
55.80	313.0
56.90	749.0
59.90	329.0
61.00	1474.0
61.90	1489.0
63.00	1283.0
63.90	229.0
64.90	249.0
67.90	3058.0
68.90	3120.0
70.00	350.0
71.90	160.0
72.90	1293.0
74.00	4891.0
75.00	15525.0
75.90	1514.0
76.80	253.0
77.90	173.0
78.90	1287.0
79.90	351.0
80.80	1269.0
81.80	234.0
87.00	1657.0
87.90	1449.0
90.80	138.0
91.90	952.0
93.00	1434.0
94.00	3852.0
95.00	33112.0
96.00	2100.0
103.90	138.0
105.80	131.0
115.90	142.0
116.80	281.0
118.80	238.0
129.80	113.0
140.90	300.0
142.90	516.0
144.90	303.0
171.90	416.0
173.90	28112.0
174.90	2230.0
175.90	27016.0
176.90	1896.0

Instrument :
MSVOA_U
ClientSampleId :
BFB181

m/z	Abundance
35.90	187.0
36.90	1168.0
37.90	1001.0
38.90	393.0
39.90	120.0
43.80	409.0
44.90	235.0
47.00	289.0
47.90	163.0
48.90	1074.0
50.00	4772.0
51.00	1224.0
55.80	272.0
57.00	734.0
59.90	388.0
61.00	1345.0
62.00	1391.0
63.00	1167.0
63.90	227.0
64.90	279.0
67.90	2781.0
68.90	2802.0
70.00	270.0
71.90	123.0
72.90	1256.0
74.00	4531.0
75.00	14298.0
75.90	1405.0
76.80	200.0
77.90	138.0
78.90	1247.0
79.90	329.0
80.80	1237.0
81.80	241.0
86.90	1526.0
87.90	1389.0
90.80	121.0
91.90	883.0
93.00	1470.0
94.00	3700.0
95.00	31112.0
96.00	1981.0
103.90	131.0
105.80	110.0
115.80	150.0
116.80	277.0
118.80	257.0
140.90	297.0
142.90	508.0
144.90	294.0
147.80	104.0
171.90	458.0
173.90	26480.0
174.90	1974.0
175.90	25688.0
177.00	1840.0

Instrument :
MSVOA_U
ClientSampleId :
BFB181