

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080918\
 Data File : VU026028.D
 Acq On : 10 Aug 2018 04:32
 Operator : MD/SY
 Sample : J4401-14 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 10 07:44:12 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 10 07:39:13 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	291192	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	276161	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	122973	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	73141	34.36	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	68.72%
7) Chloroethane-d5	1.65	69	68107	40.36	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.72%
11) 1,1-Dichloroethene-d2	2.27	63	112352	27.78	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	55.56%#
21) 2-Butanone-d5	4.18	46	150333	84.74	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	84.74%
24) Chloroform-d	4.65	84	185415	41.08	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.16%
26) 1,2-Dichloroethane-d4	5.31	65	128761	42.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.46%
32) Benzene-d6	5.34	84	352285	41.08	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.16%
36) 1,2-Dichloropropane-d6	6.33	67	117723	42.43	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.86%
41) Toluene-d8	7.57	98	319558	38.95	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	77.90%#
43) trans-1,3-Dichloropropene-	7.85	79	54792	39.19	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.38%
47) 2-Hexanone-d5	8.31	63	111694	88.63	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.63%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	176799	43.57	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.14%
64) 1,2-Dichlorobenzene-d4	11.86	152	133902	44.17	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.34%

Target Compounds


					Ovalue
37) 1,2-Dichloropropane	6.33	63	14475	6.726 ug/L #	88
59) 1,2,3-Trichloropropane	11.49	75	15751	5.675 ug/L	95
67) 1,3,5-Trichlorobenzene	13.51	180	4643	1.623 ug/L #	93
68) 1,2,4-trichlorobenzene	13.51	180	4643	1.919 ug/L #	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080918\
Data File : VU026028.D
Acq On : 10 Aug 2018 04:32
Operator : MD/SY
Sample : J4401-14 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Aug 10 07:44:12 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 10 07:39:13 2018
Response via : Initial Calibration




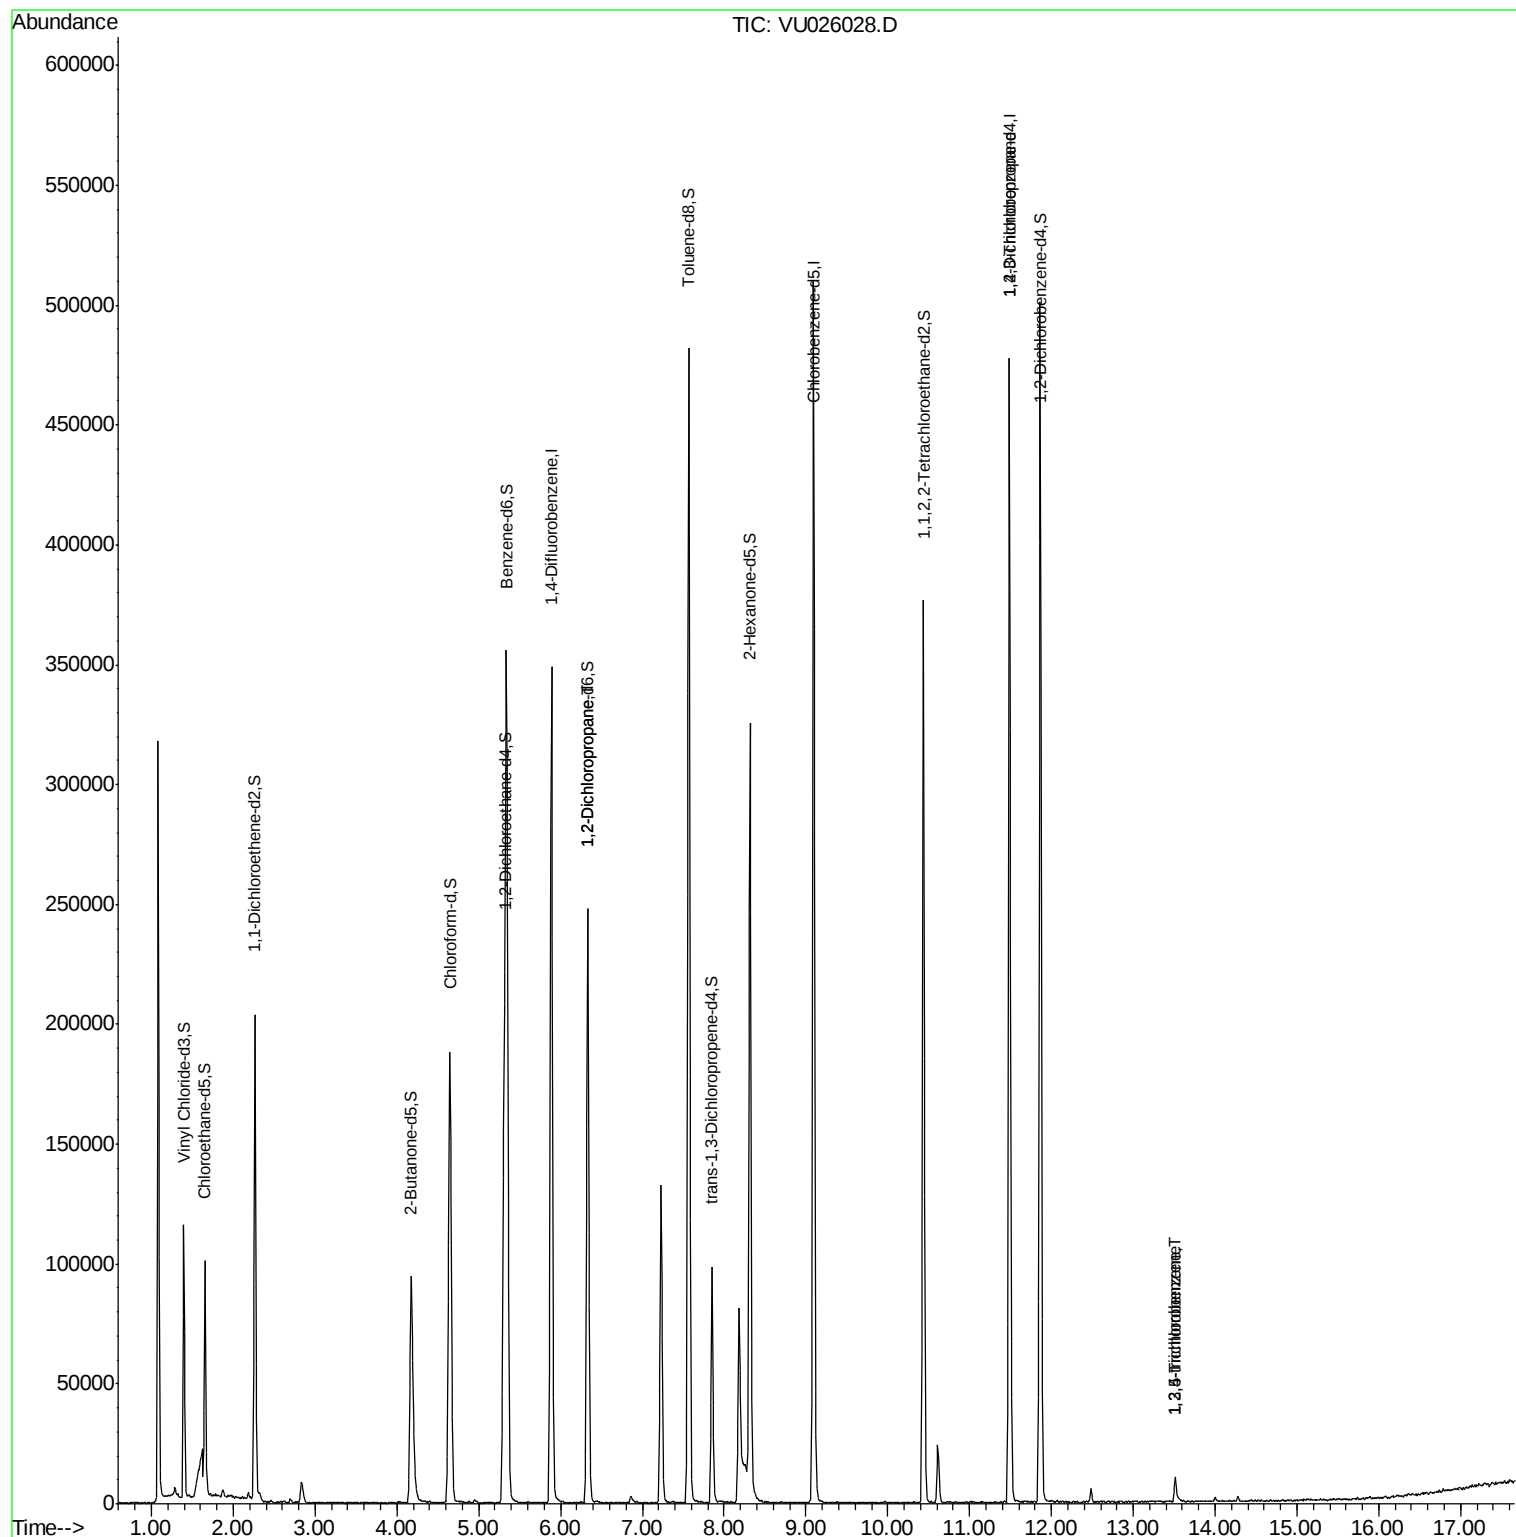


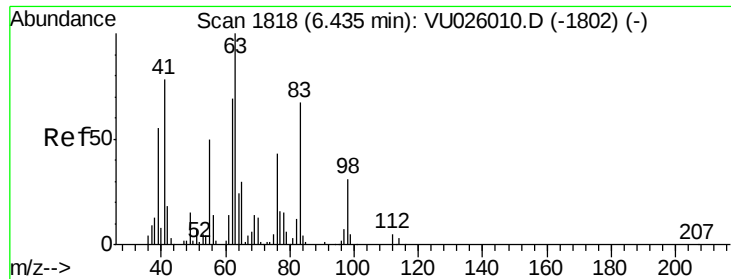

#37
 1,2-Dichloropropane
 Concen: 6.726 ug/L
 RT: 6.33 min Scan# 1786
 Delta R.T. -0.10 min
 Lab File: VU026028.D
 Acq: 10 Aug 2018 04:32




Instrument :
 MSVOA_U
 ClientSampleId :


Tot Ion: 63 Resp: 14475
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.2 4.8#

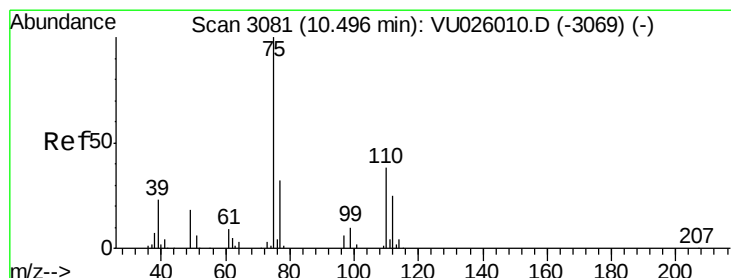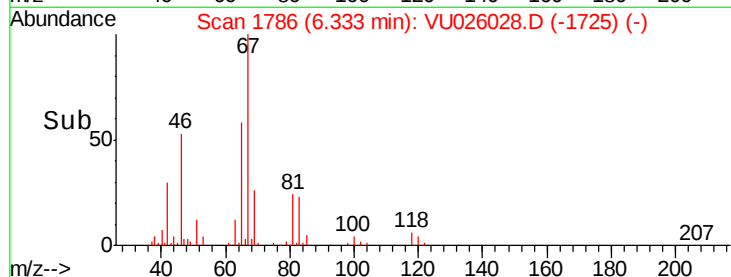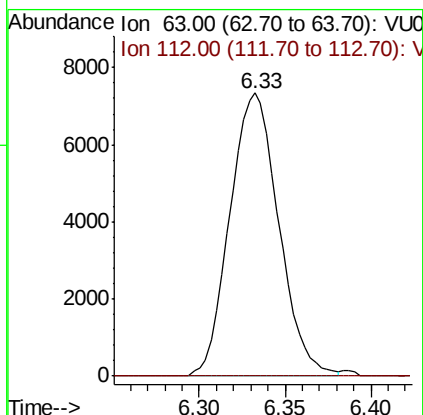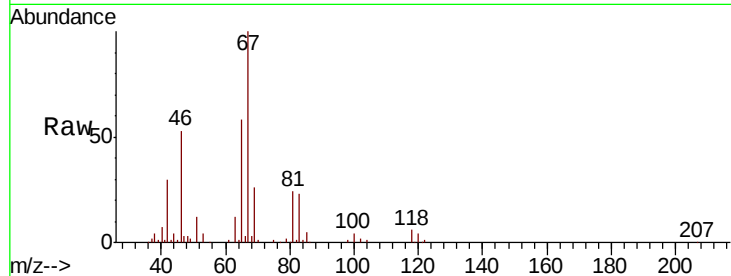

#59
 1,2,3-Trichloropropane
 Concen: 5.675 ug/L
 RT: 11.49 min Scan# 3389
 Delta R.T. 0.99 min
 Lab File: VU026028.D
 Acq: 10 Aug 2018 04:32

Tgt Ion: 75 Resp: 15751
 Ion Ratio Lower Upper
 75 100
 77 34.4 25.3 37.9


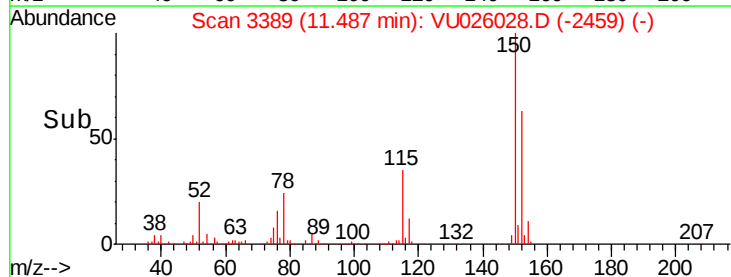
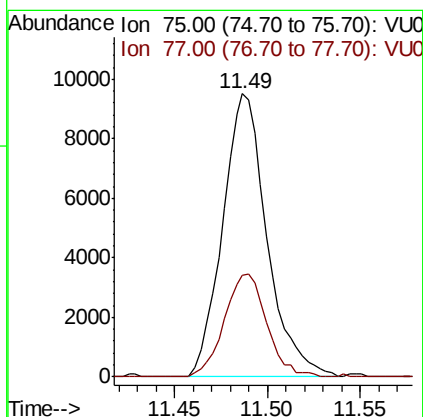
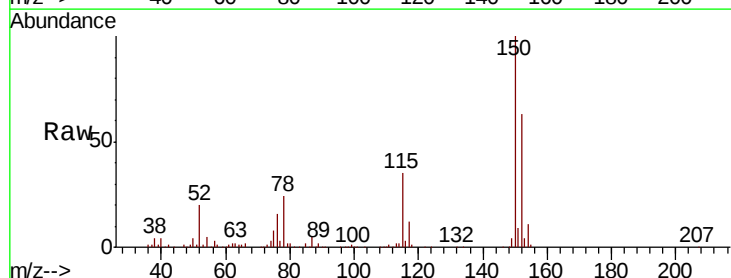


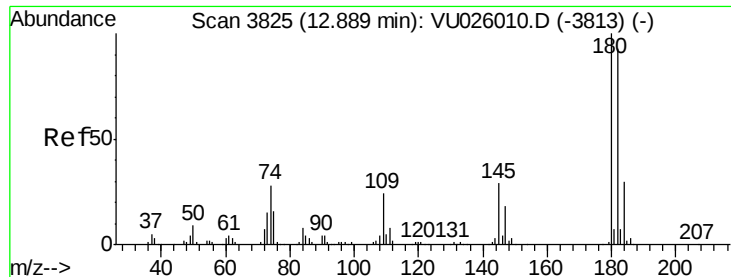

#67
 1,3,5-Trichlorobenzene
 Concen: 1.623 ug/L
 RT: 13.51 min Scan# 4018
 Delta R.T. 0.62 min
 Lab File: VU026028.D
 Acq: 10 Aug 2018 04:32

Instrument :
 MSVOA_U
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
180	100		
182	94.0	76.5	114.7
184	28.3	24.3	36.5
145	14.8	23.5	35.3

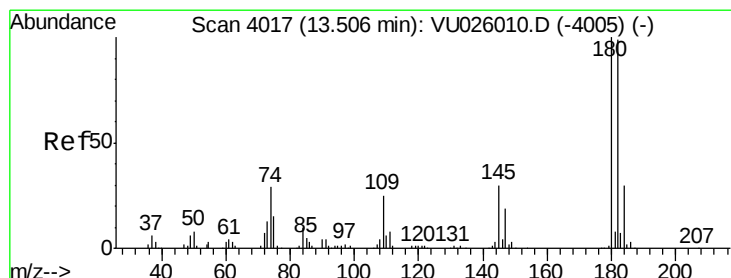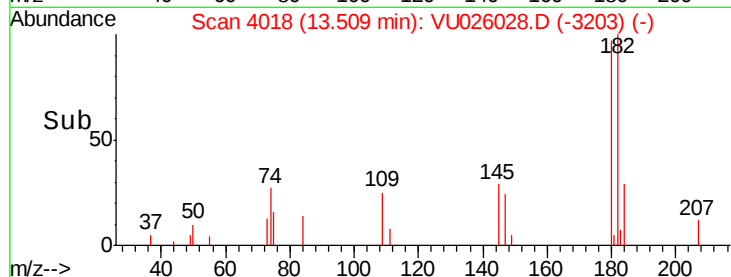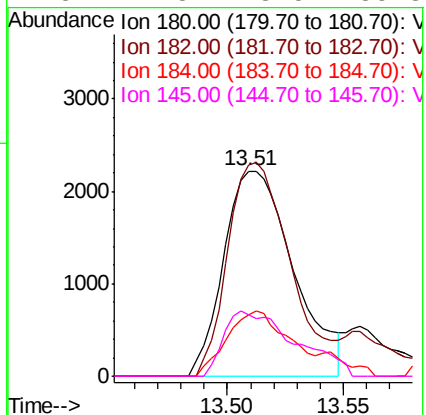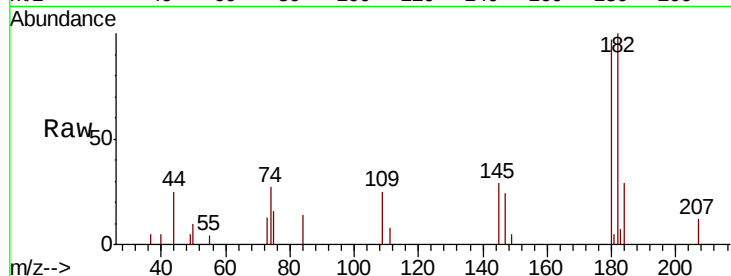

#68
 1,2,4-trichlorobenzene
 Concen: 1.919 ug/L
 RT: 13.51 min Scan# 4018
 Delta R.T. 0.00 min
 Lab File: VU026028.D
 Acq: 10 Aug 2018 04:32

Tgt Ion	Ratio	Lower	Upper
180	100		
182	94.0	76.5	114.7
145	14.8	24.2	36.4

