

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080918\
 Data File : VU025998.D
 Acq On : 09 Aug 2018 15:59
 Operator : MD/SY
 Sample : J4361-24DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZA7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.677	24	27	31	rBV2	349	361	0.03%	0.003%
2	0.812	66	69	72	rBV	339	261	0.02%	0.002%
3	0.995	122	126	132	rVB2	287	274	0.02%	0.002%
4	1.085	135	154	176	rBV	498695	584783	44.58%	5.287%
5	1.401	244	252	262	rBV	143772	149944	11.43%	1.356%
6	1.677	330	338	352	rBV	109232	144182	10.99%	1.304%
7	2.272	512	523	535	rBV	251552	380810	29.03%	3.443%
8	2.449	576	578	581	rVB3	611	328	0.03%	0.003%
9	2.703	649	657	665	rVB4	1834	2956	0.23%	0.027%
10	2.757	672	674	679	rVB2	382	306	0.02%	0.003%
11	2.835	688	698	711	rVV3	2598	5711	0.44%	0.052%
12	2.992	744	747	752	rVV2	482	352	0.03%	0.003%
13	3.359	858	861	864	rBV2	401	260	0.02%	0.002%
14	3.384	865	869	871	rBV3	308	250	0.02%	0.002%
15	3.921	1031	1036	1039	rVB3	276	322	0.02%	0.003%
16	3.979	1049	1054	1059	rVB	558	549	0.04%	0.005%
17	4.002	1059	1061	1065	rBV	411	294	0.02%	0.003%
18	4.056	1075	1078	1083	rBV3	382	392	0.03%	0.004%
19	4.179	1095	1116	1139	rBV	111838	301814	23.01%	2.729%
20	4.391	1179	1182	1184	rVV	500	339	0.03%	0.003%
21	4.651	1244	1263	1288	rVV	211765	498941	38.04%	4.511%
22	4.741	1288	1291	1295	rBV4	725	529	0.04%	0.005%
23	4.873	1328	1332	1334	rVV2	523	447	0.03%	0.004%
24	4.892	1335	1338	1349	rVB5	1132	1437	0.11%	0.013%
25	4.960	1355	1359	1361	rBV3	430	275	0.02%	0.002%
26	4.995	1368	1370	1373	rVB3	494	254	0.02%	0.002%
27	5.024	1373	1379	1382	rBV3	338	417	0.03%	0.004%
28	5.085	1392	1398	1403	rBV3	569	677	0.05%	0.006%
29	5.172	1422	1425	1428	rBV2	411	291	0.02%	0.003%
30	5.342	1453	1478	1508	rBV2	406496	1229061	93.69%	11.113%
31	5.670	1576	1580	1585	rVB2	563	506	0.04%	0.005%
32	5.754	1599	1606	1610	rBV3	376	481	0.04%	0.004%
33	5.786	1612	1616	1619	rBV2	346	303	0.02%	0.003%
34	5.802	1619	1621	1627	rVB	310	254	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080918\
 Data File : VU025998.D
 Acq On : 09 Aug 2018 15:59
 Operator : MD/SY
 Sample : J4361-24DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZA7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Title : VOC Analysis

35	5.831	1627	1630	1633	rBV2	268	248	0.02%	0.002%
36	5.889	1633	1648	1672	rBV	350942	685826	52.28%	6.201%
37	5.998	1679	1682	1687	rVB3	561	545	0.04%	0.005%
38	6.169	1732	1735	1737	rBV3	343	266	0.02%	0.002%
39	6.217	1747	1750	1756	rBV	392	339	0.03%	0.003%
40	6.333	1772	1786	1805	rBV	276756	555774	42.37%	5.025%
41	6.506	1837	1840	1843	rVB2	513	360	0.03%	0.003%
42	6.529	1843	1847	1849	rBV2	388	308	0.02%	0.003%
43	6.690	1893	1897	1899	rBV2	448	313	0.02%	0.003%
44	6.738	1908	1912	1917	rVV2	397	352	0.03%	0.003%
45	6.857	1943	1949	1956	rBV6	1388	2038	0.16%	0.018%
46	6.960	1978	1981	1985	rVB2	368	328	0.03%	0.003%
47	7.018	1992	1999	2005	rBV2	475	639	0.05%	0.006%
48	7.047	2005	2008	2010	rBV	420	264	0.02%	0.002%
49	7.159	2039	2043	2046	rBV2	576	598	0.05%	0.005%
50	7.230	2053	2065	2088	rBV	162578	289404	22.06%	2.617%
51	7.371	2105	2109	2110	rBV3	396	320	0.02%	0.003%
52	7.461	2135	2137	2140	rBV2	461	301	0.02%	0.003%
53	7.567	2157	2170	2188	rBV	556276	965006	73.56%	8.725%
54	7.744	2222	2225	2232	rVB3	360	330	0.03%	0.003%
55	7.850	2247	2258	2280	rBV	116038	198097	15.10%	1.791%
56	8.011	2305	2308	2313	rBV3	528	513	0.04%	0.005%
57	8.185	2348	2362	2380	rBV2	58622	138967	10.59%	1.256%
58	8.313	2391	2402	2432	rVB	351572	594194	45.30%	5.373%
59	8.503	2459	2461	2466	rVB2	635	462	0.04%	0.004%
60	8.526	2466	2468	2470	rBV2	544	273	0.02%	0.002%
61	8.603	2489	2492	2497	rVB2	482	323	0.02%	0.003%
62	8.902	2580	2585	2590	rBB3	538	610	0.05%	0.006%
63	8.934	2590	2595	2598	rBV3	393	399	0.03%	0.004%
64	8.989	2608	2612	2614	rBV2	334	284	0.02%	0.003%
65	9.091	2627	2644	2650	rBV	502104	871278	66.42%	7.878%
66	9.281	2701	2703	2709	rBV2	260	294	0.02%	0.003%
67	9.371	2728	2731	2737	rVB4	368	441	0.03%	0.004%
68	9.609	2800	2805	2808	rBV3	304	270	0.02%	0.002%
69	9.696	2828	2832	2838	rVB	509	496	0.04%	0.004%
70	9.731	2838	2843	2845	rBV3	461	392	0.03%	0.004%
71	9.799	2858	2864	2867	rBV3	446	515	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080918\
 Data File : VU025998.D
 Acq On : 09 Aug 2018 15:59
 Operator : MD/SY
 Sample : J4361-24DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZA7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Title : VOC Analysis

72	9.934	2900	2906	2910	rBV2	294	372	0.03%	0.003%
73	9.969	2913	2917	2919	rBV	339	292	0.02%	0.003%
74	10.320	3022	3026	3027	rBV	823	458	0.03%	0.004%
75	10.435	3048	3062	3085	rBV	394450	633061	48.26%	5.724%
76	10.558	3093	3100	3104	rVB3	371	500	0.04%	0.005%
77	10.612	3104	3117	3133	rBV2	20444	35991	2.74%	0.325%
78	10.709	3142	3147	3149	rBV3	403	351	0.03%	0.003%
79	10.870	3194	3197	3199	rBV	408	249	0.02%	0.002%
80	10.985	3227	3233	3236	rBV3	468	362	0.03%	0.003%
81	11.011	3236	3241	3245	rBV3	456	592	0.05%	0.005%
82	11.085	3260	3264	3267	rBV3	591	463	0.04%	0.004%
83	11.153	3282	3285	3289	rBV3	477	392	0.03%	0.004%
84	11.317	3333	3336	3340	rBV	416	386	0.03%	0.003%
85	11.419	3359	3368	3377	rBV	25915	39053	2.98%	0.353%
86	11.487	3377	3389	3414	rVB2	484562	1097128	83.64%	9.920%
87	11.651	3438	3440	3444	rVB2	429	314	0.02%	0.003%
88	11.866	3491	3507	3532	rBV3	615584	1311784	100.00%	11.861%
89	11.976	3537	3541	3544	rBV3	546	410	0.03%	0.004%
90	12.050	3561	3564	3566	rBV2	526	390	0.03%	0.004%
91	12.484	3689	3699	3709	rBV	4467	7500	0.57%	0.068%
92	12.551	3716	3720	3725	rBV2	514	476	0.04%	0.004%
93	12.580	3725	3729	3730	rBV2	416	302	0.02%	0.003%
94	12.751	3779	3782	3789	rBV2	356	406	0.03%	0.004%
95	13.506	4005	4017	4044	rBV2	147888	252067	19.22%	2.279%
96	13.619	4050	4052	4060	rVB3	894	733	0.06%	0.007%
97	13.712	4079	4081	4084	rBV2	451	249	0.02%	0.002%
98	13.992	4159	4168	4181	rBV4	32708	55011	4.19%	0.497%
99	14.599	4355	4357	4360	rBV	486	371	0.03%	0.003%
100	15.014	4483	4486	4488	rBV	725	494	0.04%	0.004%


Sum of corrected areas: 11059885

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080918\
Data File : VU025998.D
Acq On : 09 Aug 2018 15:59
Operator : MD/SY
Sample : J4361-24DL 40X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
A4ZA7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

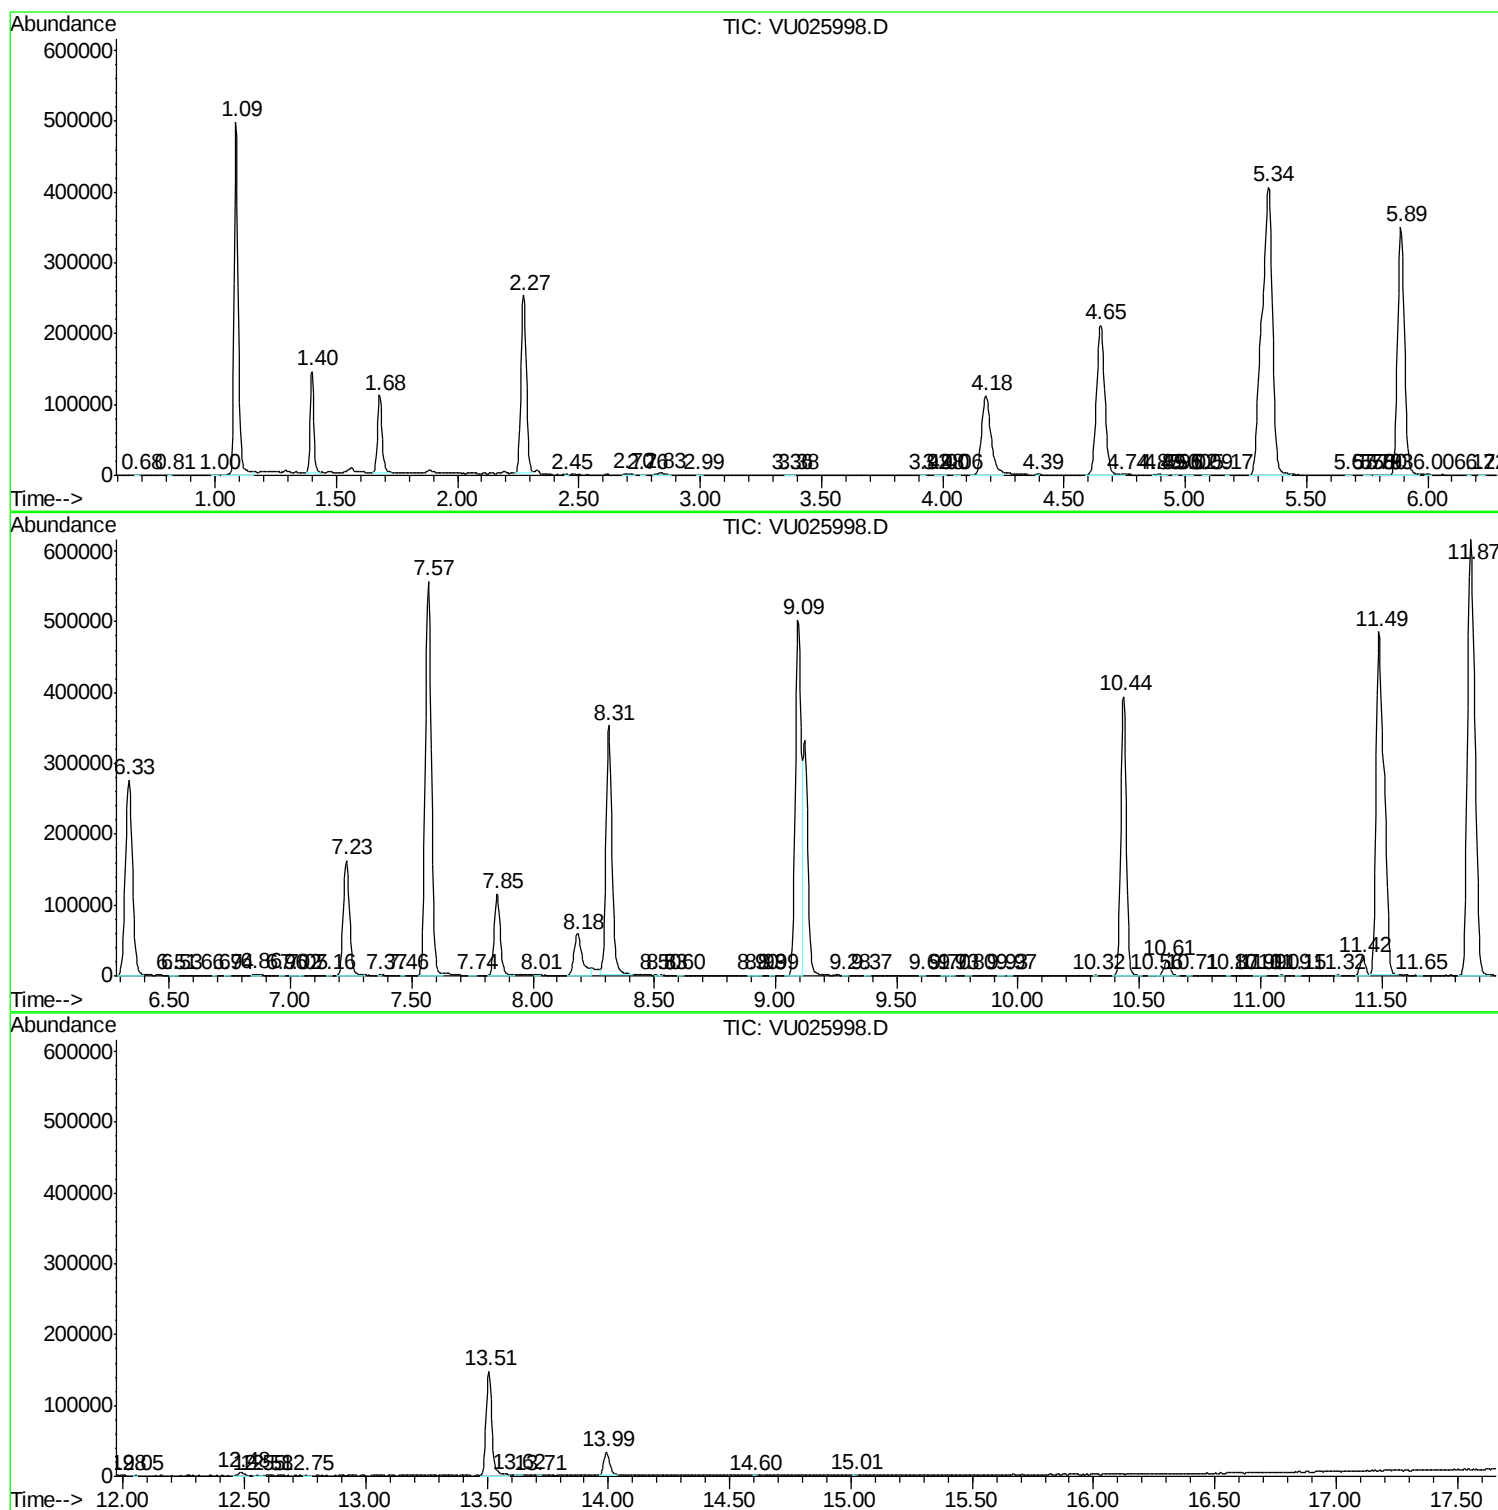

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080918\
Data File : VU025998.D
Acq On : 09 Aug 2018 15:59
Operator : MD/SY
Sample : J4361-24DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZA7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080918\
Data File : VU025998.D
Acq On : 09 Aug 2018 15:59
Operator : MD/SY
Sample : J4361-24DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZA7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc