

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080918\
 Data File : VU026021.D
 Acq On : 10 Aug 2018 01:42
 Operator : MD/SY
 Sample : J4401-05 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZE3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.619	6	9	13	rBV2	382	409	0.04%	0.005%
2	0.645	13	17	18	rBV2	257	182	0.02%	0.002%
3	0.873	86	88	91	rBV3	167	88	0.01%	0.001%
4	0.921	102	103	105	rVB3	101	36	0.00%	0.000%
5	0.944	105	110	113	rBV	402	425	0.04%	0.005%
6	1.085	136	154	173	rBV	337693	395474	36.31%	4.469%
7	1.400	245	252	266	rVB	121276	123731	11.36%	1.398%
8	1.677	330	338	353	rVB	95694	127646	11.72%	1.442%
9	2.272	513	523	537	rBV	205933	311436	28.59%	3.519%
10	2.577	614	618	620	rBV	317	262	0.02%	0.003%
11	2.664	643	645	646	rBV	416	158	0.01%	0.002%
12	2.921	723	725	729	rBV3	389	246	0.02%	0.003%
13	2.966	735	739	743	rBV4	365	361	0.03%	0.004%
14	3.043	760	763	765	rVB	270	138	0.01%	0.002%
15	3.140	790	793	796	rBV2	258	143	0.01%	0.002%
16	3.223	816	819	820	rBV2	203	117	0.01%	0.001%
17	3.243	820	825	828	rVV	208	236	0.02%	0.003%
18	3.339	853	855	858	rBV	345	257	0.02%	0.003%
19	3.381	864	868	873	rVB3	451	529	0.05%	0.006%
20	3.407	873	876	881	rBV	481	401	0.04%	0.005%
21	3.455	888	891	894	rBV	376	283	0.03%	0.003%
22	3.481	897	899	902	rBV	334	229	0.02%	0.003%
23	3.616	938	941	942	rBV	135	77	0.01%	0.001%
24	3.658	950	954	957	rBV2	322	267	0.02%	0.003%
25	3.805	998	1000	1002	rBV2	239	96	0.01%	0.001%
26	3.905	1029	1031	1033	rBV2	217	125	0.01%	0.001%
27	3.953	1041	1046	1047	rBV2	161	168	0.02%	0.002%
28	3.982	1052	1055	1056	rBV2	217	119	0.01%	0.001%
29	4.034	1067	1071	1074	rVB2	253	189	0.02%	0.002%
30	4.050	1074	1076	1080	rBV2	256	190	0.02%	0.002%
31	4.076	1080	1084	1088	rVB2	382	334	0.03%	0.004%
32	4.095	1088	1090	1092	rBV	217	128	0.01%	0.001%
33	4.175	1101	1115	1142	rBV	98490	266477	24.46%	3.011%
34	4.558	1230	1234	1236	rBV2	292	191	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080918\
 Data File : VU026021.D
 Acq On : 10 Aug 2018 01:42
 Operator : MD/SY
 Sample : J4401-05 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZE3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Title : VOC Analysis

35	4.651	1246	1263	1284	rBV	190517	448049	41.13%	5.063%
36	4.995	1368	1370	1375	rVB3	513	262	0.02%	0.003%
37	5.040	1383	1384	1385	rBV3	225	73	0.01%	0.001%
38	5.069	1391	1393	1399	rVB3	245	174	0.02%	0.002%
39	5.114	1404	1407	1408	rBV	147	77	0.01%	0.001%
40	5.182	1426	1428	1432	rVB2	185	144	0.01%	0.002%
41	5.204	1432	1435	1436	rBV	314	160	0.01%	0.002%
42	5.342	1453	1478	1507	rBV2	361085	1089298	100.00%	12.309%
43	5.664	1575	1578	1579	rBV	206	91	0.01%	0.001%
44	5.725	1594	1597	1599	rVB2	400	224	0.02%	0.003%
45	5.744	1599	1603	1604	rBV2	254	204	0.02%	0.002%
46	5.786	1614	1616	1620	rBV2	294	225	0.02%	0.003%
47	5.818	1623	1626	1627	rBV	259	113	0.01%	0.001%
48	5.889	1634	1648	1669	rBV	347210	679447	62.37%	7.678%
49	6.108	1713	1716	1719	rBV2	302	253	0.02%	0.003%
50	6.188	1739	1741	1743	rBV	201	115	0.01%	0.001%
51	6.243	1757	1758	1759	rBV	228	82	0.01%	0.001%
52	6.333	1772	1786	1807	rBV	251711	501348	46.02%	5.665%
53	6.825	1934	1939	1940	rBV	344	229	0.02%	0.003%
54	7.043	2005	2007	2009	rBV	192	98	0.01%	0.001%
55	7.059	2009	2012	2014	rBV	263	151	0.01%	0.002%
56	7.091	2019	2022	2024	rBV2	278	190	0.02%	0.002%
57	7.140	2035	2037	2040	rBV2	219	133	0.01%	0.002%
58	7.230	2052	2065	2082	rBV	136430	240641	22.09%	2.719%
59	7.490	2139	2146	2150	rBV2	370	577	0.05%	0.007%
60	7.567	2157	2170	2191	rBV	484267	839440	77.06%	9.486%
61	7.850	2245	2258	2277	rBV	95819	166723	15.31%	1.884%
62	8.185	2349	2362	2377	rBV	79626	182937	16.79%	2.067%
63	8.313	2393	2402	2424	rVB	322584	538011	49.39%	6.080%
64	8.503	2458	2461	2462	rBV2	480	298	0.03%	0.003%
65	8.644	2503	2505	2506	rBV	263	93	0.01%	0.001%
66	8.754	2534	2539	2544	rBV2	360	553	0.05%	0.006%
67	8.805	2552	2555	2558	rBV2	330	265	0.02%	0.003%
68	9.091	2631	2644	2677	rBV	484894	816179	74.93%	9.223%
69	9.230	2684	2687	2691	rVB3	438	356	0.03%	0.004%
70	9.265	2696	2698	2699	rBV	371	138	0.01%	0.002%
71	9.368	2728	2730	2731	rBV	187	61	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080918\
 Data File : VU026021.D
 Acq On : 10 Aug 2018 01:42
 Operator : MD/SY
 Sample : J4401-05 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZE3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Title : VOC Analysis

72	9.381	2731	2734	2740	rVV3	353	361	0.03%	0.004%
73	9.432	2748	2750	2751	rBV	314	156	0.01%	0.002%
74	9.593	2799	2800	2801	rBV	247	87	0.01%	0.001%
75	9.718	2836	2839	2848	rVB2	301	280	0.03%	0.003%
76	9.799	2862	2864	2866	rBV	217	120	0.01%	0.001%
77	9.915	2897	2900	2901	rBV	254	160	0.01%	0.002%
78	9.988	2917	2923	2928	rBV2	438	449	0.04%	0.005%
79	10.075	2948	2950	2951	rBV2	226	90	0.01%	0.001%
80	10.107	2959	2960	2962	rBV2	249	100	0.01%	0.001%
81	10.156	2973	2975	2977	rVB	195	56	0.01%	0.001%
82	10.378	3040	3044	3047	rBV2	257	216	0.02%	0.002%
83	10.435	3049	3062	3079	rVV	359816	576635	52.94%	6.516%
84	10.612	3106	3117	3131	rBV2	25779	46048	4.23%	0.520%
85	10.702	3142	3145	3152	rBV3	388	462	0.04%	0.005%
86	10.783	3164	3170	3172	rBV3	477	434	0.04%	0.005%
87	11.487	3377	3389	3409	rBV	440646	701439	64.39%	7.926%
88	11.696	3451	3454	3457	rBV2	568	348	0.03%	0.004%
89	11.863	3493	3506	3523	rBV	477727	766912	70.40%	8.666%
90	12.484	3694	3699	3709	rVB2	4849	6607	0.61%	0.075%
91	13.509	4011	4018	4030	rBV6	5578	9868	0.91%	0.112%


Sum of corrected areas: 8849388

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080918\
Data File : VU026021.D
Acq On : 10 Aug 2018 01:42
Operator : MD/SY
Sample : J4401-05 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZE3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

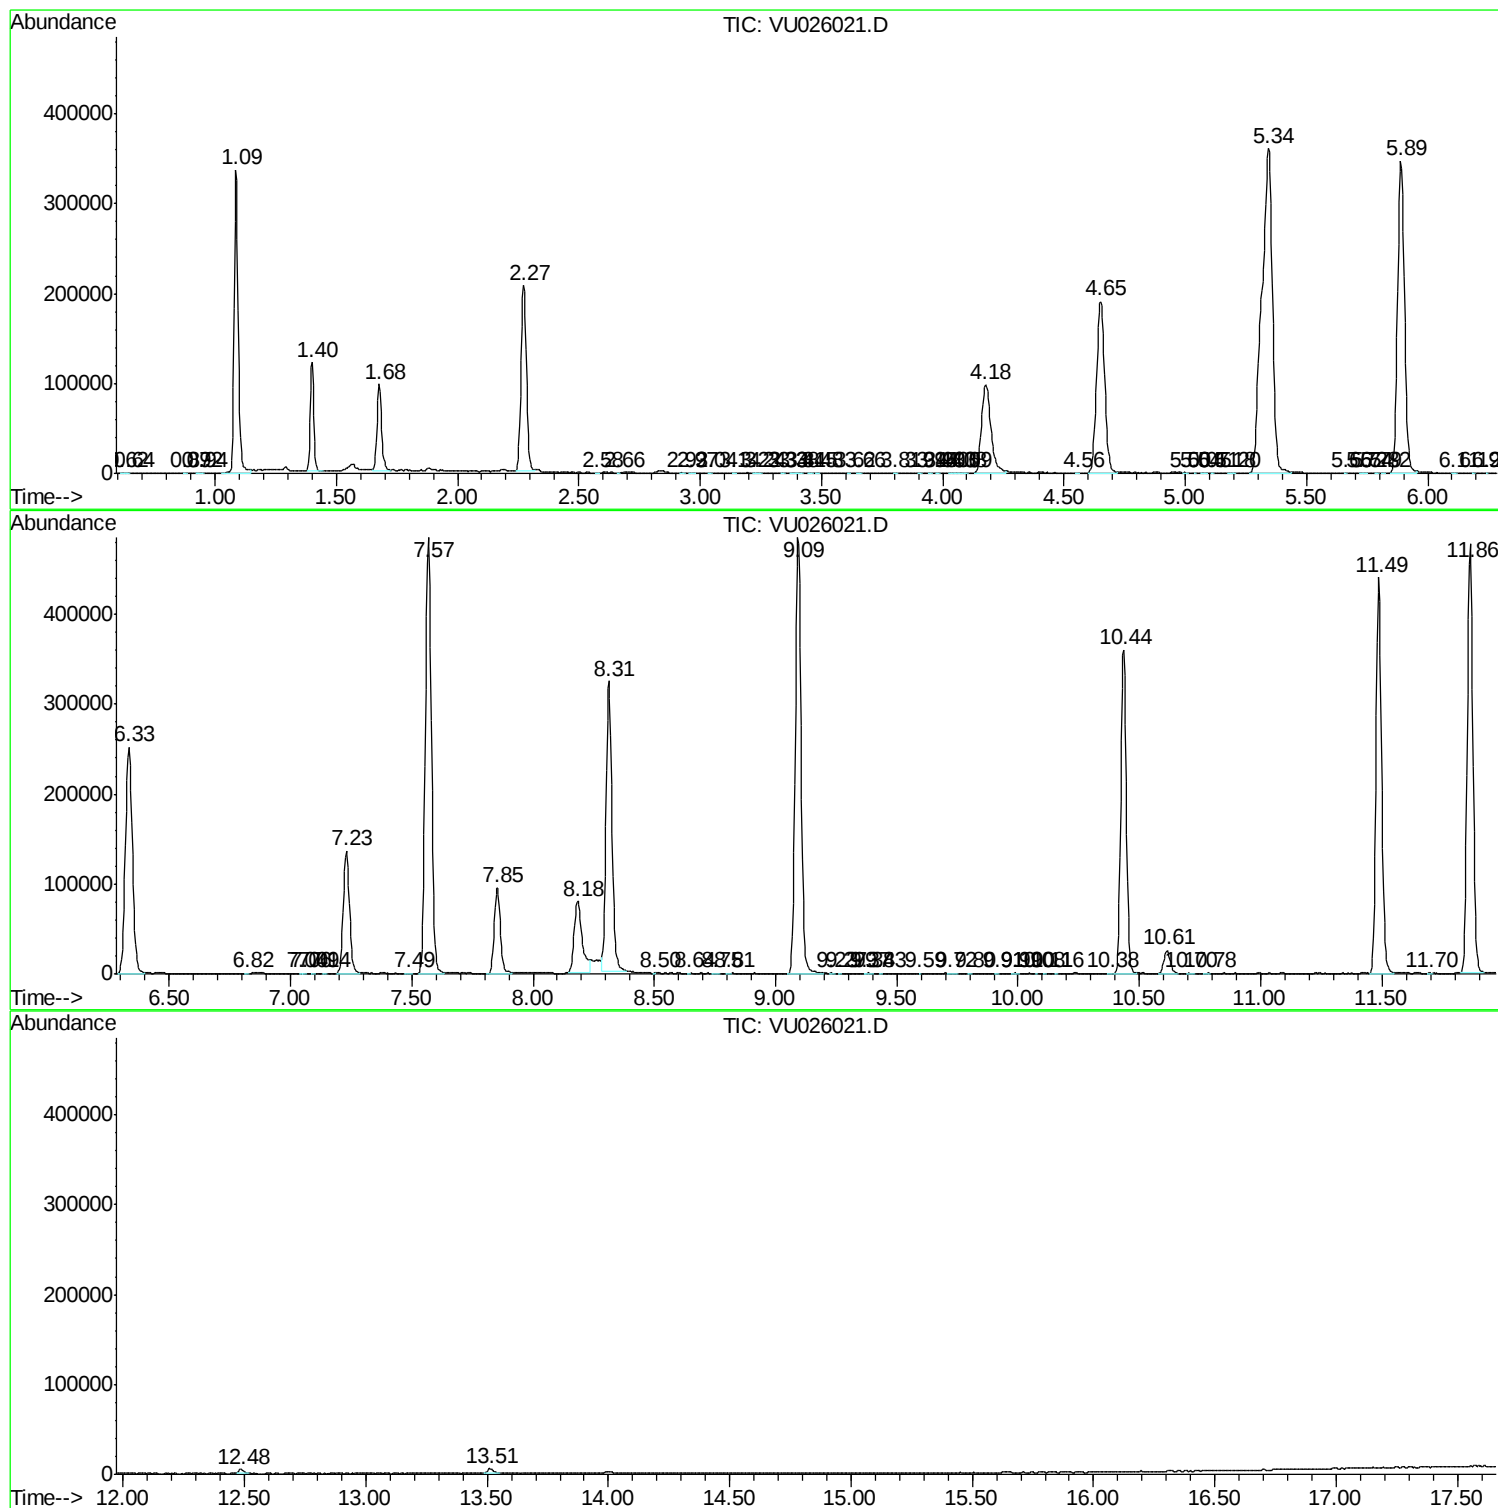

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080918\
Data File : VU026021.D
Acq On : 10 Aug 2018 01:42
Operator : MD/SY
Sample : J4401-05 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZE3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU080918\
Data File : VU026021.D
Acq On : 10 Aug 2018 01:42
Operator : MD/SY
Sample : J4401-05 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZE3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc