


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080918\
Data File : VU025977.D
Acq On : 08 Aug 2018 18:28
Operator : MD/SY
Sample : BFB42
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB42

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Title : VOC Analysis
Last Update : Fri Aug 10 07:39:13 2018

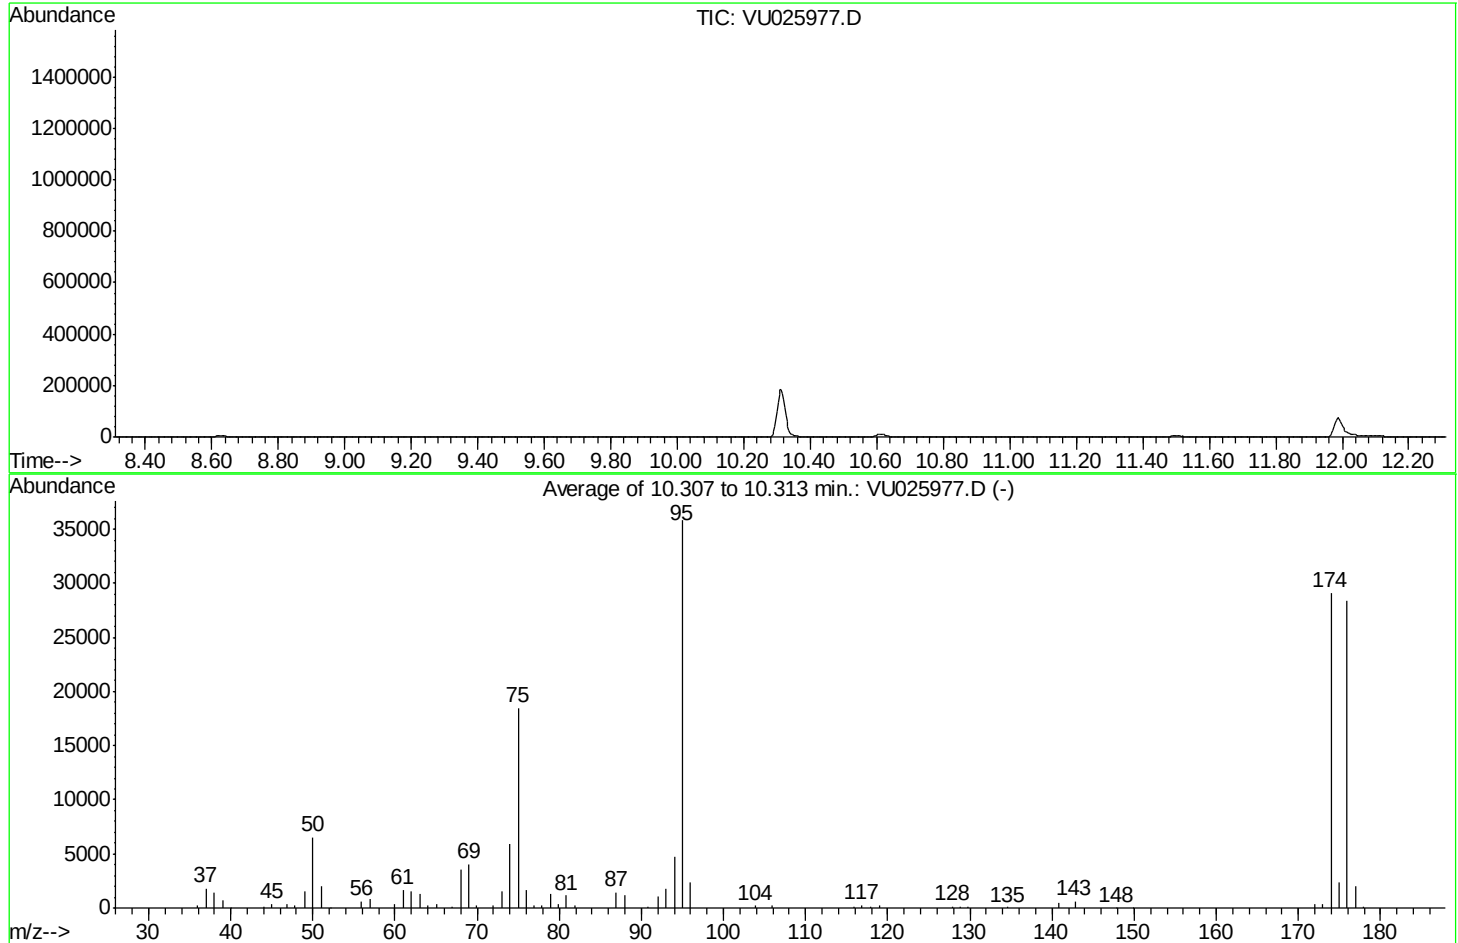

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	6536	PASS
75	95	30	80	51.6	18469	PASS
95	95	100	100	100.0	35821	PASS
96	95	5	9	6.6	2363	PASS
173	174	0.00	2	1.1	312	PASS
174	95	50	120	81.4	29157	PASS
175	174	5	9	8.0	2337	PASS
176	174	95	101	97.5	28429	PASS
177	176	5	9	7.3	2066	PASS

Scan 3011 (10.271 min): VU025977.D
BFB42

m/z	Abundance
39.90	161.0
44.00	462.0
206.90	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	334.0
37.00	1787.0
38.00	1377.0
39.00	724.0
39.90	219.0
44.00	598.0
45.00	409.0
46.80	334.0
47.80	259.0
49.00	1389.0
50.00	6004.0
51.00	1922.0
55.90	610.0
57.00	824.0
60.00	380.0
61.00	1588.0
62.00	1400.0
63.00	1290.0
64.10	286.0
65.00	290.0
66.90	142.0
68.00	3514.0
69.00	3593.0
69.90	303.0
72.00	202.0
73.00	1349.0
74.00	5431.0
75.00	17248.0
76.00	1549.0
76.90	334.0
77.90	198.0
78.90	1258.0
80.00	378.0
80.80	1165.0
81.90	304.0
87.00	1332.0
88.00	913.0
92.00	1015.0
93.00	1670.0
94.00	4465.0
95.00	33568.0
96.00	2207.0
103.90	169.0
105.90	174.0
115.90	135.0
116.80	232.0
117.80	155.0
118.90	156.0
128.00	189.0
128.80	106.0
129.70	161.0
134.60	130.0
140.80	412.0
142.80	579.0
172.00	330.0
172.90	326.0
174.00	26288.0
175.00	2212.0
175.90	25960.0
177.00	1924.0
177.90	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	279.0
37.00	1927.0
38.00	1459.0
39.00	775.0
39.90	218.0
44.00	614.0
45.00	427.0
46.90	382.0
47.70	304.0
49.00	1574.0
50.00	6711.0
51.10	1990.0
56.00	650.0
57.00	849.0
60.00	401.0
61.00	1727.0
62.00	1566.0
63.00	1408.0
64.00	318.0
65.00	349.0
66.90	134.0
68.00	3591.0
69.00	4166.0
69.90	270.0
72.00	232.0
73.00	1565.0
74.00	6064.0
75.00	19136.0
76.00	1777.0
76.90	267.0
77.90	219.0
78.90	1329.0
80.00	348.0
80.80	1237.0
81.80	282.0
86.90	1460.0
88.00	1197.0
90.80	140.0
92.00	1040.0
93.00	1893.0
94.00	4967.0
95.00	37096.0
96.00	2425.0
103.90	206.0
105.80	213.0
115.80	145.0
116.90	255.0
117.80	163.0
119.00	186.0
128.00	153.0
128.80	100.0
129.70	157.0
134.70	131.0
140.80	488.0
142.80	650.0
149.80	102.0
172.00	388.0
172.90	299.0
174.00	29840.0
174.90	2432.0
175.90	29032.0
177.00	2126.0
177.90	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	235.0
37.00	1768.0
38.00	1439.0
39.00	717.0
39.90	213.0
44.00	667.0
45.00	405.0
46.90	395.0
47.70	283.0
49.00	1533.0
50.00	6894.0
51.00	2008.0
52.10	104.0
56.00	646.0
57.00	908.0
60.00	343.0
61.00	1731.0
62.00	1612.0
63.00	1380.0
64.00	272.0
65.00	401.0
66.90	137.0
68.00	3547.0
69.00	4339.0
70.00	239.0
72.00	229.0
73.00	1586.0
74.00	6260.0
75.00	19024.0
76.00	1820.0
76.90	183.0
77.90	155.0
78.90	1297.0
79.90	330.0
80.90	1142.0
81.80	275.0
86.90	1508.0
88.00	1382.0
90.80	181.0
92.00	1000.0
93.00	1849.0
94.00	4638.0
95.00	36800.0
96.00	2458.0
103.90	247.0
105.80	228.0
115.80	137.0
116.90	284.0
117.90	130.0
119.00	228.0
127.90	116.0
129.70	121.0
140.80	474.0
142.90	631.0
147.90	115.0
172.00	423.0
172.90	311.0
174.00	31344.0
174.90	2369.0
176.00	30296.0
176.90	2150.0
207.00	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42