


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080918\
Data File : VU025984.D
Acq On : 09 Aug 2018 09:15
Operator : MD/SY
Sample : BFB43
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB43

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Title : VOC Analysis
Last Update : Fri Aug 10 07:39:13 2018

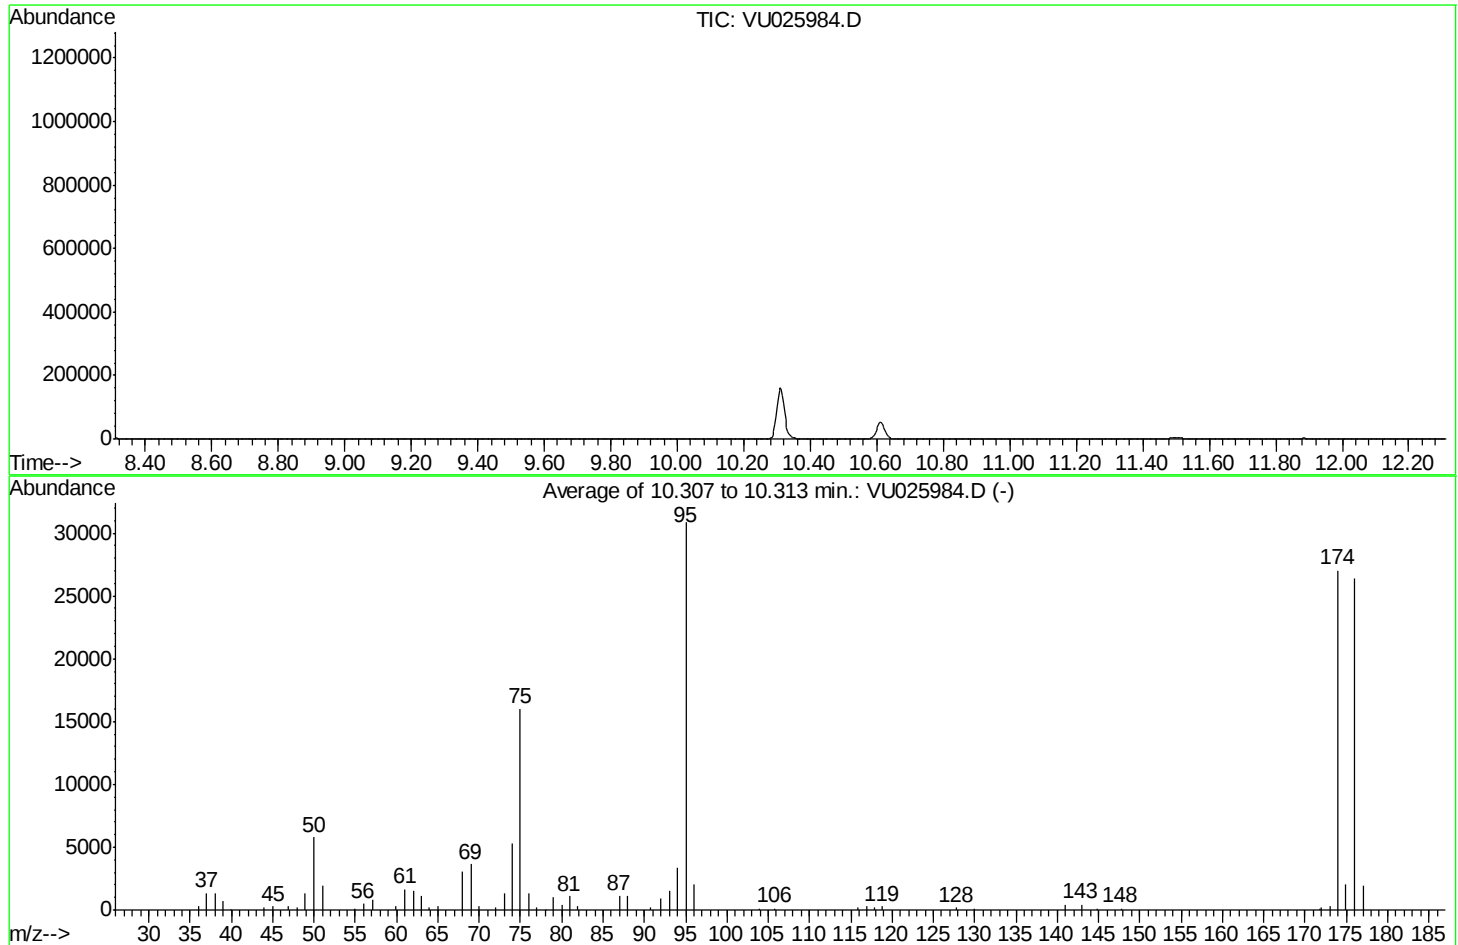

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	5780	PASS
75	95	30	80	52.0	16045	PASS
95	95	100	100	100.0	30856	PASS
96	95	5	9	6.6	2025	PASS
173	174	0.00	2	1.1	298	PASS
174	95	50	120	87.6	27037	PASS
175	174	5	9	7.4	1994	PASS
176	174	95	101	97.4	26344	PASS
177	176	5	9	7.4	1947	PASS

Scan 3011 (10.271 min): VU025984.D
BFB43

m/z	Abundance
39.90	206.0
44.00	300.0
207.10	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
35.90	364.0
37.00	1455.0
38.00	1300.0
39.00	705.0
39.80	185.0
44.00	479.0
45.10	282.0
46.90	379.0
47.90	179.0
48.90	1280.0
50.00	5849.0
51.00	1878.0
55.00	117.0
56.00	529.0
57.10	884.0
59.90	336.0
61.00	1540.0
62.00	1514.0
63.00	1139.0
63.90	182.0
65.00	223.0
68.00	3071.0
69.00	3349.0
70.00	239.0
72.10	181.0
73.00	1473.0
74.10	5230.0
75.00	15462.0
76.00	1432.0
76.90	157.0
78.10	116.0
78.90	990.0
80.00	353.0
80.90	1003.0
81.90	271.0
87.00	1178.0
88.00	1134.0
90.80	183.0
92.00	859.0
93.00	1521.0
94.00	3318.0
95.00	30592.0
96.00	2108.0
103.90	124.0
105.80	161.0
115.80	156.0
116.90	260.0
117.90	213.0
118.90	301.0
127.90	136.0
129.90	135.0
140.90	321.0
142.90	396.0
144.90	106.0
147.70	110.0
171.80	299.0
174.00	25424.0
174.90	1927.0
176.00	25168.0
177.00	1926.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
35.90	361.0
37.00	1399.0
38.00	1361.0
39.00	706.0
39.90	224.0
43.90	485.0
45.10	306.0
46.90	304.0
47.90	182.0
49.00	1414.0
50.00	5902.0
51.00	2026.0
55.00	100.0
56.00	512.0
57.10	898.0
59.90	338.0
61.00	1702.0
62.00	1544.0
63.00	1143.0
63.90	226.0
65.00	277.0
68.00	3166.0
69.00	3799.0
70.00	291.0
71.90	157.0
73.00	1388.0
74.00	5410.0
75.00	16512.0
76.00	1380.0
76.90	212.0
78.90	1032.0
80.00	382.0
80.90	1113.0
81.90	315.0
87.00	1189.0
88.00	1085.0
90.80	167.0
92.00	908.0
93.00	1641.0
94.00	3417.0
95.00	31792.0
96.00	2064.0
103.90	153.0
105.80	138.0
115.80	177.0
116.90	295.0
117.90	253.0
118.80	278.0
127.80	187.0
129.90	137.0
140.90	363.0
142.90	431.0
144.80	129.0
147.70	132.0
172.00	335.0
173.00	447.0
174.00	27912.0
174.90	2048.0
176.00	27264.0
177.00	2007.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	343.0
37.00	1260.0
38.00	1300.0
39.00	636.0
39.90	216.0
43.90	479.0
45.00	311.0
46.90	282.0
48.00	166.0
49.00	1361.0
50.00	5589.0
51.00	1989.0
56.00	467.0
57.10	794.0
59.90	278.0
61.00	1698.0
62.00	1414.0
63.00	1082.0
63.90	189.0
65.00	326.0
68.00	3044.0
69.00	3754.0
70.00	296.0
71.90	135.0
73.00	1226.0
74.00	5249.0
75.00	16162.0
76.00	1192.0
77.00	271.0
78.90	1053.0
80.00	364.0
80.90	1182.0
81.90	356.0
87.00	1134.0
87.90	1022.0
90.80	128.0
92.00	1004.0
93.00	1516.0
94.00	3234.0
95.00	30184.0
96.00	1905.0
104.00	164.0
105.90	146.0
115.80	149.0
116.90	261.0
117.90	221.0
118.80	252.0
127.80	197.0
130.00	126.0
140.90	411.0
142.90	485.0
144.80	135.0
147.80	139.0
172.00	360.0
173.00	449.0
174.00	27776.0
174.90	2008.0
176.00	26600.0
177.00	1910.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43