

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU080919\
 Data File : VU033704.D
 Acq On : 09 Aug 2019 23:39
 Operator : JC/SP
 Sample : K4202-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2B43

Quant Time: Aug 12 03:16:15 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080919WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 10 04:26:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	351605	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	341679	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	169930	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	129846	50.17	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	100.34%
7) Chloroethane-d5	1.67	69	116211	44.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.60%
11) 1,1-Dichloroethene-d2	2.26	63	174365	40.07	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.14%
21) 2-Butanone-d5	4.15	46	249429	155.45	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	155.45%#
24) Chloroform-d	4.62	84	246088	64.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	128.00%#
26) 1,2-Dichloroethane-d4	5.29	65	165382	68.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	137.56%#
32) Benzene-d6	5.32	84	502828	62.36	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	124.72%
36) 1,2-Dichloropropane-d6	6.31	67	166126	67.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	134.26%#
41) Toluene-d8	7.55	98	447844	59.05	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	118.10%
43) trans-1,3-Dichloropropene-	7.83	79	77104	61.70	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	123.40%
47) 2-Hexanone-d5	8.29	63	188719	147.24	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	147.24%#
57) 1,1,2,2-Tetrachloroethane-	10.41	84	253634	69.29	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	138.58%#
64) 1,2-Dichlorobenzene-d4	11.84	152	193993	67.83	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	135.66%#


Target Compounds					Qvalue
13) Acetone	2.31	43	5901	3.658 ug/L	97
20) cis-1,2-Dichloroethene	4.20	96	2683	1.061 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080919\
Data File : VU033704.D
Acq On : 09 Aug 2019 23:39
Operator : JC/SP
Sample : K4202-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B43

Quant Time: Aug 12 03:16:15 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080919WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 10 04:26:55 2019
Response via : Initial Calibration

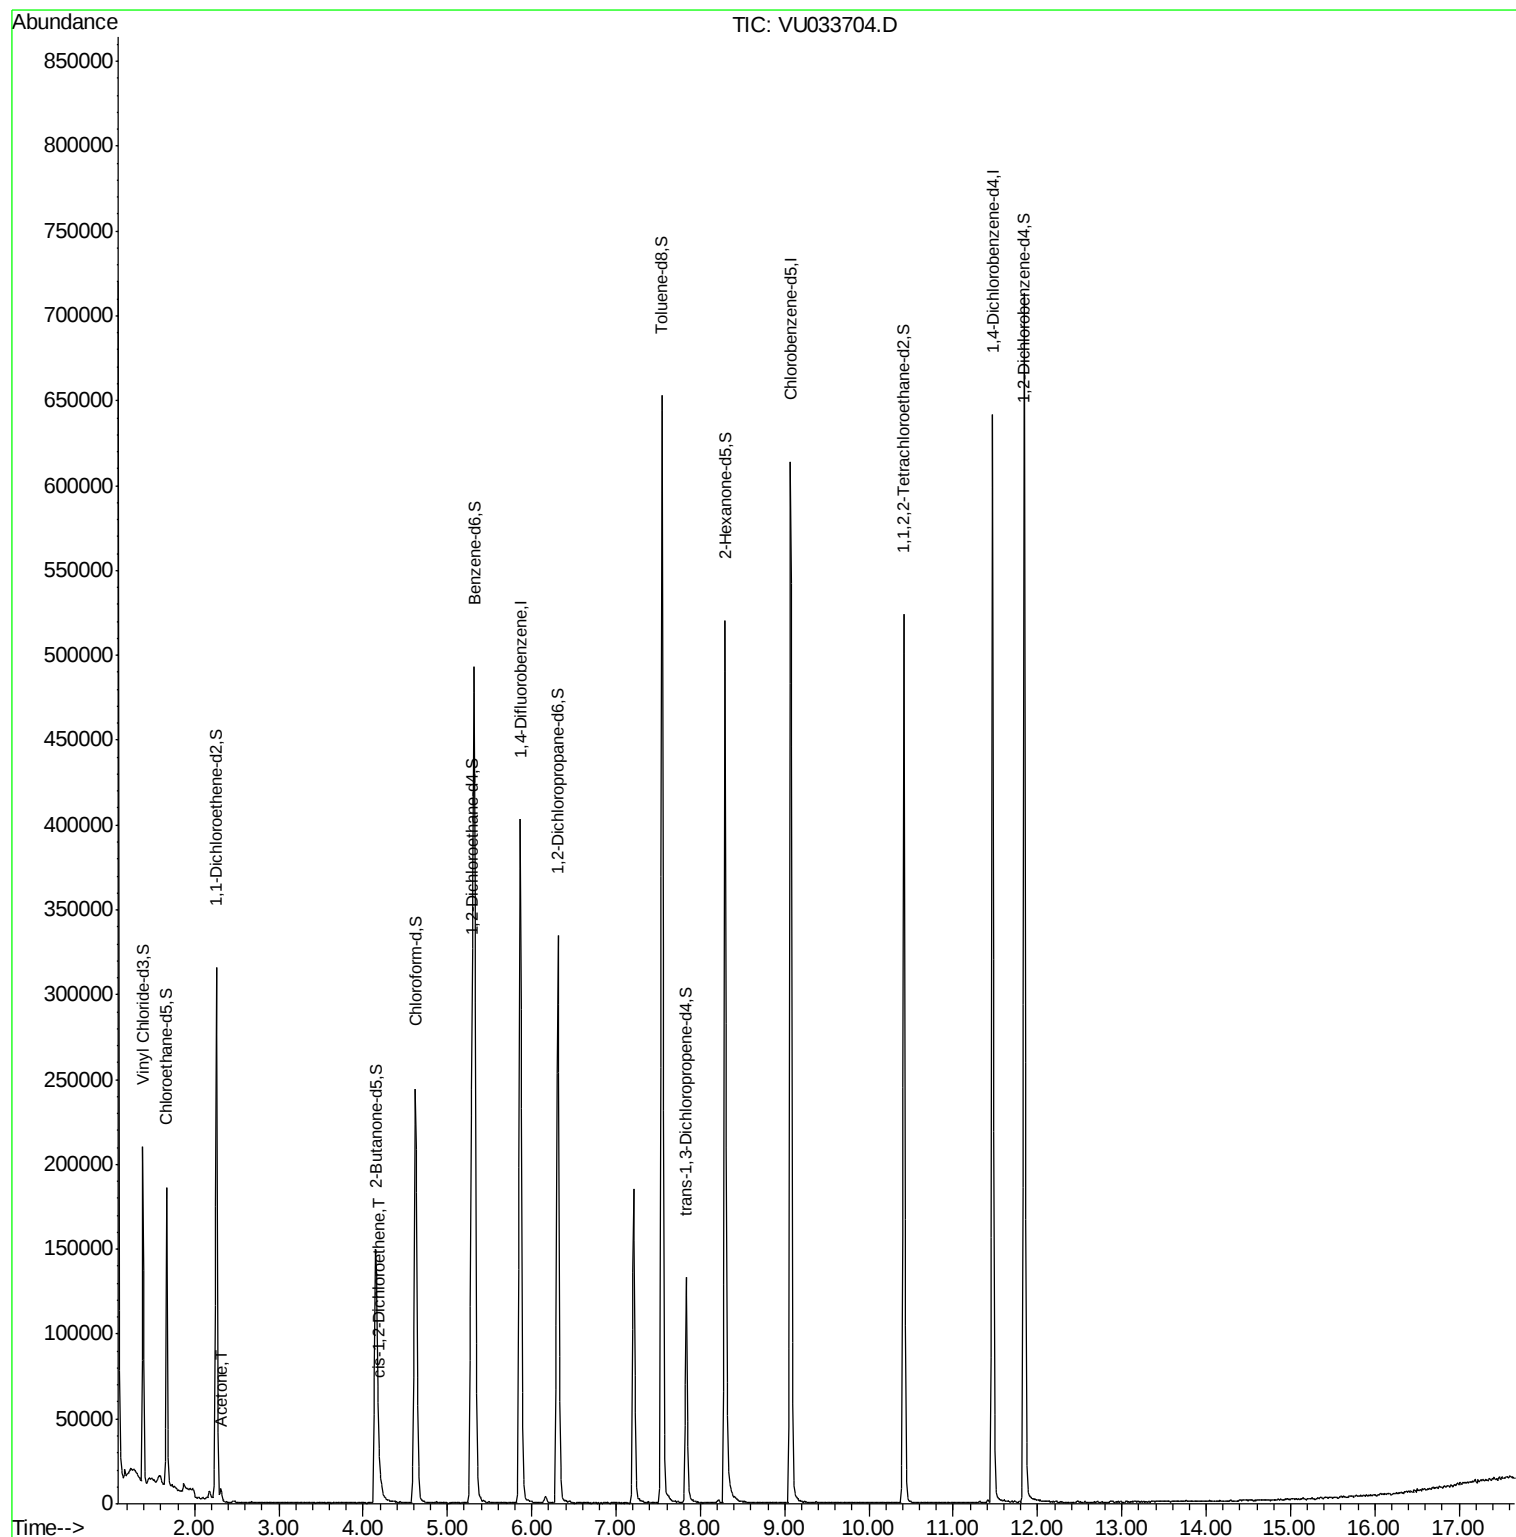

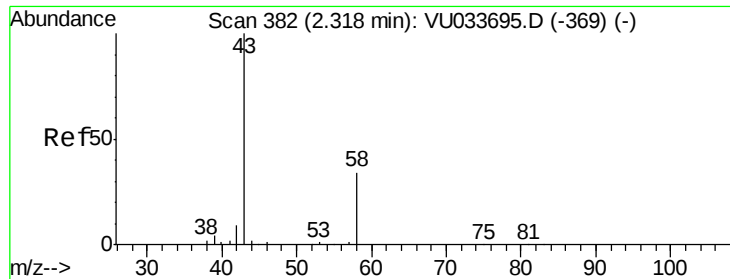

#13

Acetone

Concen: 3.658 ug/L

RT: 2.31 min Scan# 380

Delta R.T. -0.01 min

Lab File: VU033704.D

Acq: 09 Aug 2019 23:39

Instrument :

MSVOA_U

ClientSampleId :


F2B43

Tgt Ion: 43 Resp: 5901

Ion Ratio Lower Upper




43 100

58 31.4 0.0 65.6

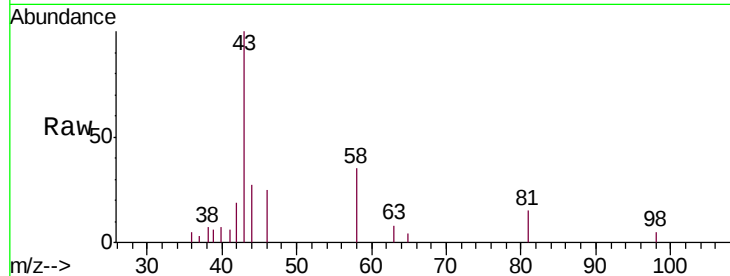

Abundance Ion 43.00 (42.70 to 43.70): VU033704.D (-289) (-)

Ion 58.00 (57.70 to 58.70): VU033704.D (-289) (-)

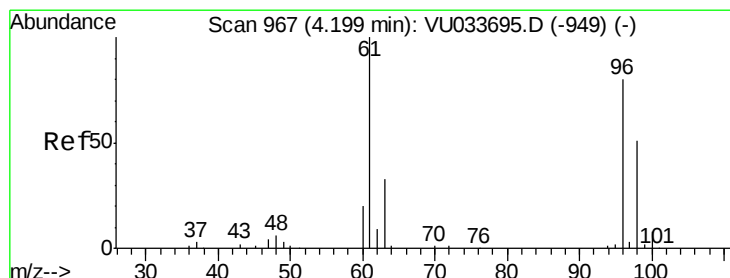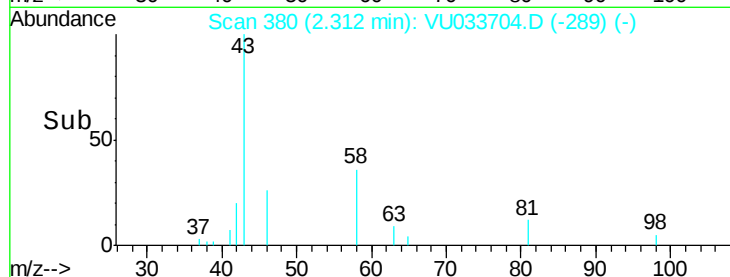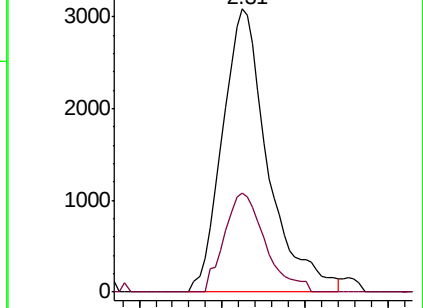

#20

cis-1,2-Dichloroethene

Concen: 1.061 ug/L

RT: 4.20 min Scan# 966

Delta R.T. -0.00 min

Lab File: VU033704.D

Acq: 09 Aug 2019 23:39


Tgt Ion: 96 Resp: 2683

Ion Ratio Lower Upper

96 100

61 108.2 87.0 161.6

68 0.0 0.0 0.0

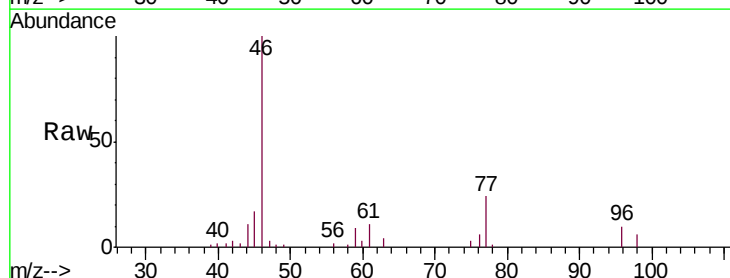

Abundance Ion 96.00 (95.70 to 96.70): VU033704.D (-874) (-)

Ion 61.00 (60.70 to 61.70): VU033704.D (-874) (-)

Ion 68.00 (67.70 to 68.70): VU033704.D (-874) (-)

