

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU080919\
 Data File : VU033713.D
 Acq On : 10 Aug 2019 03:08
 Operator : JC/SP
 Sample : K4289-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F2B20

Quant Time: Aug 12 03:33:53 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080919WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 10 04:26:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	335521	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	326795	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	158847	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	115411	46.73	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.46%
7) Chloroethane-d5	1.67	69	117679	47.54	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.08%
11) 1,1-Dichloroethene-d2	2.26	63	161010	38.77	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.54%
21) 2-Butanone-d5	4.16	46	238182	155.56	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	155.56%#
24) Chloroform-d	4.62	84	228540	62.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	124.56%
26) 1,2-Dichloroethane-d4	5.29	65	152733	66.57	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	133.14%#
32) Benzene-d6	5.32	84	461845	59.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	119.76%
36) 1,2-Dichloropropane-d6	6.31	67	152934	64.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	129.24%#
41) Toluene-d8	7.55	98	406433	56.03	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.06%
43) trans-1,3-Dichloropropene-	7.83	79	70798	59.24	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	118.48%
47) 2-Hexanone-d5	8.30	63	179625	146.52	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	146.52%#
57) 1,1,2,2-Tetrachloroethane-	10.41	84	238345	68.08	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	136.16%#
64) 1,2-Dichlorobenzene-d4	11.84	152	174879	65.41	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	130.82%#


Target Compounds					Qvalue
20) cis-1,2-Dichloroethene	4.20	96	7203	2.986 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080919\
Data File : VU033713.D
Acq On : 10 Aug 2019 03:08
Operator : JC/SP
Sample : K4289-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F2B20

Quant Time: Aug 12 03:33:53 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080919WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 10 04:26:55 2019
Response via : Initial Calibration

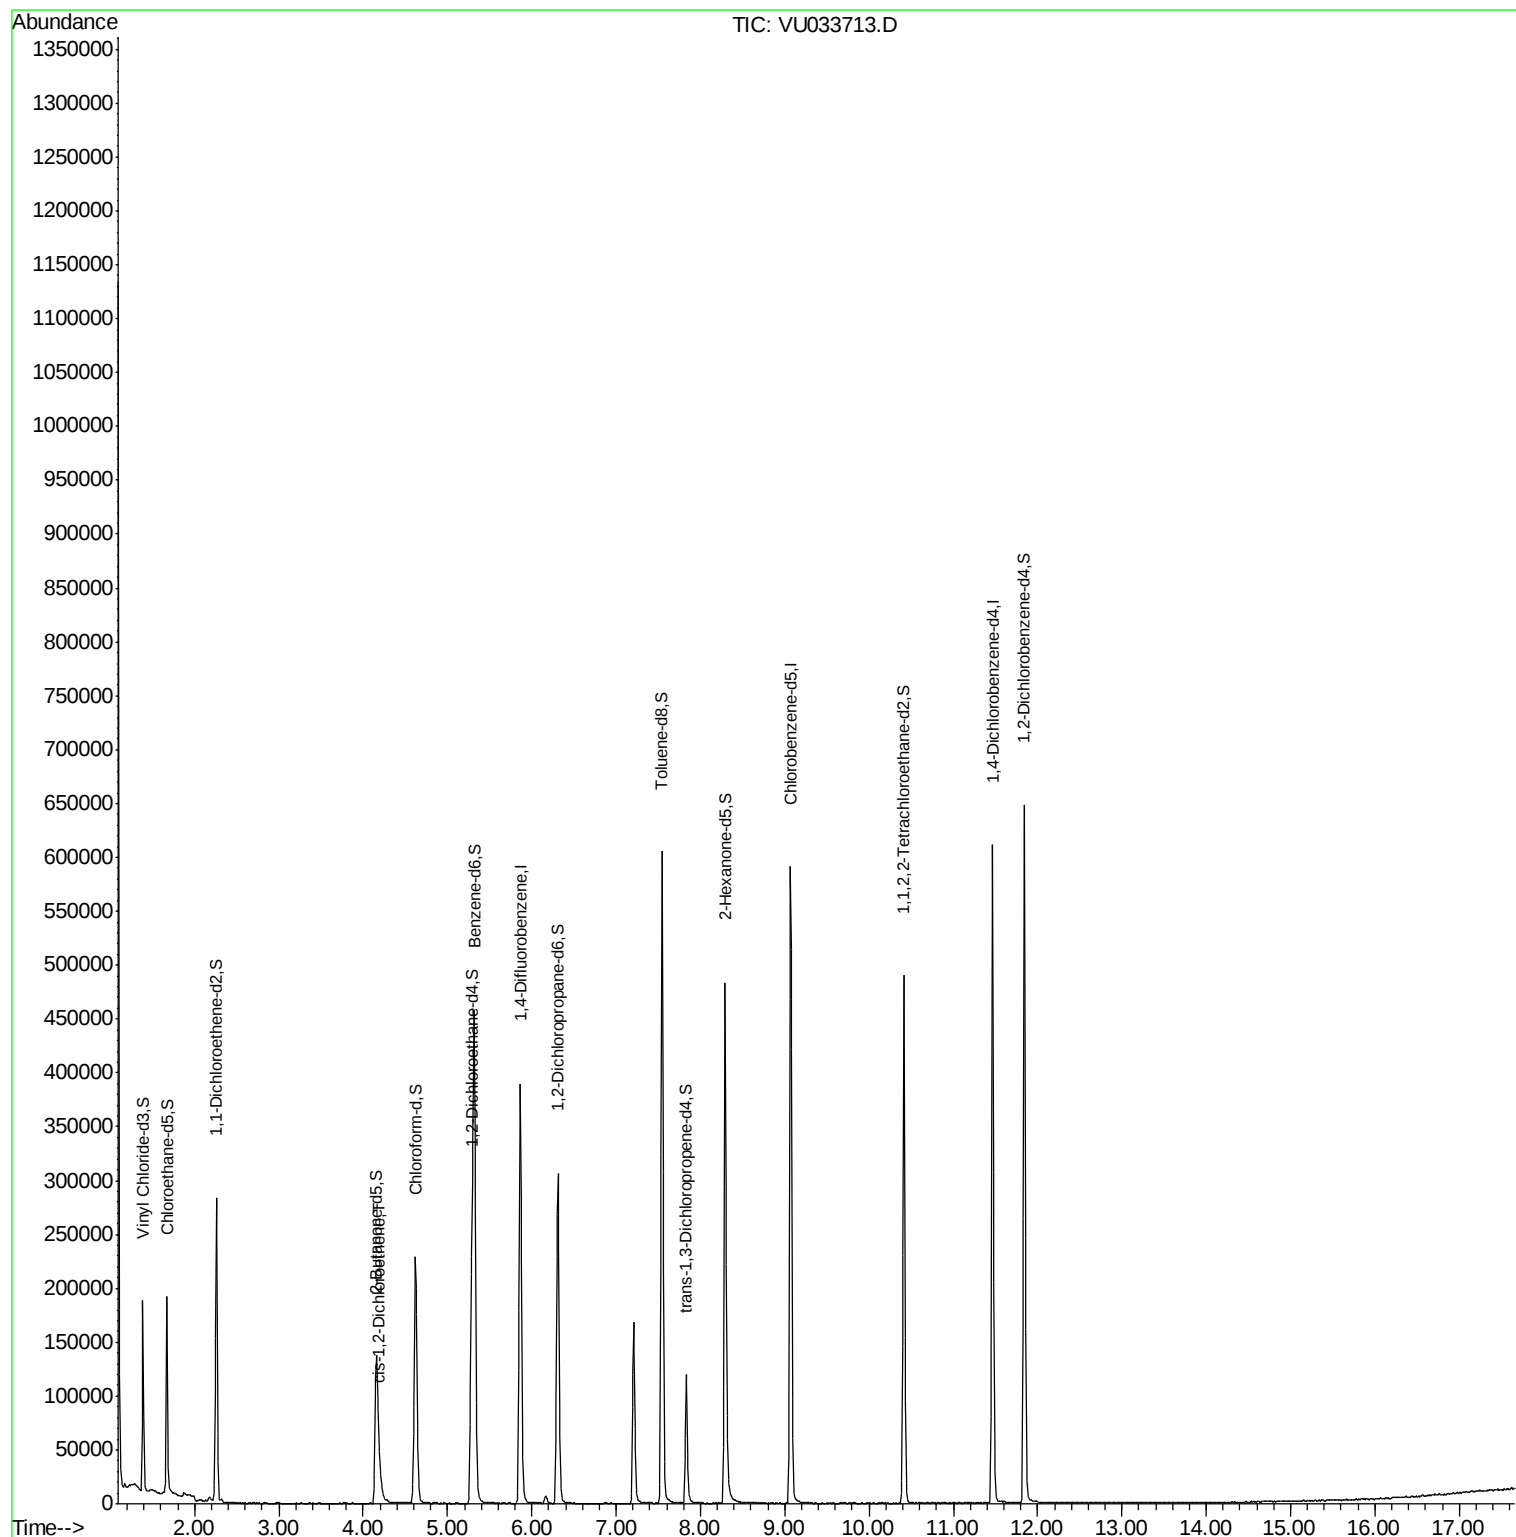

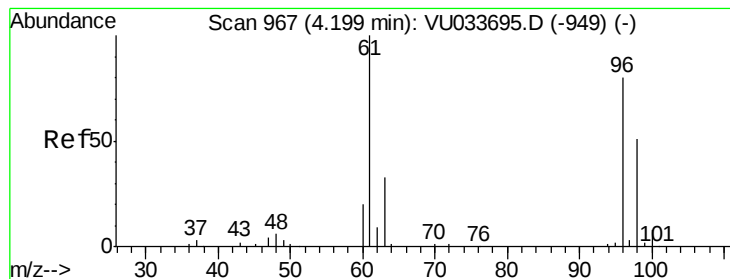

#20

cis-1,2-Dichloroethene
 Concen: 2.986 ug/L
 RT: 4.20 min Scan# 967
 Delta R.T. 0.00 min
 Lab File: VU033713.D
 Acq: 10 Aug 2019 03:08

Instrument :
 MSVOA_U
 ClientSampleId :
 F2B20

Tgt Ion: 96 Resp: 7203
 Ion Ratio Lower Upper
 96 100
 61 129.9 87.0 161.6
 68 0.0 0.0 0.0

